

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV012825\  
 Data File : VV038555.D  
 Acq On : 28 Jan 2025 11:57  
 Operator : SY/MD  
 Sample : VV0128WBL02  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :

Quant Time: Jan 29 09:24:49 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVSIM012725.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Tue Jan 28 08:06:10 2025  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc     | Units | Dev(Min)  |
|-------------------------------|----------------|------|------------|----------|-------|-----------|
| -----                         |                |      |            |          |       |           |
| Internal Standards            |                |      |            |          |       |           |
| 1) 1,4-Difluorobenzene        | 5.566          | 114  | 5565       | 0.500    | ug/L  | 0.00      |
| 5) Chlorobenzene-d5           | 8.800          | 117  | 5542       | 0.500    | ug/L  | 0.00      |
| 11) 1,4-Dichlorobenzene-d4    | 11.191         | 152  | 2603       | 0.500    | ug/L  | 0.00      |
| System Monitoring Compounds   |                |      |            |          |       |           |
| 2) Vinyl Chloride-d3          | 1.273          | 65   | 2573       | 0.458    | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 40 - 130 |      | Recovery = | 92.000%  |       |           |
| 4) 1,2-Dichloroethane-d4      | 4.969          | 65   | 2219       | 0.495    | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 70 - 130 |      | Recovery = | 100.000% |       |           |
| 7) 1,2-Dichloropropane-d6     | 5.995          | 67   | 2623       | 0.482    | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 60 - 140 |      | Recovery = | 96.000%  |       |           |
| 8) Toluene-d8                 | 7.253          | 98   | 4896       | 0.448    | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 70 - 130 |      | Recovery = | 90.000%  |       |           |
| 10) 1,1,2,2-Tetrachloroeth... | 10.146         | 84   | 2384       | 0.513    | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 65 - 120 |      | Recovery = | 102.000% |       |           |
| Target Compounds              |                |      |            |          |       |           |
| 13) 1,2-Dibromo-3-chloropr... | 12.168         | 75   | 15         | 0.032    | ug/L  | Qvalue 91 |
| -----                         |                |      |            |          |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV012825\  
Data File : VV038555.D  
Acq On : 28 Jan 2025 11:57  
Operator : SY/MD  
Sample : VV0128WBL02  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :


Quant Time: Jan 29 09:24:49 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVSIM012725.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Tue Jan 28 08:06:10 2025  
Response via : Initial Calibration

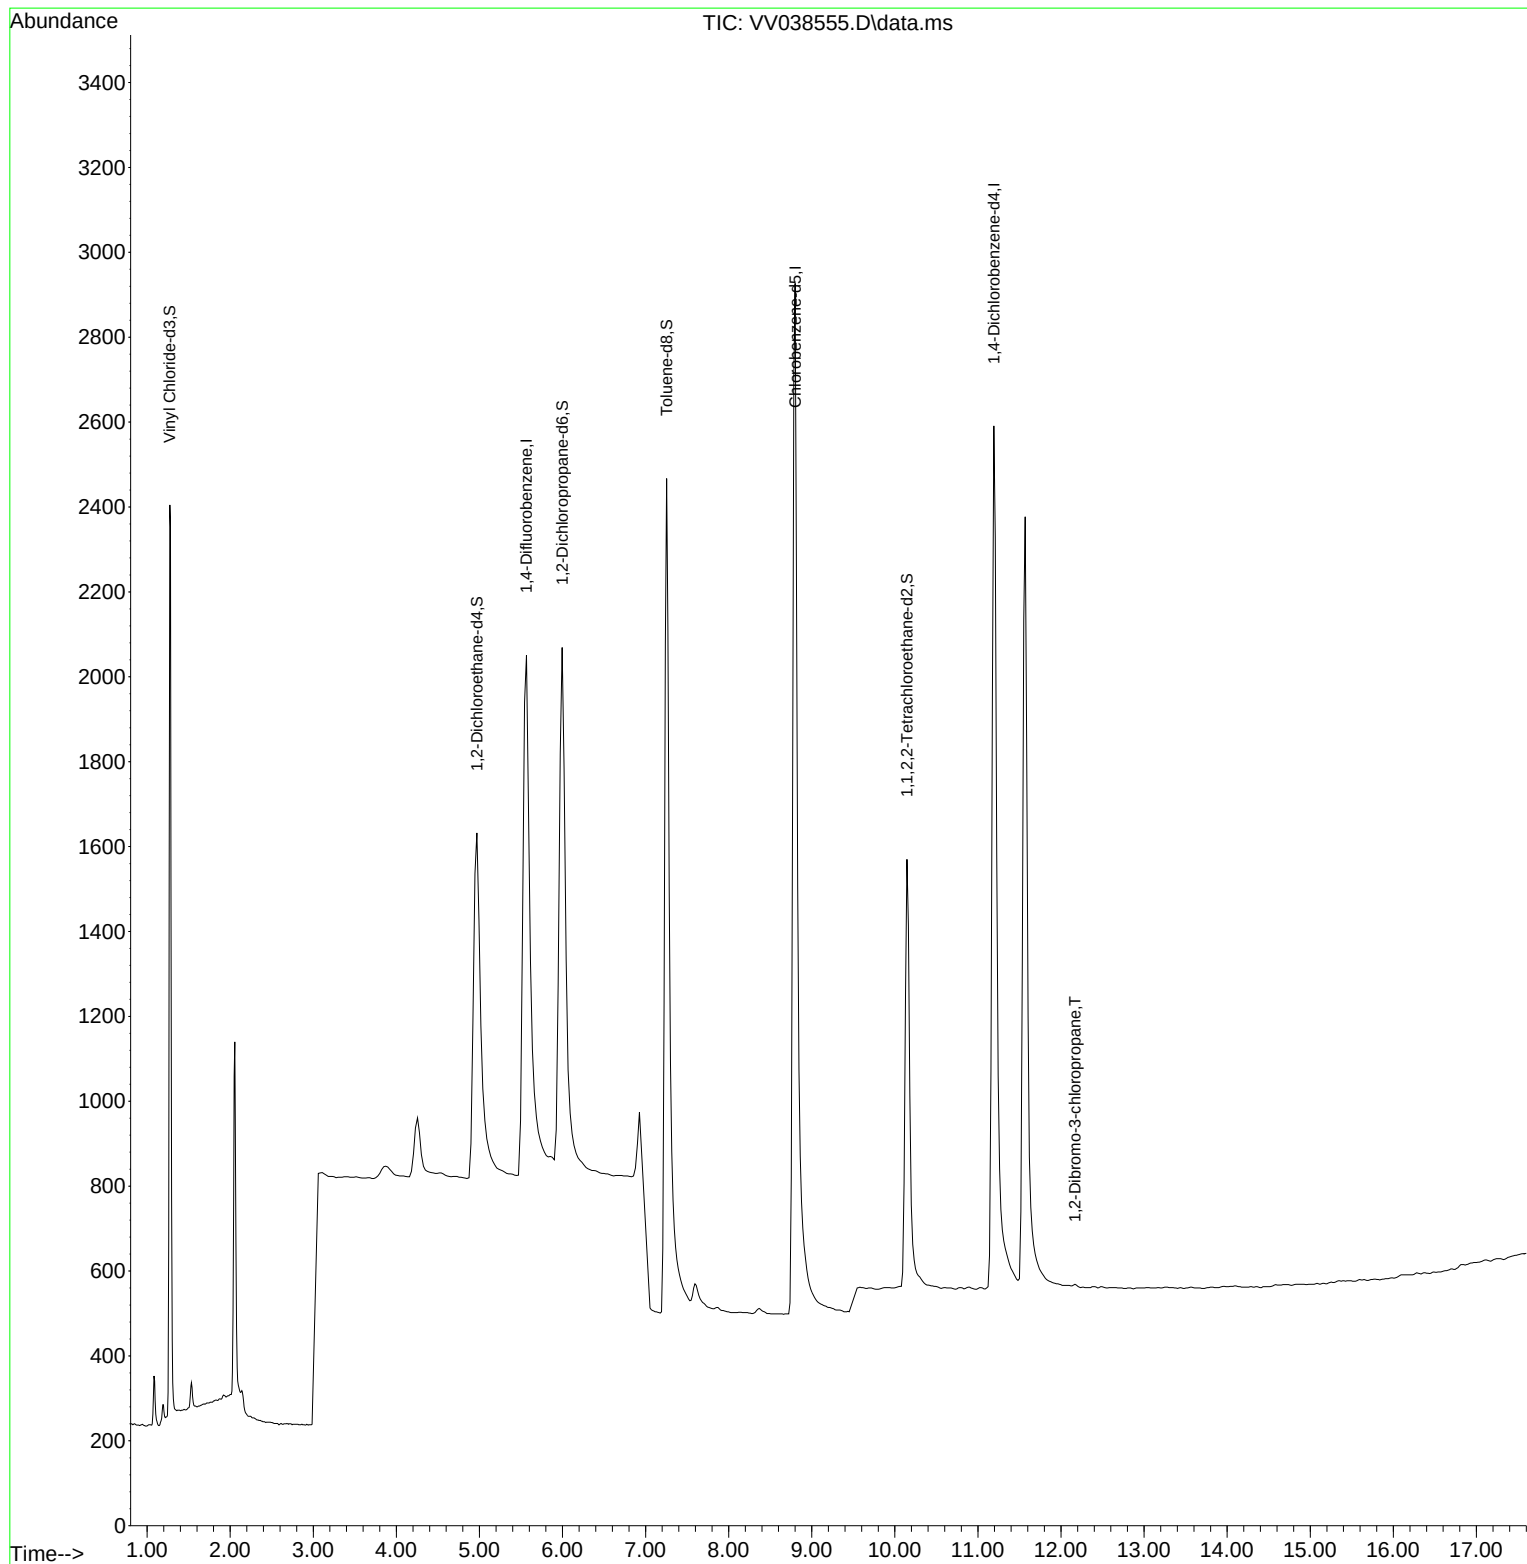

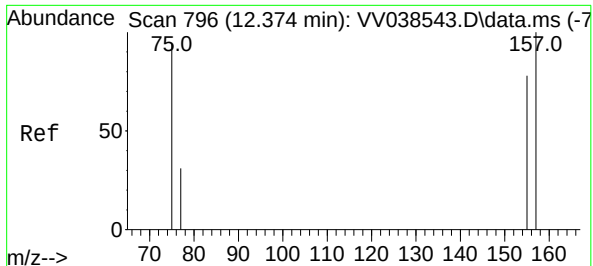

#13  
 1,2-Dibromo-3-chloropropane  
 Concen: 0.032 ug/L  
 RT: 12.168 min Scan# 71  
 Delta R.T. -0.205 min  
 Lab File: VV038555.D  
 Acq: 28 Jan 2025 11:57

Instrument :  
 MSVOA\_V  
 ClientSampleId :

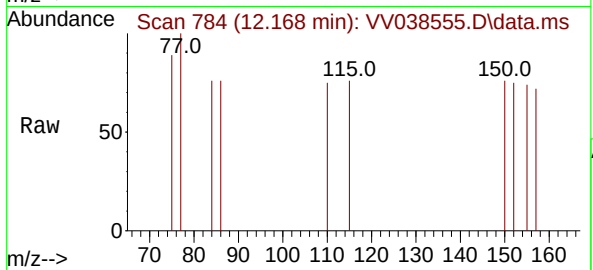

|             |       |             |
|-------------|-------|-------------|
| Tgt Ion: 75 | Resp: | 15          |
| Ion         | Ratio | Lower Upper |
| 75          | 100   |             |
| 157         | 81.3  | 77.0 115.6  |
| 155         | 82.8  | 68.2 102.2  |

