
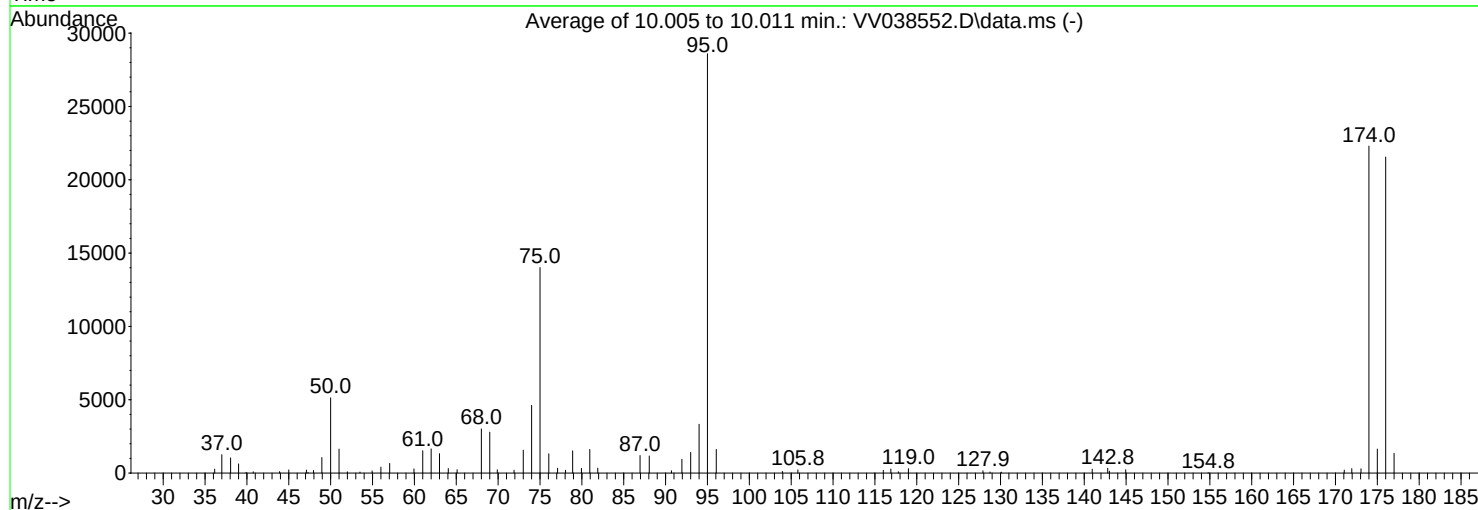


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012825\
Data File : VV038552.D
Acq On : 28 Jan 2025 10:26
Operator : SY/MD
Sample : BFB229
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB229

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jan 28 08:06:10 2025

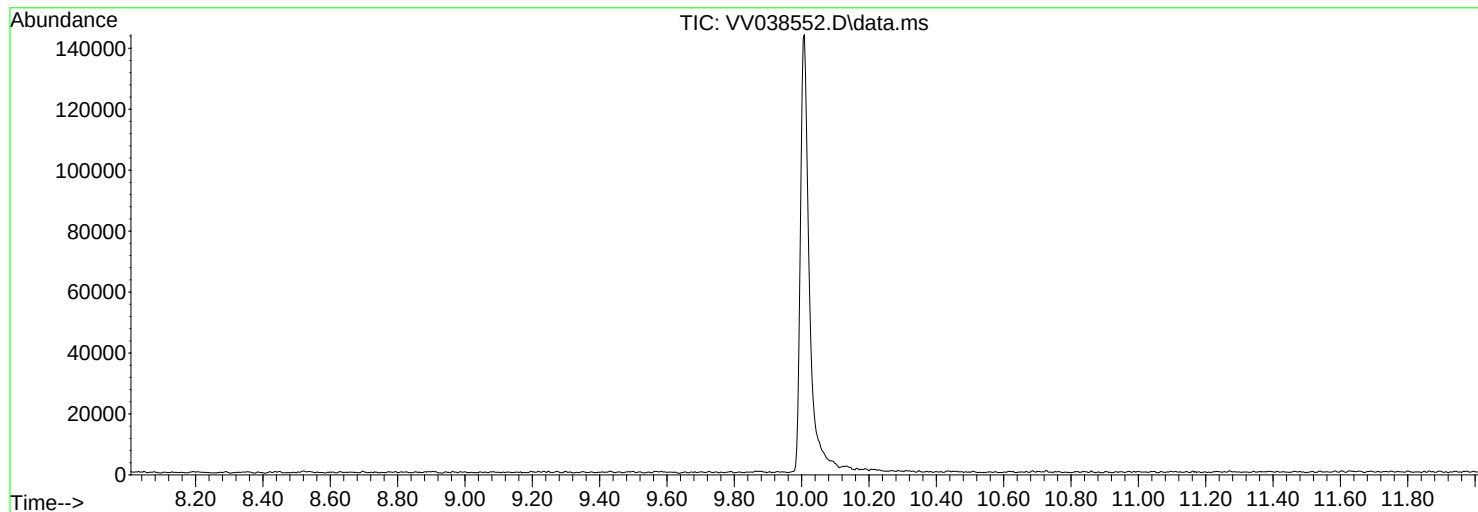

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	5128	PASS
75	95	30	80	49.0	14019	PASS
95	95	100	100	100.0	28595	PASS
96	95	5	9	5.6	1614	PASS
173	174	0.00	2	1.3	295	PASS
174	95	50	120	78.0	22299	PASS
175	174	5	9	7.4	1640	PASS
176	174	95	101	96.7	21555	PASS
177	176	5	9	6.3	1353	PASS

m/z	Abundance
39.90	405.0
43.90	460.0
46.00	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.20	272.0
37.00	1296.0
38.10	1014.0
39.00	590.0
39.90	463.0
40.70	170.0
43.90	606.0
45.00	217.0
47.10	383.0
48.00	185.0
49.00	1113.0
50.00	5265.0
51.00	1596.0
52.00	142.0
55.00	114.0
56.00	404.0
57.00	611.0
59.90	315.0
61.00	1637.0
62.00	1737.0
63.00	1351.0
64.00	373.0
65.10	237.0
68.00	3176.0
69.00	2983.0
69.90	239.0
71.90	187.0
73.00	1484.0
74.00	4663.0
75.00	14888.0
76.10	1282.0
77.10	245.0
78.00	174.0
78.90	1469.0
79.90	337.0
81.00	1638.0
81.90	357.0
87.00	1307.0
88.00	1027.0
90.70	181.0
91.90	1023.0
93.00	1459.0
94.00	3473.0
95.00	29400.0
96.00	1787.0
103.90	129.0
105.80	174.0
115.90	134.0
116.80	227.0
117.80	149.0
119.00	312.0
127.90	116.0
128.70	117.0
140.90	274.0
142.80	515.0
145.00	250.0
171.00	220.0
171.90	266.0
173.10	299.0
174.00	22616.0
175.00	1656.0
176.00	21488.0
177.00	1400.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.10	286.0
37.00	1266.0
38.10	1030.0
39.00	665.0
39.90	469.0
40.80	103.0
43.90	569.0
45.00	214.0
47.10	234.0
47.90	173.0
49.00	1073.0
50.00	5315.0
51.00	1693.0
52.00	122.0
53.50	101.0
54.90	144.0
56.00	428.0
57.00	630.0
59.90	293.0
61.00	1546.0
62.00	1702.0
63.00	1348.0
64.10	311.0
65.10	248.0
68.00	3101.0
69.00	2865.0
69.90	233.0
71.90	208.0
73.00	1615.0
74.00	4696.0
75.00	14502.0
76.00	1380.0
77.10	345.0
78.10	209.0
78.90	1559.0
79.90	341.0
80.90	1614.0
81.90	336.0
87.00	1229.0
88.10	1170.0
90.70	171.0
91.90	988.0
93.00	1446.0
94.00	3481.0
95.00	29496.0
96.00	1594.0
104.00	110.0
105.80	234.0
116.00	190.0
116.90	301.0
117.80	123.0
119.00	316.0
127.90	162.0
128.80	107.0
130.10	103.0
141.00	286.0
142.80	470.0
145.00	225.0
154.80	103.0
171.10	215.0
171.90	332.0
173.00	304.0
174.00	22928.0
175.00	1689.0
176.00	22312.0
177.00	1425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.10	257.0
37.00	1207.0
38.00	1056.0
39.00	621.0
39.90	441.0
43.90	508.0
45.00	228.0
47.30	129.0
47.90	161.0
48.90	989.0
50.00	4804.0
51.00	1623.0
53.50	116.0
54.90	198.0
56.00	397.0
57.10	740.0
60.00	252.0
61.00	1387.0
62.00	1515.0
63.00	1267.0
64.10	249.0
65.10	218.0
68.00	2767.0
69.00	2517.0
69.90	195.0
71.90	203.0
73.00	1593.0
74.00	4499.0
75.00	12667.0
76.00	1275.0
77.10	407.0
78.10	205.0
78.90	1520.0
80.00	287.0
80.90	1576.0
81.90	321.0
86.90	1064.0
88.00	1296.0
90.70	130.0
92.00	810.0
93.00	1325.0
94.00	3035.0
95.00	26888.0
96.10	1462.0
104.00	106.0
105.80	250.0
116.10	240.0
117.00	306.0
119.00	289.0
127.90	190.0
130.10	106.0
141.00	247.0
143.00	391.0
144.90	220.0
171.10	179.0
172.00	328.0
173.00	281.0
174.00	21352.0
175.00	1576.0
176.00	20864.0
177.00	1234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229