


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV012920\
 Data File : VV014423.D
 Acq On : 29 Jan 2020 14:17
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB35

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR012920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jan 31 23:09:59 2020

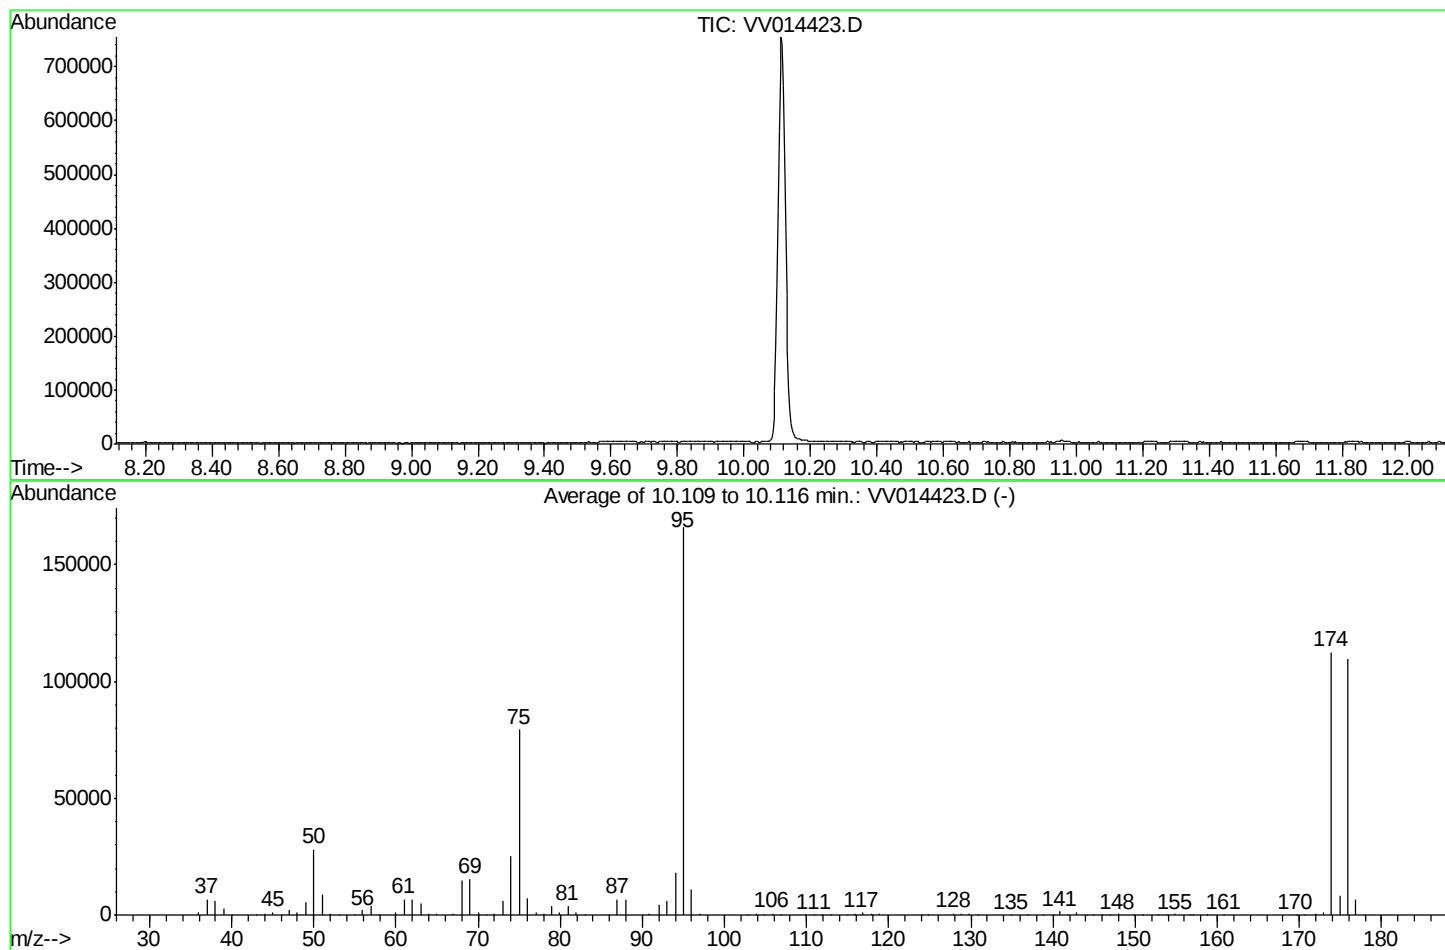

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	28109	PASS
75	95	30	80	47.8	79389	PASS
95	95	100	100	100.0	166080	PASS
96	95	5	9	6.6	10961	PASS
173	174	0.00	2	1.2	1330	PASS
174	95	50	120	67.8	112525	PASS
175	174	5	9	7.4	8288	PASS
176	174	95	101	97.2	109426	PASS
177	176	5	9	6.1	6729	PASS

m/z	Abundance
36.00	2366.0
37.00	6389.0
38.00	6578.0
39.00	2655.0
39.90	560.0
40.90	135.0
43.00	271.0
44.00	1196.0
45.00	1234.0
46.10	204.0
47.00	1852.0
47.90	1081.0
49.00	5532.0
50.00	27160.0
51.00	8719.0
52.00	284.0
55.00	391.0
56.00	1948.0
57.00	3712.0
57.90	238.0
59.90	1410.0
61.00	6659.0
62.00	6383.0
63.00	4854.0
63.90	572.0
64.90	305.0
67.00	467.0
68.00	14463.0
69.00	15007.0
70.00	1306.0
71.90	837.0
73.00	6056.0
74.00	24088.0
75.00	76112.0
76.00	6824.0
77.10	1104.0
77.90	717.0
78.90	3712.0
80.00	1021.0
80.90	3834.0
81.90	922.0
82.90	131.0
86.00	190.0
86.90	6697.0
88.00	6113.0
90.80	618.0
92.00	4279.0
93.00	5802.0
94.00	17128.0
95.00	158720.0
96.00	10613.0
97.00	313.0
102.80	121.0
103.90	595.0
104.70	158.0
105.90	675.0
106.80	151.0
109.90	117.0
110.90	187.0
113.00	154.0
115.00	164.0
115.90	509.0
116.80	855.0
117.90	515.0
118.80	660.0
124.00	161.0
124.80	137.0
127.90	602.0
128.80	266.0
129.80	517.0
130.80	246.0
135.00	226.0
136.90	278.0
140.00	124.0
140.90	1397.0
141.80	219.0
142.90	1115.0
144.10	137.0
144.90	174.0
146.00	215.0
146.80	131.0
148.00	309.0
149.90	186.0
152.80	114.0
153.90	164.0
154.90	363.0
156.80	223.0
158.70	131.0
160.80	136.0
169.70	108.0
172.00	478.0
173.00	1269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

173.90	104832.0
174.90	8026.0
175.90	101168.0
176.90	6574.0
177.90	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.90	2446.0
37.00	7025.0
38.00	6886.0
39.00	2811.0
40.00	535.0
40.90	170.0
41.90	125.0
43.00	254.0
44.00	1240.0
45.00	1346.0
46.10	181.0
47.00	2141.0
47.90	1132.0
49.00	5684.0
50.00	29184.0
51.00	9271.0
51.90	365.0
53.10	125.0
55.00	409.0
55.90	2056.0
57.00	4112.0
57.90	256.0
59.90	1314.0
61.00	7019.0
62.00	6789.0
63.00	5239.0
63.90	514.0
64.90	349.0
66.90	403.0
68.00	15348.0
69.00	15954.0
70.00	1453.0
70.90	126.0
71.90	844.0
73.00	6356.0
74.00	25912.0
75.00	82160.0
76.00	7070.0
77.10	1105.0
77.90	771.0
78.90	4081.0
79.90	1186.0
80.90	4078.0
81.90	1004.0
83.00	168.0
86.00	192.0
86.90	6949.0
88.00	7016.0
90.90	658.0
92.00	4679.0
93.00	6534.0
94.00	18800.0
95.00	171456.0
96.00	11370.0
97.10	343.0
102.90	156.0
103.90	629.0
104.80	161.0
105.90	660.0
106.80	181.0
109.80	119.0
110.90	177.0
111.80	128.0
112.90	160.0
115.00	177.0
115.90	562.0
116.80	886.0
117.90	523.0
118.80	768.0
123.90	167.0
124.80	108.0
127.90	585.0
128.80	302.0
129.80	548.0
130.80	275.0
134.90	243.0
136.90	268.0
140.00	122.0
140.90	1614.0
141.80	209.0
142.90	1320.0
144.00	159.0
144.90	190.0
146.00	241.0
146.90	157.0
147.90	380.0
149.90	187.0
151.00	114.0
152.80	111.0
153.90	144.0
154.90	398.0
156.80	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

158.80	163.0
160.80	178.0
169.60	112.0
172.00	494.0
173.00	1359.0
173.90	116032.0
174.90	8501.0
175.90	112888.0
176.90	6888.0
177.90	260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.90	2488.0
37.00	7152.0
38.00	6486.0
39.00	2519.0
40.00	505.0
40.90	164.0
41.90	123.0
42.90	213.0
44.00	1213.0
45.00	1315.0
46.10	162.0
47.00	2205.0
47.90	1023.0
49.00	5300.0
50.00	27984.0
51.00	8683.0
51.90	401.0
53.10	113.0
55.00	386.0
55.90	2063.0
57.00	4131.0
57.90	243.0
59.90	1145.0
61.00	6740.0
62.00	6455.0
63.00	5139.0
63.90	462.0
64.90	326.0
66.80	326.0
68.00	14907.0
69.00	15365.0
70.00	1327.0
71.00	148.0
72.00	752.0
73.00	6255.0
74.00	25312.0
75.00	79896.0
76.00	6781.0
77.00	1026.0
78.00	726.0
78.90	4134.0
79.90	1257.0
80.90	3987.0
81.90	979.0
83.00	162.0
85.90	181.0
86.90	6723.0
88.00	6667.0
90.90	618.0
92.00	4500.0
93.00	6487.0
94.00	18488.0
95.00	168064.0
96.00	10901.0
97.10	290.0
102.90	166.0
103.90	609.0
104.90	173.0
105.90	587.0
106.90	194.0
109.80	119.0
110.90	132.0
111.90	146.0
112.80	172.0
114.90	150.0
115.90	579.0
116.80	891.0
117.90	536.0
118.80	846.0
123.90	145.0
127.90	541.0
128.90	350.0
129.80	493.0
130.80	259.0
134.90	232.0
136.90	246.0
138.80	116.0
140.90	1714.0
141.80	212.0
142.90	1376.0
144.00	159.0
144.90	201.0
145.90	276.0
146.80	127.0
147.90	408.0
149.80	176.0
151.00	116.0
152.70	123.0
153.90	116.0
154.90	381.0
156.70	165.0
157.10	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

158.80	187.0
160.80	215.0
170.60	102.0
172.00	456.0
173.00	1363.0
173.90	116712.0
174.90	8337.0
175.90	114224.0
176.90	6726.0
177.90	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	1451.0
37.00	199.0
38.00	617.0
39.90	446.0
41.00	172.0
41.90	132.0
42.90	117.0
43.90	625.0
55.10	109.0
155.70	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35