

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012921\
 Data File : VV020213.D
 Acq On : 28 Jan 2021 13:08
 Operator : SY/MD
 Sample : VV0129WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK702

Quant Time: Jan 29 00:52:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 28 12:11:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	458708	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	436481	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.257	152	231331	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.303	65	152337	4.69	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.80%	
7) Chloroethane-d5	1.566	69	127200	4.54	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.80%	
11) 1,1-Dichloroethene-d2	2.106	63	152771	3.37	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.40%	
20) 2-Butanone-d5	3.930	46	308137	46.27	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	92.54%	
24) Chloroform-d	4.354	84	286870	4.57	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.40%	
26) 1,2-Dichloroethane-d4	5.039	65	146368	4.70	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.00%	
32) Benzene-d6	5.055	84	560612	4.83	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.60%	
36) 1,2-Dichloropropane-d6	6.074	67	168827	4.93	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.60%	
41) Toluene-d8	7.318	98	509108	4.74	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.80%	
43) trans-1,3-Dichloroprop...	7.627	79	57208	4.48	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.60%	
46) 2-Hexanone-d5	8.097	63	244488	46.14	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.28%	
56) 1,1,2,2-Tetrachloroeth...	10.225	84	114463	4.94	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.80%	
66) 1,2-Dichlorobenzene-d4	11.633	152	207928	5.16	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.20%	
Target Compounds						
16) Methylene chloride	2.508	84	5293	0.16	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012921\
Data File : VV020213.D
Acq On : 28 Jan 2021 13:08
Operator : SY/MD
Sample : VV0129WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK702

Quant Time: Jan 29 00:52:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 28 12:11:07 2021
Response via : Initial Calibration

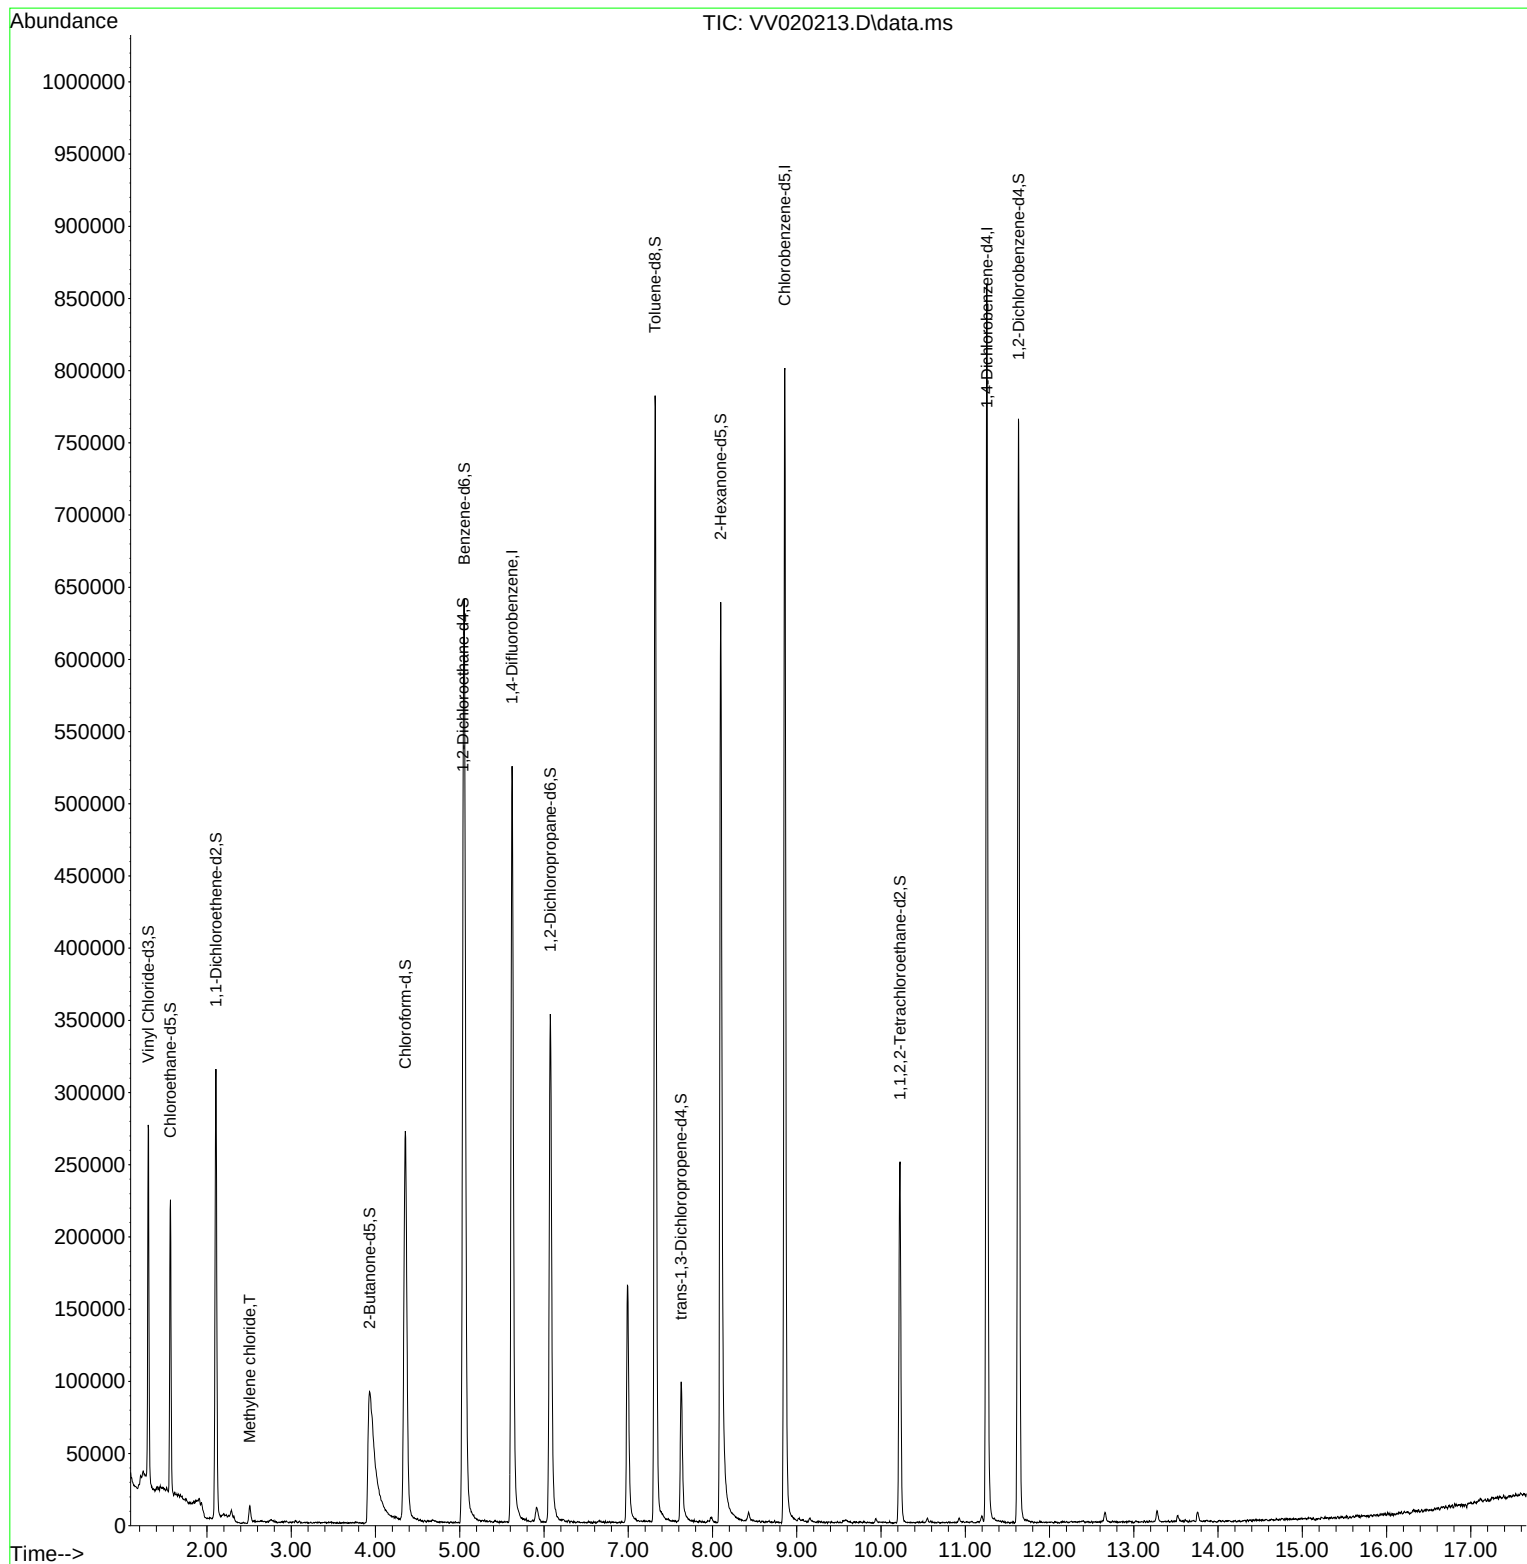

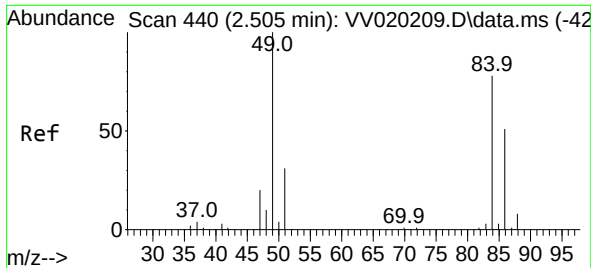

#16
Methylene chloride
Concen: 0.16 ug/L
RT: 2.508 min Scan# 441
Delta R.T. 0.003 min
Lab File: VV020213.D
Acq: 28 Jan 2021 13:08

Instrument :
MSVOA_V
ClientSampleId :
VBLK702

Tgt Ion:	84	Resp:	5293
Ion	Ratio	Lower	Upper
84	100		
86	68.2	42.8	79.4
49	112.5	93.9	174.3

