
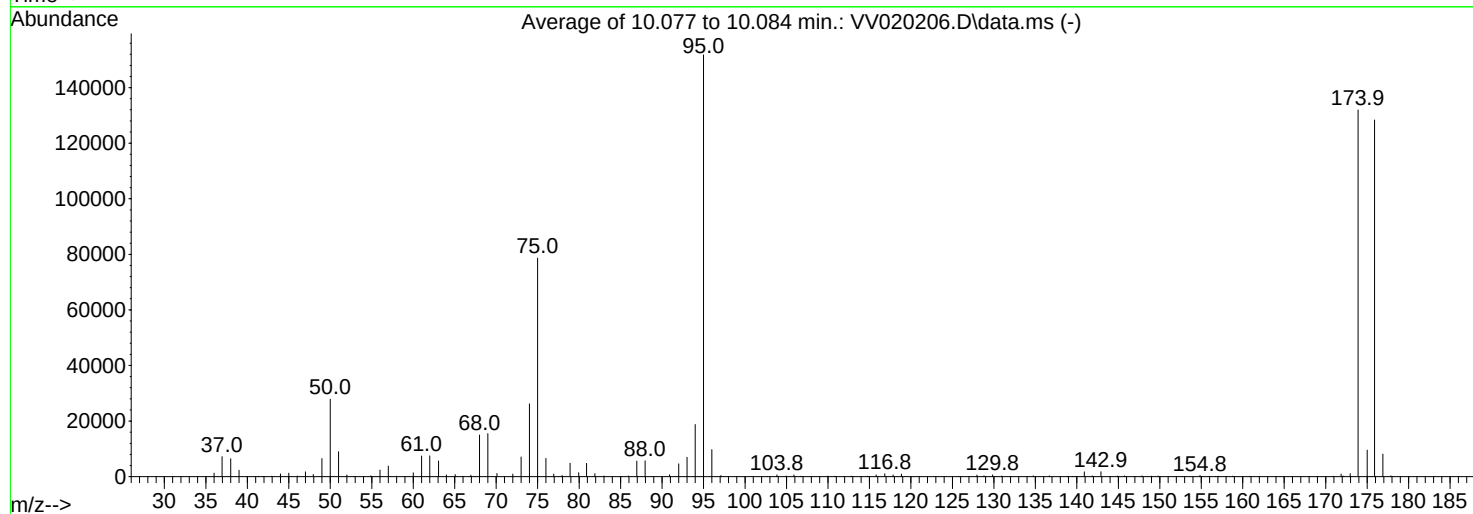


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012921\
 Data File : VV020206.D
 Acq On : 28 Jan 2021 08:48
 Operator : SY/MD
 Sample : BFB84
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012921WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jan 30 02:26:26 2021

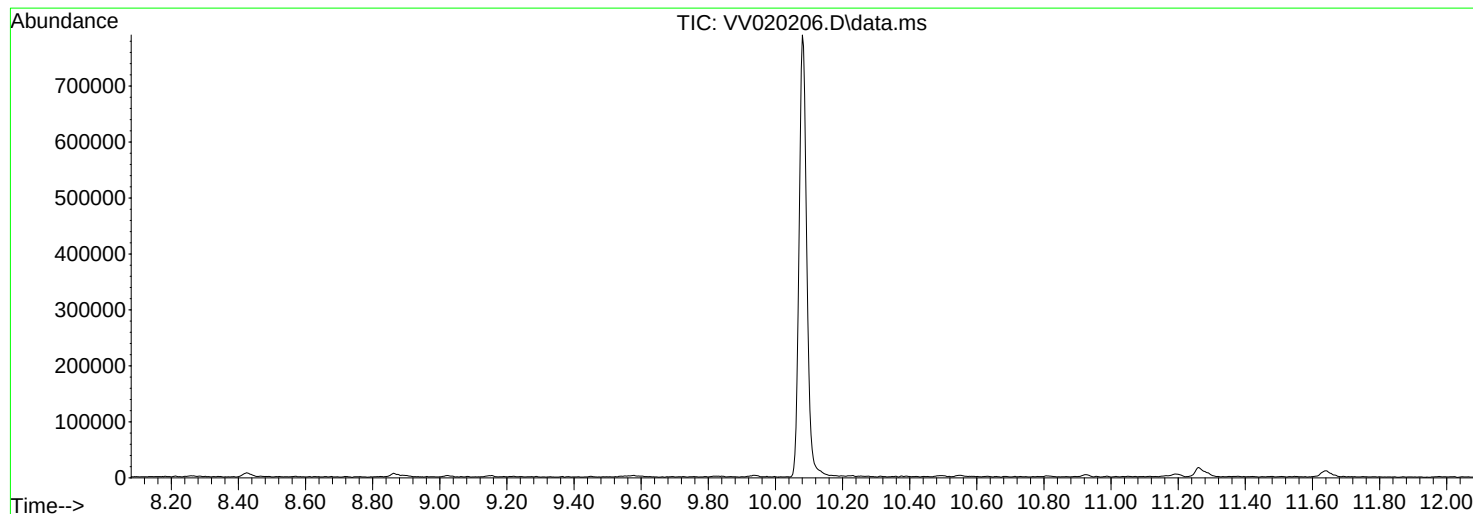

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	27885	PASS
75	95	30	80	51.8	78680	PASS
95	95	100	100	100.0	151787	PASS
96	95	5	9	6.4	9740	PASS
173	174	0.00	2	0.9	1127	PASS
174	95	50	120	87.0	131987	PASS
175	174	5	9	7.2	9549	PASS
176	174	95	105	97.2	128344	PASS
177	176	5	10	6.3	8116	PASS

m/z	Abundance
35.10	125.0
36.90	119.0
39.00	125.0
40.00	416.0
42.00	113.0
44.00	627.0
48.60	110.0
53.90	130.0
54.80	112.0
78.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1161.0
37.00	6977.0
38.00	6358.0
39.00	2545.0
39.90	330.0
41.40	116.0
41.90	129.0
42.90	173.0
44.00	1497.0
45.00	1159.0
46.10	211.0
47.00	1586.0
48.00	867.0
49.00	6321.0
50.00	26912.0
51.00	8840.0
52.00	572.0
52.80	163.0
55.00	399.0
56.00	2361.0
57.00	3948.0
58.00	147.0
60.00	1299.0
61.00	7249.0
62.00	7346.0
63.10	5398.0
64.00	572.0
65.00	773.0
65.90	119.0
67.00	470.0
68.00	14376.0
69.00	14753.0
70.10	1119.0
72.00	828.0
73.00	6921.0
74.00	25168.0
75.00	75904.0
76.00	6545.0
77.00	1042.0
78.00	524.0
78.90	4883.0
80.00	1350.0
80.90	4507.0
81.90	1088.0
83.00	237.0
85.90	196.0
86.90	5425.0
88.00	5507.0
88.80	230.0
90.90	693.0
92.00	4273.0
93.00	6722.0
94.00	18208.0
95.00	145792.0
96.00	9916.0
97.10	430.0
102.70	113.0
103.90	578.0
104.90	217.0
105.90	496.0
106.70	183.0
110.00	202.0
110.90	147.0
112.90	168.0
114.80	168.0
115.80	555.0
116.80	1024.0
117.80	577.0
118.90	949.0
127.90	579.0
128.80	330.0
129.80	593.0
131.00	190.0
134.70	275.0
136.70	315.0
138.80	124.0
139.80	120.0
140.90	1642.0
141.90	227.0
142.90	1620.0
144.90	216.0
145.70	343.0
147.80	338.0
149.00	175.0
149.80	271.0
152.70	156.0
154.80	368.0
156.80	216.0
158.80	204.0
170.90	205.0
171.80	821.0
172.10	700.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

172.90	1570.0
173.90	123384.0
175.00	8882.0
175.90	120072.0
176.90	7895.0
177.90	287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1302.0
37.00	7609.0
38.00	6701.0
39.00	2467.0
39.90	284.0
41.40	142.0
41.80	141.0
42.90	156.0
44.00	1654.0
45.00	1310.0
46.00	267.0
47.00	1816.0
48.00	832.0
49.00	6758.0
50.00	28688.0
51.00	9297.0
52.00	649.0
52.80	115.0
55.00	448.0
56.00	2433.0
57.00	3896.0
58.00	182.0
60.00	1432.0
61.00	7674.0
62.00	7776.0
63.00	5909.0
64.00	646.0
65.10	759.0
65.90	143.0
66.90	540.0
68.00	15485.0
69.00	16027.0
70.10	1172.0
72.00	959.0
73.00	7322.0
74.00	27008.0
75.00	81424.0
76.00	6792.0
77.00	955.0
78.00	573.0
78.90	5025.0
79.90	1482.0
80.90	4976.0
81.90	1158.0
83.00	234.0
85.90	211.0
86.90	5718.0
88.00	5915.0
90.90	699.0
92.00	4754.0
93.00	7213.0
94.00	19496.0
95.00	157376.0
96.00	10068.0
97.10	391.0
102.70	109.0
103.80	678.0
105.00	241.0
105.90	599.0
106.70	172.0
110.00	159.0
110.80	161.0
112.00	129.0
112.80	210.0
114.70	176.0
115.80	669.0
116.90	1044.0
117.80	674.0
118.90	973.0
125.80	111.0
128.00	633.0
128.80	353.0
129.80	648.0
130.90	248.0
134.80	318.0
136.70	345.0
138.90	149.0
139.50	108.0
139.90	141.0
140.90	1812.0
141.80	282.0
142.90	1872.0
144.90	234.0
145.70	327.0
146.90	110.0
147.90	305.0
149.00	162.0
149.80	243.0
152.70	127.0
154.90	483.0
156.70	237.0
157.10	245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

158.80	222.0
160.90	137.0
170.90	180.0
171.80	906.0
173.00	1810.0
173.90	136256.0
175.00	9909.0
175.90	132992.0
176.90	8417.0
177.90	296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1345.0
37.00	7342.0
38.00	6362.0
39.00	2295.0
40.00	279.0
41.30	127.0
41.80	188.0
43.00	164.0
44.00	1684.0
45.00	1366.0
46.00	246.0
47.00	1808.0
47.90	767.0
49.00	6392.0
50.00	28056.0
51.00	8789.0
52.00	655.0
52.90	110.0
54.90	424.0
56.00	2316.0
57.00	3641.0
58.00	193.0
60.00	1411.0
61.00	7398.0
62.00	7294.0
63.00	5636.0
64.00	637.0
65.00	666.0
66.00	148.0
66.90	511.0
68.00	15088.0
69.00	15770.0
70.10	1158.0
72.00	925.0
73.00	7081.0
74.00	26352.0
75.00	78712.0
76.00	6374.0
76.90	799.0
77.90	535.0
78.90	4644.0
79.90	1468.0
80.90	4848.0
81.90	1083.0
83.00	213.0
86.00	227.0
87.00	5573.0
87.90	5706.0
90.90	638.0
92.00	4737.0
93.00	6942.0
94.00	18592.0
95.00	152192.0
96.00	9235.0
97.10	332.0
103.80	706.0
105.00	258.0
105.90	730.0
106.80	142.0
109.80	124.0
110.80	181.0
111.90	175.0
112.70	228.0
114.70	206.0
115.80	697.0
116.90	1039.0
117.90	691.0
118.80	886.0
125.80	131.0
127.90	529.0
128.80	323.0
129.90	636.0
130.90	316.0
134.80	306.0
136.70	286.0
138.90	139.0
139.50	135.0
140.00	158.0
140.90	1773.0
141.80	285.0
142.90	1889.0
144.00	134.0
144.90	234.0
145.80	272.0
146.90	118.0
147.80	298.0
149.00	135.0
149.80	175.0
154.90	522.0
157.00	278.0
158.80	196.0
160.80	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

170.90	171.0
171.90	1002.0
173.90	136320.0
175.00	9856.0
175.90	131968.0
176.90	8037.0
177.80	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84