
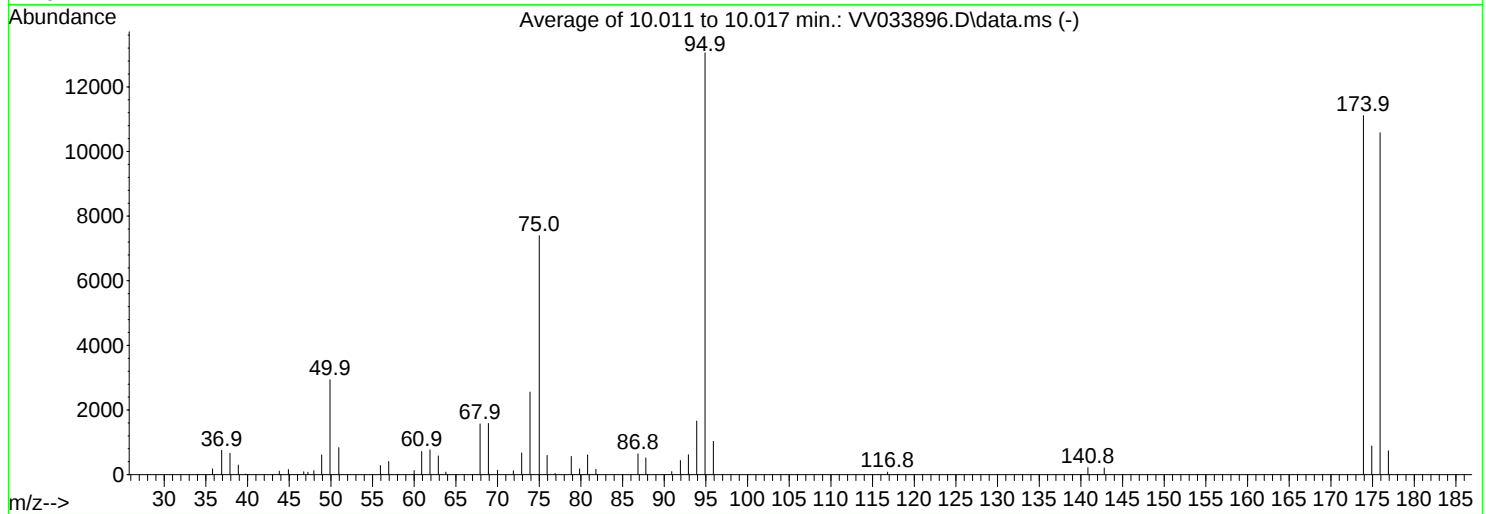


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012924\
Data File : VV033896.D
Acq On : 29 Jan 2024 09:54
Operator : SY/MD
Sample : BFB243
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB243

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 30 03:43:29 2024

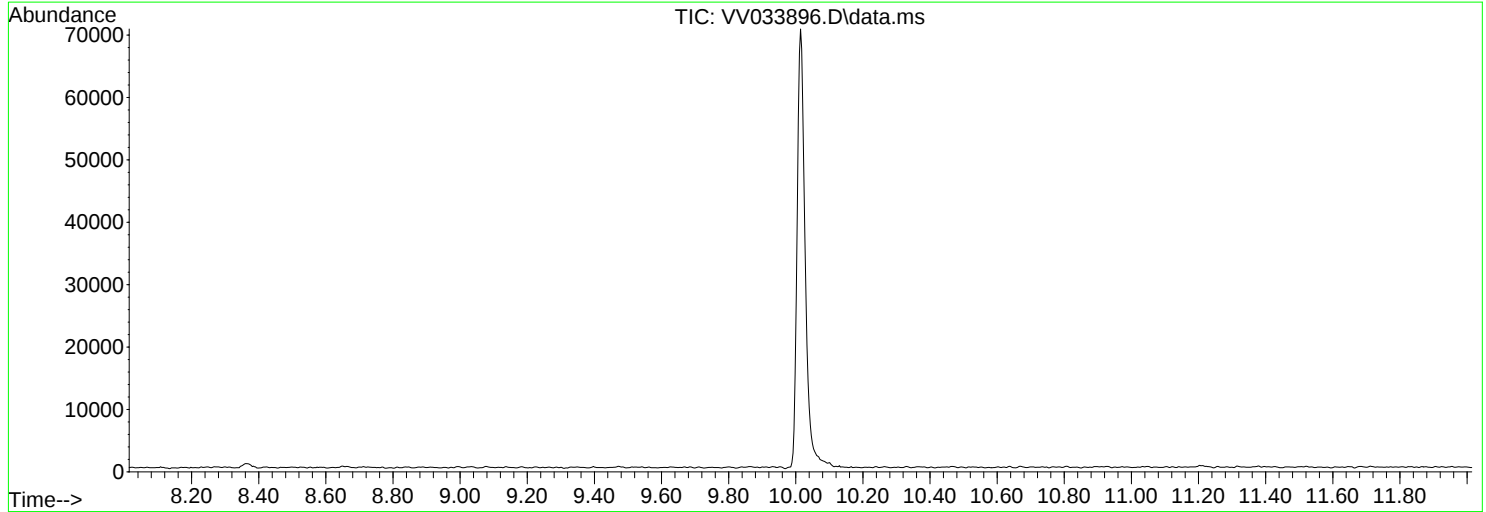

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	2935	PASS
75	95	30	80	56.7	7400	PASS
95	95	100	100	100.0	13053	PASS
96	95	5	9	7.9	1029	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.1	11111	PASS
175	174	5	9	8.0	885	PASS
176	174	95	105	95.2	10581	PASS
177	176	5	10	7.0	740	PASS

m/z	Abundance
39.80	544.0
43.70	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
35.90	187.0
36.90	757.0
37.90	678.0
38.90	286.0
39.90	592.0
43.90	297.0
44.90	122.0
46.70	136.0
47.30	121.0
48.00	109.0
48.90	578.0
49.90	2879.0
50.90	856.0
56.00	297.0
57.00	381.0
60.00	136.0
60.90	728.0
61.90	777.0
62.90	579.0
63.80	113.0
67.90	1498.0
68.90	1572.0
70.00	172.0
71.90	117.0
72.90	658.0
73.90	2426.0
75.00	7298.0
76.00	621.0
76.90	114.0
78.80	577.0
79.90	162.0
80.80	651.0
81.80	158.0
86.80	621.0
87.80	492.0
91.90	434.0
92.90	597.0
93.90	1614.0
94.90	12944.0
95.90	980.0
116.80	117.0
140.80	196.0
142.80	171.0
173.90	10548.0
174.90	830.0
175.90	10133.0
176.90	737.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
35.90	180.0
36.90	763.0
37.90	695.0
38.90	316.0
39.80	551.0
43.90	312.0
44.90	171.0
46.80	126.0
47.20	106.0
48.00	129.0
48.90	619.0
49.90	3015.0
51.00	860.0
55.90	298.0
56.90	417.0
60.00	143.0
60.90	757.0
61.90	804.0
62.90	573.0
63.80	120.0
67.90	1636.0
68.90	1645.0
70.00	138.0
71.90	130.0
72.90	697.0
73.90	2664.0
75.00	7604.0
75.90	606.0
78.90	581.0
79.80	186.0
80.80	609.0
81.80	176.0
86.90	661.0
87.80	539.0
90.90	134.0
91.90	461.0
92.90	624.0
93.90	1719.0
94.90	13426.0
95.90	1096.0
116.80	114.0
140.90	236.0
142.80	220.0
173.90	11514.0
174.90	920.0
175.90	10920.0
176.90	761.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
35.90	163.0
36.90	733.0
37.90	604.0
38.90	289.0
39.90	554.0
43.90	288.0
44.90	184.0
47.90	135.0
48.90	624.0
49.90	2911.0
51.00	802.0
55.90	248.0
56.90	417.0
60.00	115.0
60.90	675.0
61.90	728.0
62.90	582.0
67.90	1580.0
68.90	1533.0
70.00	111.0
71.90	117.0
72.90	671.0
73.90	2580.0
75.00	7299.0
75.90	554.0
78.90	543.0
79.80	182.0
80.80	568.0
81.80	162.0
86.90	652.0
87.80	532.0
90.90	146.0
92.00	417.0
92.90	621.0
93.90	1637.0
94.90	12788.0
95.90	1010.0
140.90	226.0
142.80	229.0
173.90	11271.0
174.90	905.0
175.90	10691.0
176.90	723.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243