
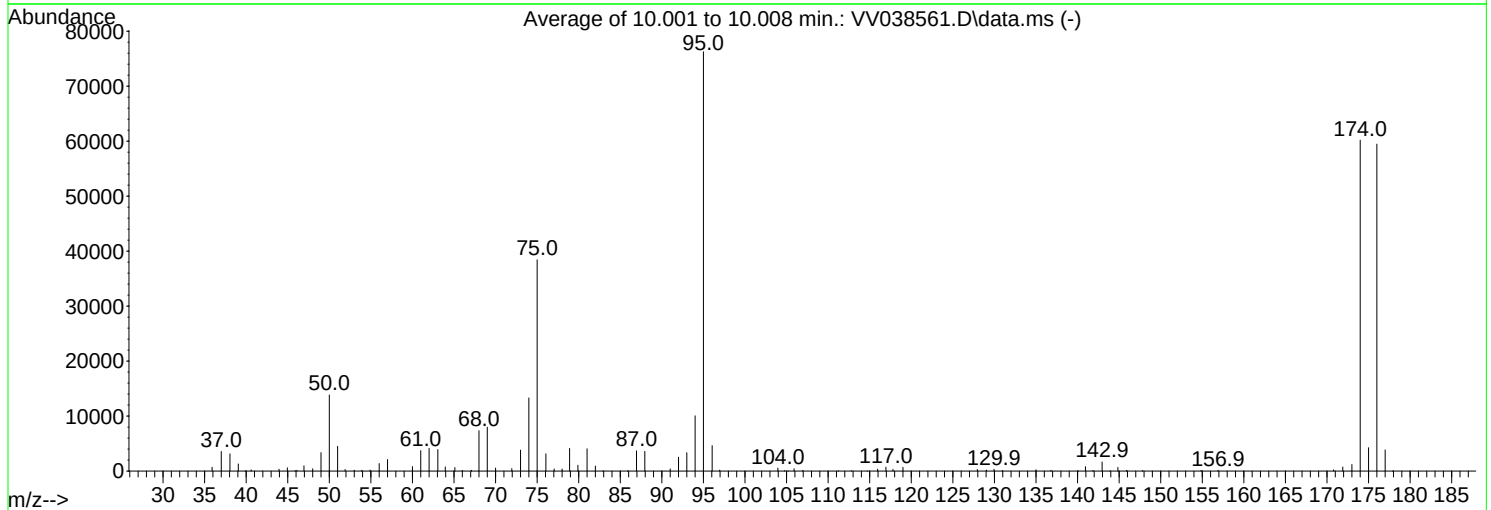


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012925\
Data File : VV038561.D
Acq On : 29 Jan 2025 08:54
Operator : SY/MD
Sample : BFB229
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB229

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jan 28 08:06:10 2025

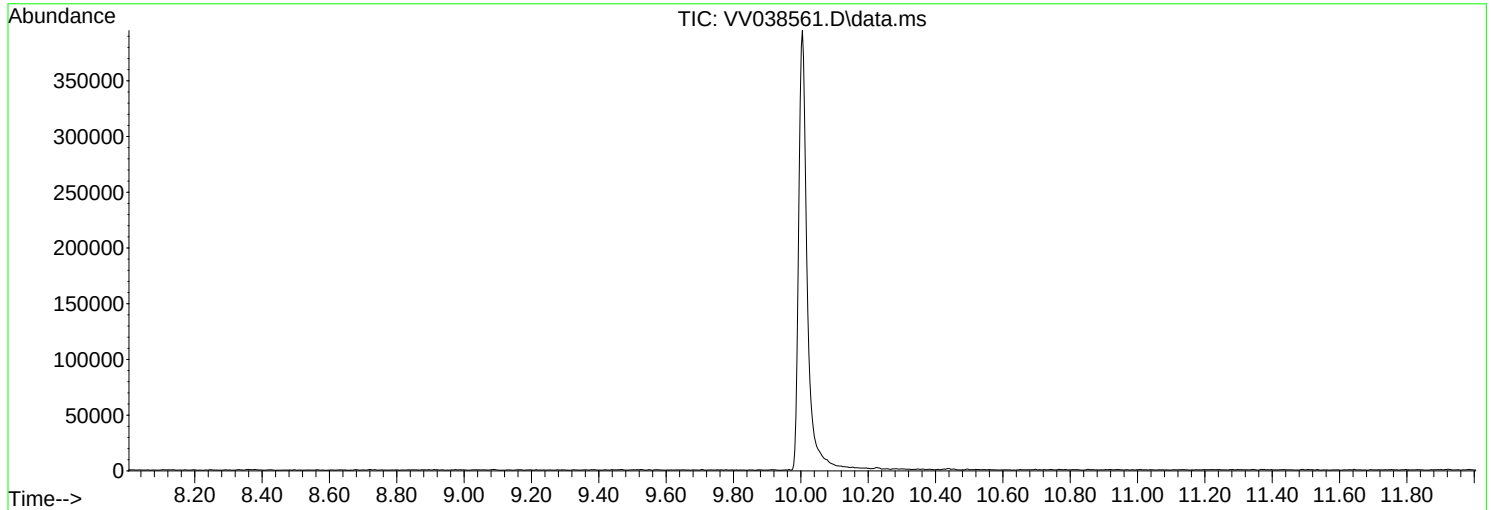

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	13842	PASS
75	95	30	80	50.4	38429	PASS
95	95	100	100	100.0	76264	PASS
96	95	5	9	6.1	4640	PASS
173	174	0.00	2	2.0	1203	PASS
174	95	50	120	78.9	60192	PASS
175	174	5	9	7.1	4249	PASS
176	174	95	101	98.8	59464	PASS
177	176	5	9	6.5	3858	PASS

m/z	Abundance
37.60	103.0
40.00	451.0
42.20	110.0
43.90	360.0
53.60	101.0
77.00	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
35.90	774.0
37.00	3728.0
38.10	3271.0
39.00	1482.0
39.90	545.0
40.60	186.0
44.00	737.0
45.00	548.0
45.90	283.0
47.00	1007.0
48.00	435.0
49.00	3508.0
50.00	14484.0
51.00	4303.0
51.90	267.0
53.00	145.0
53.90	132.0
54.90	205.0
56.00	1409.0
57.00	2052.0
60.00	755.0
61.00	3872.0
62.00	4019.0
63.10	3936.0
63.90	717.0
65.10	606.0
66.00	131.0
67.10	135.0
68.00	7345.0
69.00	7818.0
70.00	494.0
72.00	406.0
73.00	3882.0
74.00	13449.0
75.00	39336.0
76.10	3248.0
77.10	557.0
78.00	393.0
78.90	4266.0
79.90	1109.0
81.00	3783.0
82.00	848.0
86.90	3775.0
87.90	3596.0
91.00	387.0
92.00	2589.0
93.00	3428.0
94.00	9794.0
95.00	76832.0
96.10	4985.0
96.90	142.0
104.00	495.0
104.80	115.0
105.90	439.0
106.90	125.0
111.20	120.0
112.80	128.0
115.90	370.0
117.00	717.0
117.80	299.0
119.00	732.0
127.90	329.0
129.00	188.0
130.00	331.0
131.00	118.0
135.00	235.0
136.80	133.0
140.10	110.0
141.00	776.0
141.80	115.0
142.90	1673.0
144.80	659.0
145.90	152.0
147.80	115.0
154.90	140.0
156.90	150.0
170.70	252.0
171.90	725.0
173.10	813.0
174.00	58784.0
175.00	4223.0
176.00	57016.0
177.00	3936.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
35.90	734.0
37.00	3705.0
38.10	3221.0
39.00	1302.0
39.90	502.0
40.60	237.0
44.00	713.0
45.00	599.0
46.10	235.0
46.90	1001.0
48.00	410.0
49.00	3453.0
50.00	14288.0
51.00	4675.0
51.90	288.0
53.00	181.0
53.90	146.0
54.90	200.0
56.00	1403.0
57.00	2160.0
60.00	835.0
61.00	3848.0
62.00	4213.0
63.00	4055.0
64.00	765.0
65.10	685.0
66.00	110.0
67.10	142.0
68.00	7628.0
69.00	8291.0
70.00	565.0
71.90	453.0
73.00	3986.0
74.00	13789.0
75.00	39584.0
76.10	3177.0
77.10	547.0
78.00	409.0
78.90	4212.0
79.90	1103.0
81.00	4263.0
82.00	965.0
85.90	119.0
87.00	3722.0
88.00	3736.0
91.00	416.0
92.00	2592.0
93.00	3384.0
94.00	10369.0
95.00	78504.0
96.10	4706.0
96.90	169.0
103.90	588.0
104.70	100.0
105.90	463.0
106.90	136.0
111.30	102.0
112.80	106.0
116.00	379.0
117.00	736.0
117.80	332.0
119.00	716.0
127.90	289.0
129.10	189.0
129.90	361.0
131.00	125.0
135.00	267.0
136.80	166.0
140.90	824.0
141.80	119.0
143.00	1748.0
144.90	715.0
145.90	147.0
147.80	106.0
154.80	144.0
156.90	176.0
170.80	225.0
171.90	778.0
172.90	908.0
173.10	907.0
174.00	62336.0
175.00	4300.0
176.00	61832.0
177.00	3938.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
35.90	619.0
37.00	3278.0
38.00	2921.0
39.10	1090.0
39.80	504.0
40.60	254.0
44.00	666.0
44.90	629.0
46.10	187.0
46.90	914.0
48.00	421.0
49.00	3135.0
50.00	12754.0
51.00	4503.0
51.90	272.0
53.00	168.0
53.90	156.0
54.90	179.0
56.00	1299.0
57.00	2107.0
60.00	840.0
61.00	3439.0
62.00	4131.0
63.00	3744.0
64.00	798.0
65.10	662.0
66.00	120.0
67.10	145.0
68.00	7078.0
69.00	7823.0
70.00	614.0
71.90	501.0
73.00	3578.0
74.00	12684.0
75.00	36368.0
76.00	3000.0
77.10	470.0
78.00	326.0
78.90	3879.0
79.90	1026.0
81.00	4137.0
82.00	954.0
82.90	106.0
85.90	112.0
87.00	3563.0
88.00	3426.0
91.00	400.0
92.00	2402.0
93.00	3213.0
94.00	10007.0
95.00	73456.0
96.00	4229.0
97.00	206.0
104.00	562.0
105.20	120.0
105.90	370.0
107.00	124.0
114.70	110.0
116.00	317.0
116.90	692.0
117.80	304.0
119.00	627.0
128.00	248.0
129.10	170.0
129.90	347.0
130.80	122.0
135.00	244.0
136.80	144.0
140.90	808.0
141.90	137.0
143.00	1568.0
143.90	112.0
144.90	659.0
145.90	116.0
147.80	106.0
154.80	137.0
156.90	162.0
170.90	194.0
171.90	763.0
172.90	981.0
174.00	59456.0
175.00	4225.0
176.00	59544.0
177.00	3701.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229