

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV013020\
 Data File : VV014437.D
 Acq On : 30 Jan 2020 15:40
 Operator : SY/MD
 Sample : L1322-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XR9

Quant Time: Jan 31 08:11:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR012920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 31 07:45:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	215871	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	199845	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	91557	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	62621	5.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.40%
7) Chloroethane-d5	1.59	69	42363	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.20%
11) 1,1-Dichloroethene-d2	2.13	63	69743	3.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.60%
20) 2-Butanone-d5	3.95	46	152747	60.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.38%
24) Chloroform-d	4.40	84	117732	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.08	65	64630	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.60%
32) Benzene-d6	5.10	84	295861	5.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.00%
36) 1,2-Dichloropropane-d6	6.11	67	90307	5.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.00%
41) Toluene-d8	7.36	98	266151	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
43) trans-1,3-Dichloropropene-	7.66	79	35187	4.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.20%
46) 2-Hexanone-d5	8.13	63	139286	53.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.94%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	60172	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	89160	5.43	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.60%


Target Compounds					Ovalue
25) Chloroform	4.42	83	17835	0.647 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV013020\
Data File : VV014437.D
Acq On : 30 Jan 2020 15:40
Operator : SY/MD
Sample : L1322-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XR9

Quant Time: Jan 31 08:11:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR012920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 31 07:45:41 2020
Response via : Initial Calibration

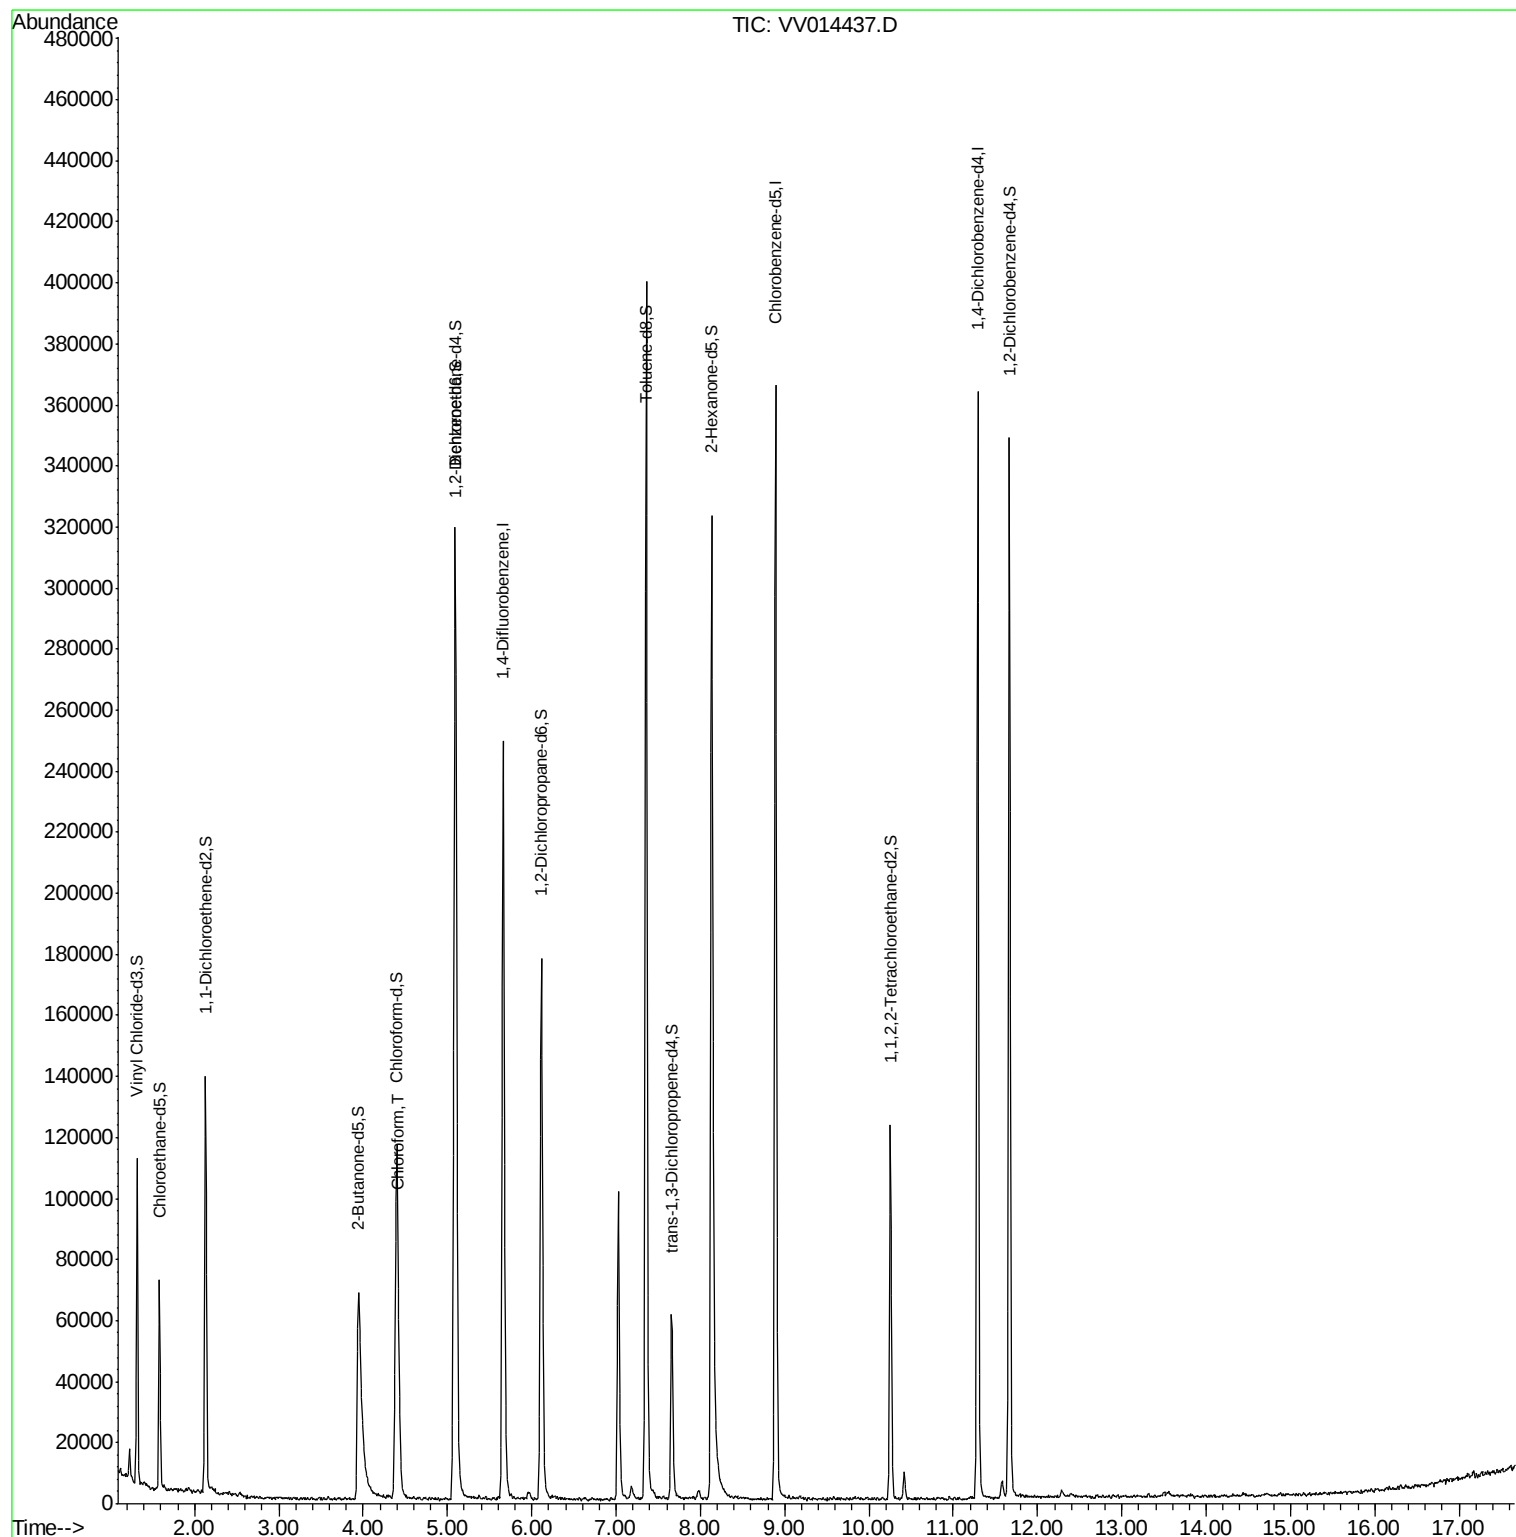

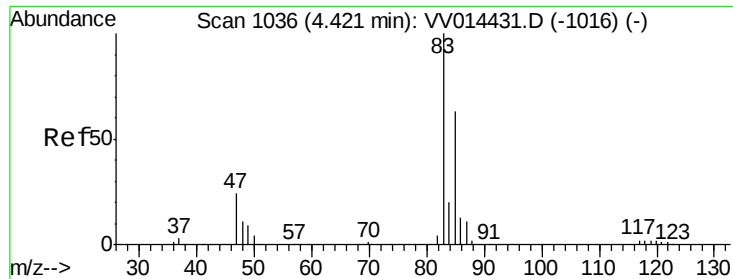

#25

Chloroform

Concen: 0.647 ug/L

RT: 4.42 min Scan# 1037

Delta R.T. 0.00 min

Lab File: VV014437.D

Acq: 30 Jan 2020 15:40

Instrument :

MSVOA_V

ClientSampleId :

C0XR9

Tot Ion: 83 Resp: 17835

Ion Ratio Lower Upper

83 100

85 62.6 45.9 85.3

