

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV013020\
 Data File : VV014438.D
 Acq On : 30 Jan 2020 16:04
 Operator : SY/MD
 Sample : L1322-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XS0

Quant Time: Jan 31 08:13:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR012920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 31 07:45:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	209669	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	192177	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	89602	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58599	4.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.80%
7) Chloroethane-d5	1.59	69	41936	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.20%
11) 1,1-Dichloroethene-d2	2.13	63	64559	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	3.95	46	105265	43.06	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.12%
24) Chloroform-d	4.40	84	114022	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.00%
26) 1,2-Dichloroethane-d4	5.08	65	59741	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	5.10	84	274555	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.12	67	82590	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.36	98	247750	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
43) trans-1,3-Dichloropropene-	7.66	79	33227	4.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.40%
46) 2-Hexanone-d5	8.14	63	130837	52.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	57840	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	82713	5.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.00%


Target Compounds				Ovalue
25) Chloroform	4.42	83	16272	0.608 ug/L 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV013020\
Data File : VV014438.D
Acq On : 30 Jan 2020 16:04
Operator : SY/MD
Sample : L1322-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XS0

Quant Time: Jan 31 08:13:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR012920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 31 07:45:41 2020
Response via : Initial Calibration

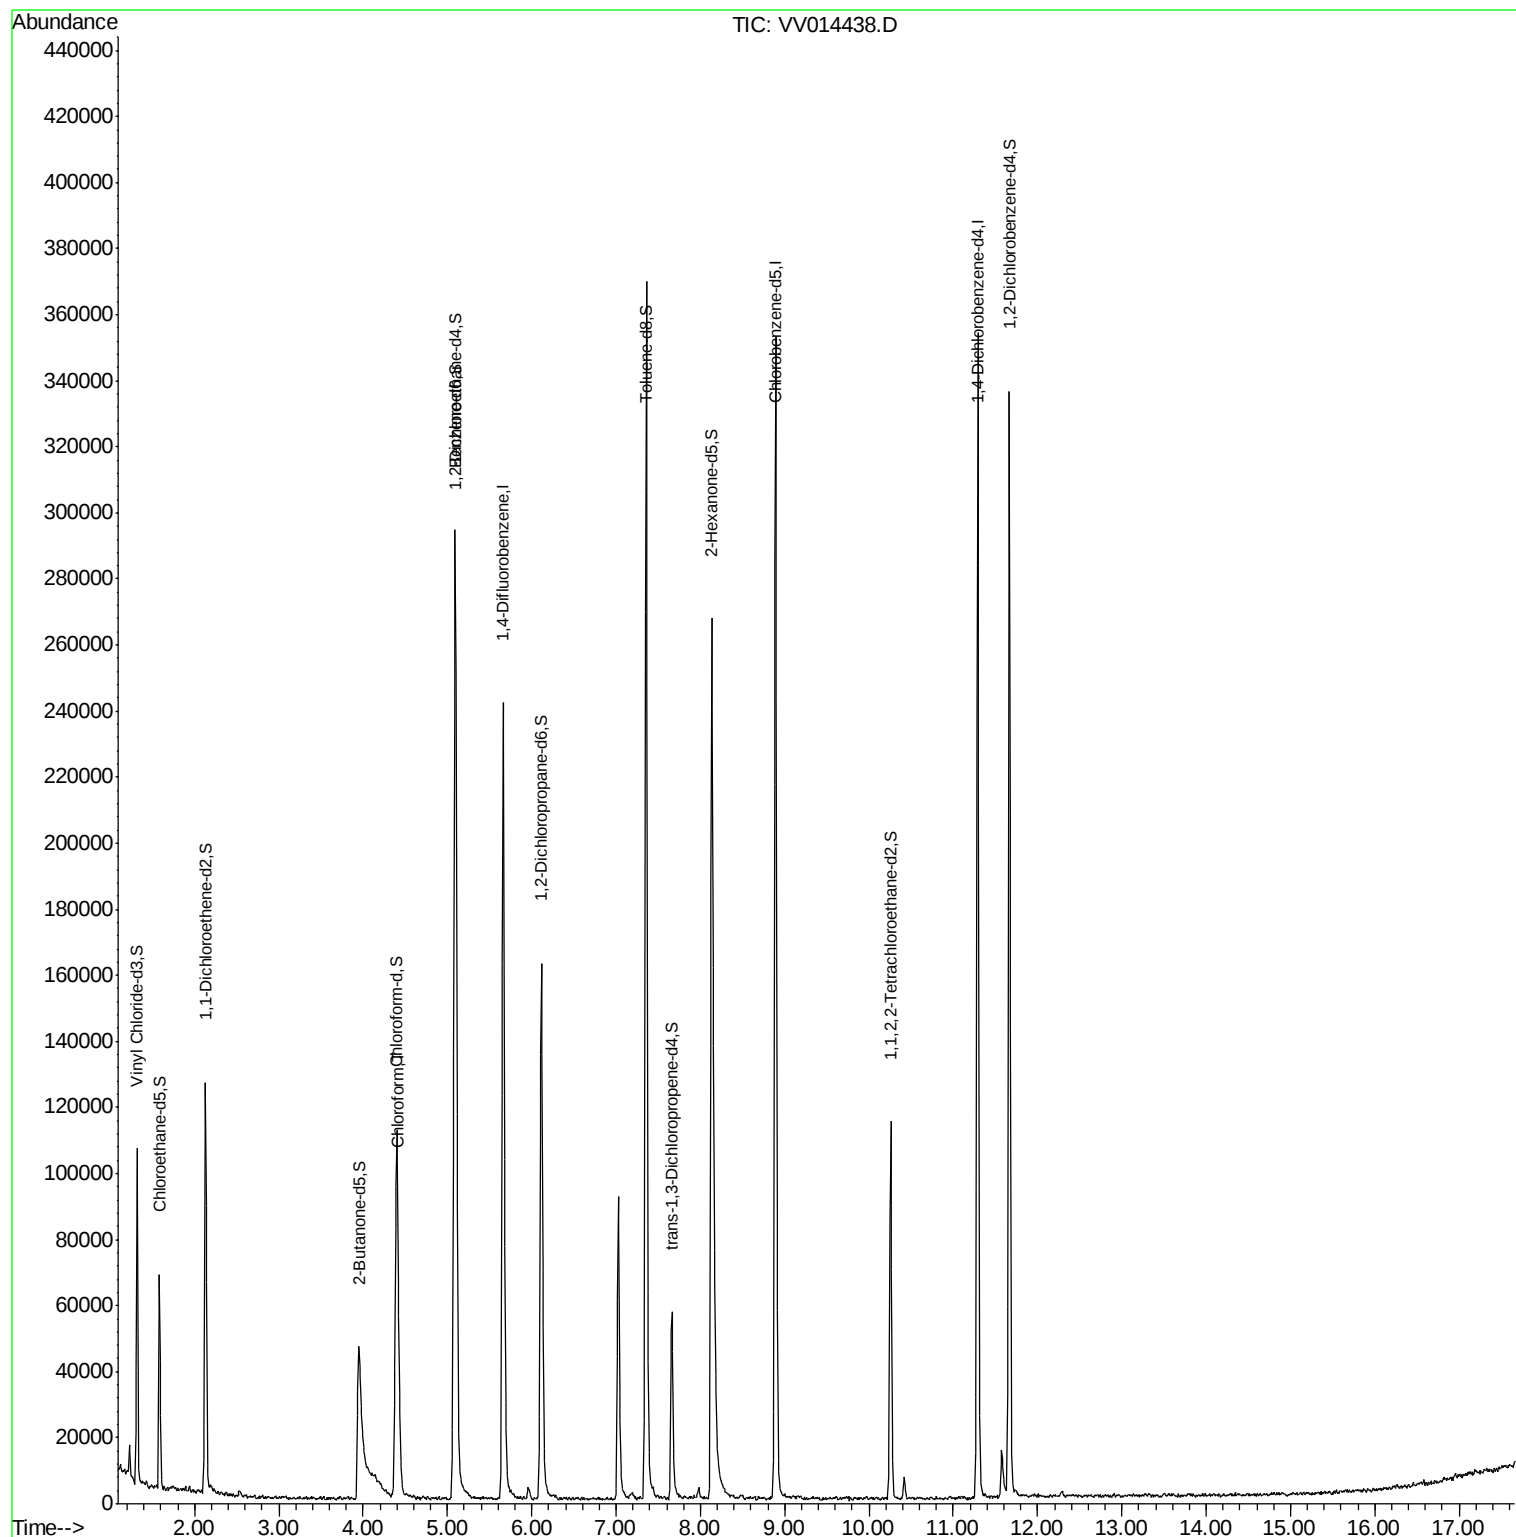

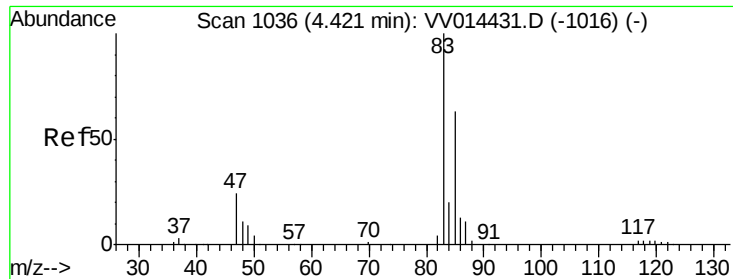

#25
 Chloroform
 Concen: 0.608 ug/L
 RT: 4.42 min Scan# 1036
 Delta R.T. 0.00 min
 Lab File: VV014438.D
 Acq: 30 Jan 2020 16:04

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XS0

Tot Ion: 83 Resp: 16272
 Ion Ratio Lower Upper
 83 100
 85 61.0 45.9 85.3

