


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV013020\
 Data File : VV014430.D
 Acq On : 30 Jan 2020 09:03
 Operator : SY/MD
 Sample : BFB36
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB36

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR012920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jan 31 23:09:59 2020

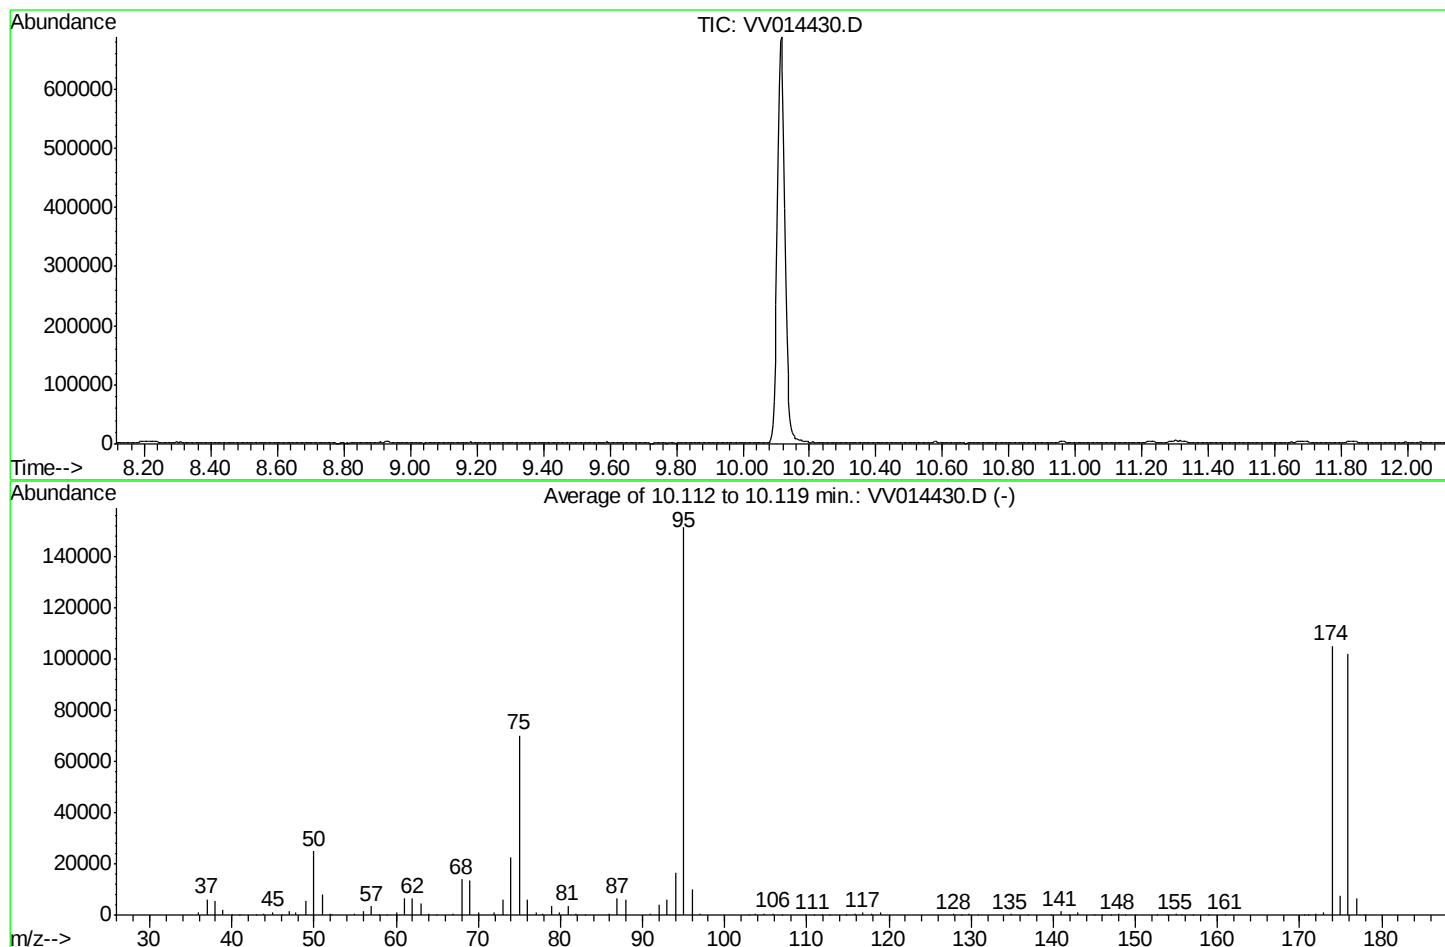

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	24994	PASS
75	95	30	80	46.3	70125	PASS
95	95	100	100	100.0	151509	PASS
96	95	5	9	6.7	10151	PASS
173	174	0.00	2	1.1	1167	PASS
174	95	50	120	69.4	105098	PASS
175	174	5	9	7.4	7732	PASS
176	174	95	101	97.2	102149	PASS
177	176	5	9	6.5	6590	PASS

m/z	Abundance
35.90	1357.0
37.00	6449.0
38.00	5633.0
39.00	2185.0
40.00	536.0
41.00	181.0
43.00	160.0
43.90	1131.0
45.00	1202.0
45.90	180.0
47.00	1593.0
47.80	1072.0
49.00	5648.0
50.00	26256.0
51.00	8011.0
51.90	336.0
55.00	370.0
56.00	1849.0
57.00	3688.0
57.90	253.0
60.00	1195.0
61.00	6518.0
62.00	6637.0
63.00	4735.0
63.90	428.0
64.90	254.0
66.90	458.0
68.00	14166.0
69.00	14409.0
70.00	1236.0
71.90	804.0
73.00	6220.0
74.00	23856.0
75.00	72240.0
76.00	6226.0
77.00	865.0
77.90	509.0
78.90	3524.0
79.90	1217.0
80.90	3581.0
81.90	758.0
83.10	133.0
85.90	332.0
86.90	6668.0
87.90	6235.0
90.90	633.0
92.00	4270.0
93.00	6290.0
94.00	16800.0
95.00	155648.0
96.00	10602.0
96.90	341.0
102.90	121.0
103.80	620.0
104.90	318.0
105.90	632.0
107.00	146.0
109.80	116.0
110.80	159.0
111.80	157.0
112.80	183.0
114.70	203.0
115.80	488.0
116.80	861.0
117.90	504.0
118.90	815.0
127.90	513.0
128.80	305.0
129.80	518.0
130.80	238.0
134.90	304.0
136.90	255.0
140.90	1430.0
141.90	181.0
142.90	1174.0
144.90	114.0
145.90	171.0
146.90	135.0
148.00	274.0
150.00	184.0
152.70	127.0
153.90	101.0
154.90	353.0
155.60	116.0
157.00	240.0
158.90	205.0
160.80	172.0
171.00	122.0
172.00	540.0
172.90	1143.0
173.90	105304.0
174.90	8010.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

175.90	100888.0
176.90	6742.0
177.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
35.90	1280.0
37.00	6227.0
38.00	5449.0
39.00	2274.0
40.00	591.0
40.90	179.0
42.90	186.0
43.90	1099.0
45.00	1197.0
46.00	180.0
47.00	1643.0
47.80	1002.0
49.00	5550.0
50.00	25744.0
51.00	8302.0
51.90	330.0
54.90	385.0
56.00	1874.0
57.00	3448.0
57.90	267.0
58.80	122.0
60.00	1153.0
61.00	6477.0
62.00	6448.0
63.00	4617.0
63.90	453.0
64.90	280.0
66.90	436.0
68.00	14373.0
69.00	14216.0
70.00	1222.0
71.90	788.0
73.00	6413.0
74.00	23448.0
75.00	72240.0
76.00	6177.0
77.00	900.0
77.80	513.0
78.90	3444.0
79.90	1184.0
80.90	3673.0
81.90	739.0
82.90	128.0
85.90	295.0
86.90	6541.0
87.90	6480.0
91.00	593.0
92.00	4214.0
93.00	5975.0
94.00	16944.0
95.00	156416.0
96.00	10406.0
96.90	304.0
102.90	137.0
103.70	621.0
104.80	287.0
105.90	645.0
107.00	148.0
109.80	123.0
110.90	181.0
111.80	157.0
112.80	196.0
114.80	189.0
115.80	522.0
116.90	884.0
117.90	534.0
118.90	794.0
127.90	508.0
128.80	237.0
129.80	483.0
130.90	249.0
134.80	284.0
136.90	261.0
139.70	117.0
140.90	1337.0
141.80	192.0
142.90	1255.0
145.00	139.0
145.90	187.0
147.00	144.0
147.90	311.0
148.80	115.0
150.00	191.0
152.70	126.0
153.80	114.0
154.90	362.0
155.60	105.0
157.00	228.0
158.80	221.0
160.90	145.0
170.50	106.0
171.10	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

172.00	503.0
172.90	1174.0
173.90	108672.0
174.90	7911.0
175.90	105344.0
176.90	6788.0
177.80	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	1124.0
37.00	5468.0
38.00	4911.0
39.00	2214.0
40.00	566.0
41.00	161.0
42.90	229.0
43.90	1018.0
45.00	1069.0
46.10	170.0
47.00	1637.0
47.80	876.0
49.00	4868.0
50.00	22984.0
51.00	7494.0
51.90	338.0
52.10	297.0
54.90	377.0
56.00	1782.0
57.00	3120.0
58.00	239.0
58.80	128.0
60.00	1099.0
61.00	5870.0
62.00	5785.0
63.00	4043.0
63.90	425.0
64.90	257.0
67.00	378.0
68.00	12863.0
69.00	12674.0
70.00	1054.0
71.90	729.0
73.00	5797.0
74.00	20800.0
75.00	65896.0
76.00	5629.0
77.00	918.0
77.80	528.0
78.90	3159.0
79.90	1049.0
80.90	3392.0
81.90	785.0
82.90	120.0
85.90	218.0
86.90	5859.0
87.90	5881.0
91.00	519.0
92.00	3731.0
93.00	5308.0
94.00	15499.0
95.00	142464.0
96.00	9447.0
97.00	253.0
102.80	138.0
103.80	530.0
104.80	218.0
105.90	558.0
107.00	148.0
109.80	115.0
110.90	151.0
111.80	147.0
112.80	174.0
114.90	183.0
115.80	508.0
116.90	826.0
117.90	489.0
118.90	736.0
127.90	436.0
128.90	173.0
129.80	419.0
130.90	221.0
134.80	246.0
136.80	266.0
139.70	128.0
140.90	1151.0
141.80	198.0
142.90	1232.0
145.00	147.0
145.90	195.0
147.00	124.0
147.90	302.0
148.80	132.0
150.00	172.0
153.80	108.0
154.90	302.0
157.00	202.0
158.70	210.0
161.00	133.0
170.50	116.0
171.90	408.0
173.00	1185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

173.90	101320.0
174.90	7275.0
175.90	100216.0
176.90	6241.0
177.80	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

Scan 2793 (10.071 min): VV014430.D
BFB36

m/z	Abundance
35.70	106.0
36.70	103.0
38.80	128.0
40.00	374.0
42.20	106.0
44.00	539.0
56.00	119.0
69.20	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36