

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013021\
 Data File : VV020218.D
 Acq On : 29 Jan 2021 10:13
 Operator : SY/MD
 Sample : VV0130WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK703

Quant Time: Jan 30 02:27:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 30 02:26:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	437752	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.858	117	426751	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.257	152	219496	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.306	65	133732	4.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.20%
7) Chloroethane-d5	1.566	69	120835	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.106	63	168213	3.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.80%
20) 2-Butanone-d5	3.933	46	289798	45.60	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.20%
24) Chloroform-d	4.354	84	270233	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
26) 1,2-Dichloroethane-d4	5.039	65	139930	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
32) Benzene-d6	5.055	84	519384	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
36) 1,2-Dichloropropane-d6	6.074	67	157165	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.318	98	460798	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloroprop...	7.627	79	53499	4.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.60%
46) 2-Hexanone-d5	8.096	63	219477	42.37	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.74%
56) 1,1,2,2-Tetrachloroeth...	10.222	84	105740	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
66) 1,2-Dichlorobenzene-d4	11.630	152	185802	4.86	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.20%
Target Compounds						Qvalue
16) Methylene chloride	2.511	84	3969	0.12	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013021\
Data File : VV020218.D
Acq On : 29 Jan 2021 10:13
Operator : SY/MD
Sample : VV0130WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK703


Quant Time: Jan 30 02:27:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jan 30 02:26:26 2021
Response via : Initial Calibration

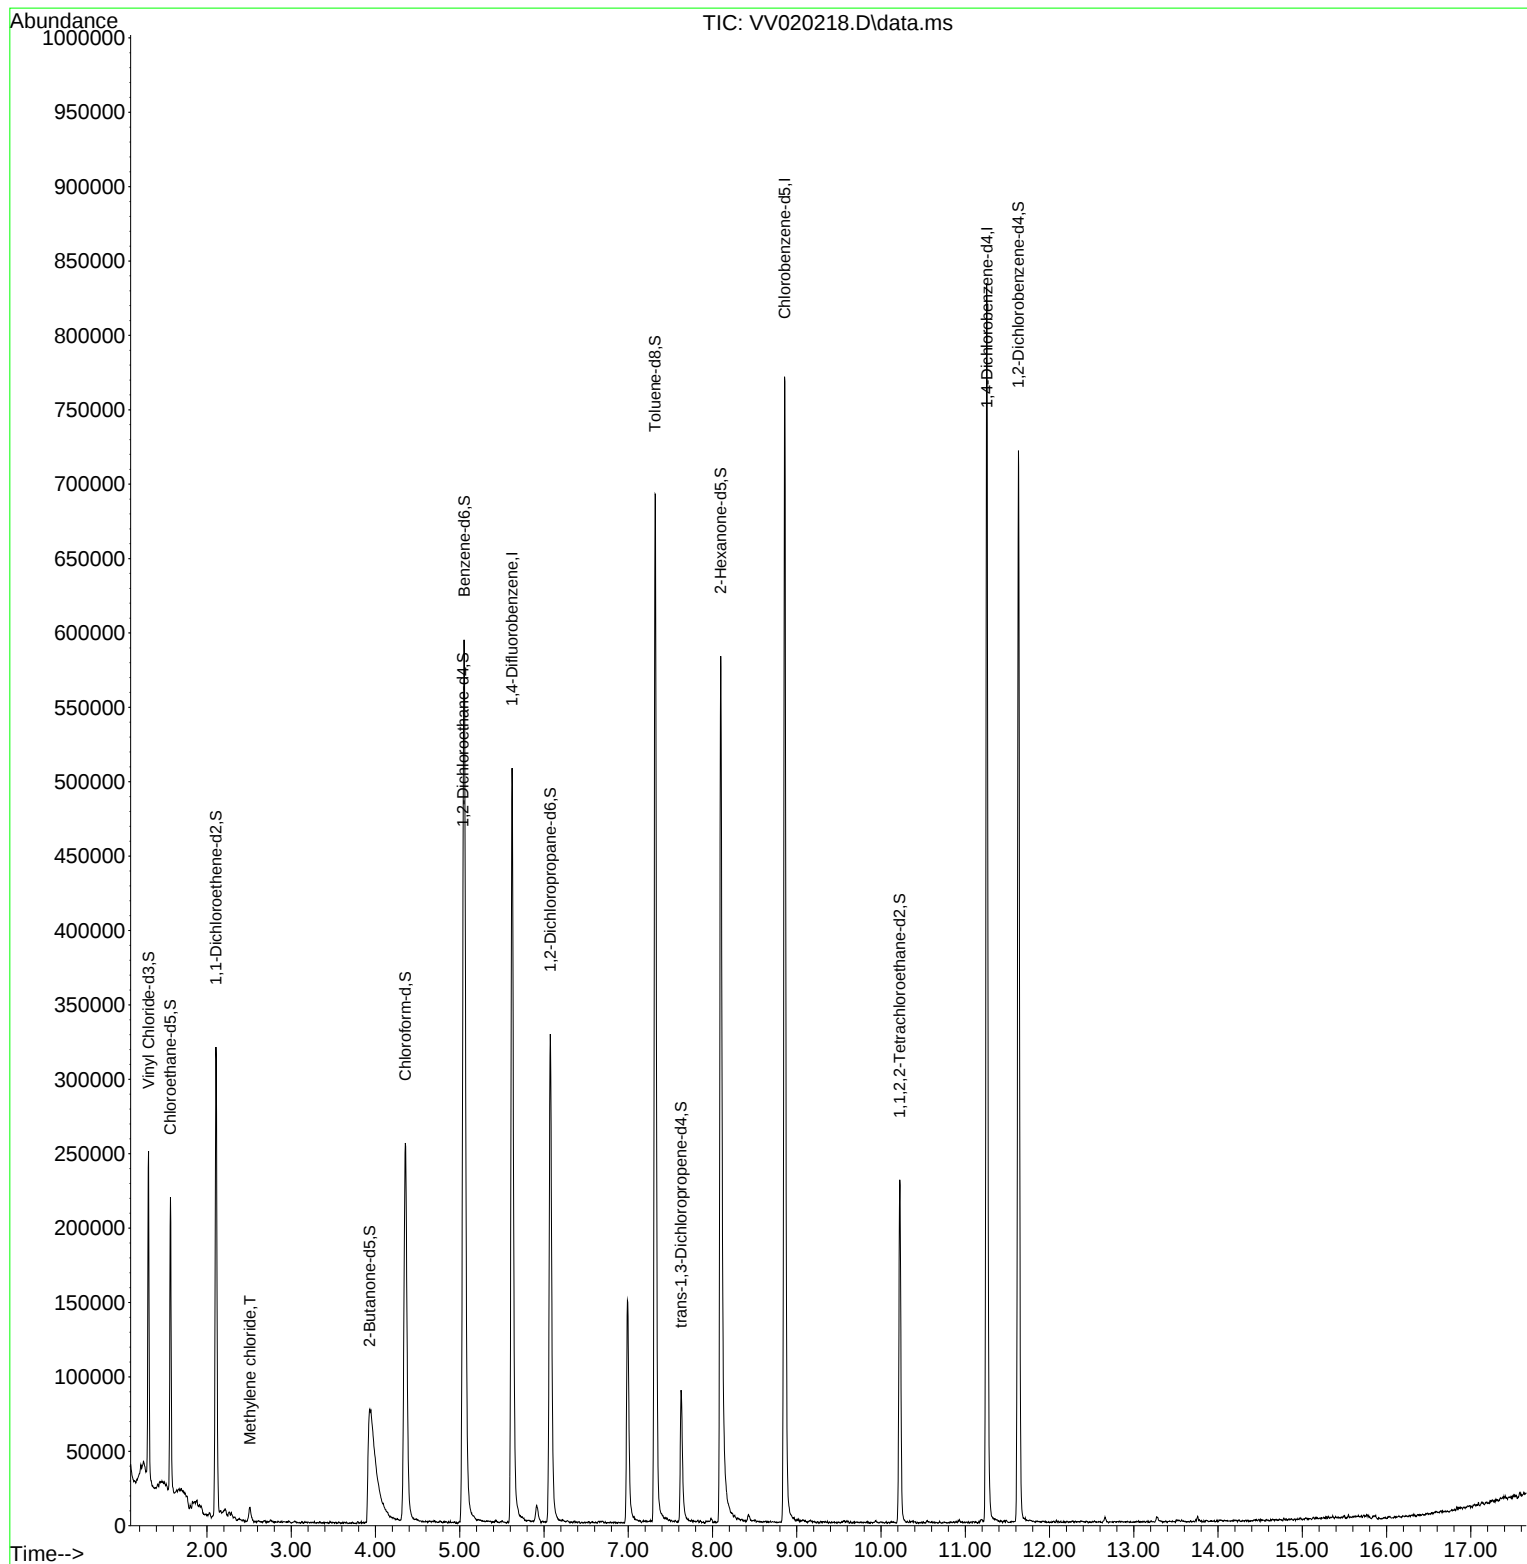

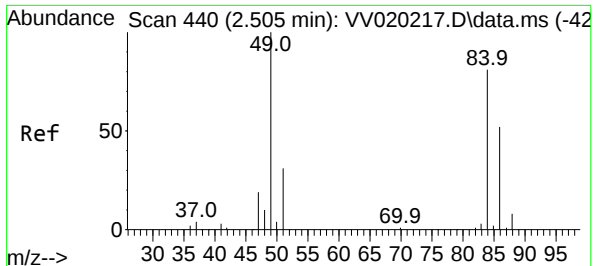

#16
Methylene chloride
Concen: 0.12 ug/L
RT: 2.511 min Scan# 442
Delta R.T. 0.006 min
Lab File: VV020218.D
Acq: 29 Jan 2021 10:13

Instrument :
MSVOA_V
ClientSampleId :
VBLK703

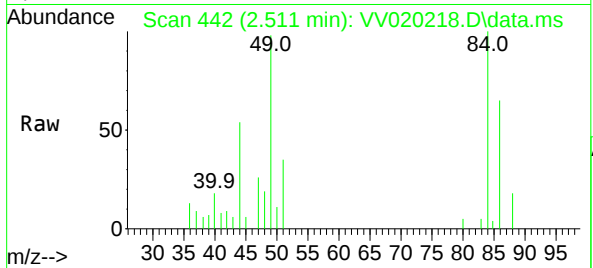

Tgt Ion:	84	Resp:	3969
Ion	Ratio	Lower	Upper
84	100		
86	65.4	42.8	79.4
49	98.4	93.9	174.3

