

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029982.D
 Acq On : 30 Jan 2023 11:30
 Operator : SY/MD
 Sample : VV0130WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jan 31 02:17:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 31 02:16:13 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	491441	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	458178	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	253897	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	173309	50.611	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 101.220%	
7) Chloroethane-d5	1.561	69	156941	54.481	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 108.960%	
11) 1,1-Dichloroethene-d2	2.102	63	236327	38.836	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 77.680%	
21) 2-Butanone-d5	3.860	46	225851	113.185	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 113.190%	
24) Chloroform-d	4.330	84	307654	48.322	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 96.640%	
26) 1,2-Dichloroethane-d4	5.015	65	182671	51.248	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 102.500%	
32) Benzene-d6	5.034	84	661122	53.934	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 107.860%	
36) 1,2-Dichloropropane-d6	6.053	67	217285	57.586	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 115.180%	
41) Toluene-d8	7.304	98	568065	50.568	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 101.140%	
43) trans-1,3-Dichloroprop...	7.606	79	93144	55.575	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 111.160%	
47) 2-Hexanone-d5	8.076	63	180302	111.133	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	= 111.130%	
56) 1,1,2,2-Tetrachloroeth...	10.201	84	288263	49.368	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 98.740%	
66) 1,2-Dichlorobenzene-d4	11.609	152	228161	50.434	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 100.860%	
Target Compounds						
61) 1,2,3-Trichloropropane	11.233	75	30224	7.310	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029982.D
Acq On : 30 Jan 2023 11:30
Operator : SY/MD
Sample : VV0130WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jan 31 02:17:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 31 02:16:13 2023
Response via : Initial Calibration

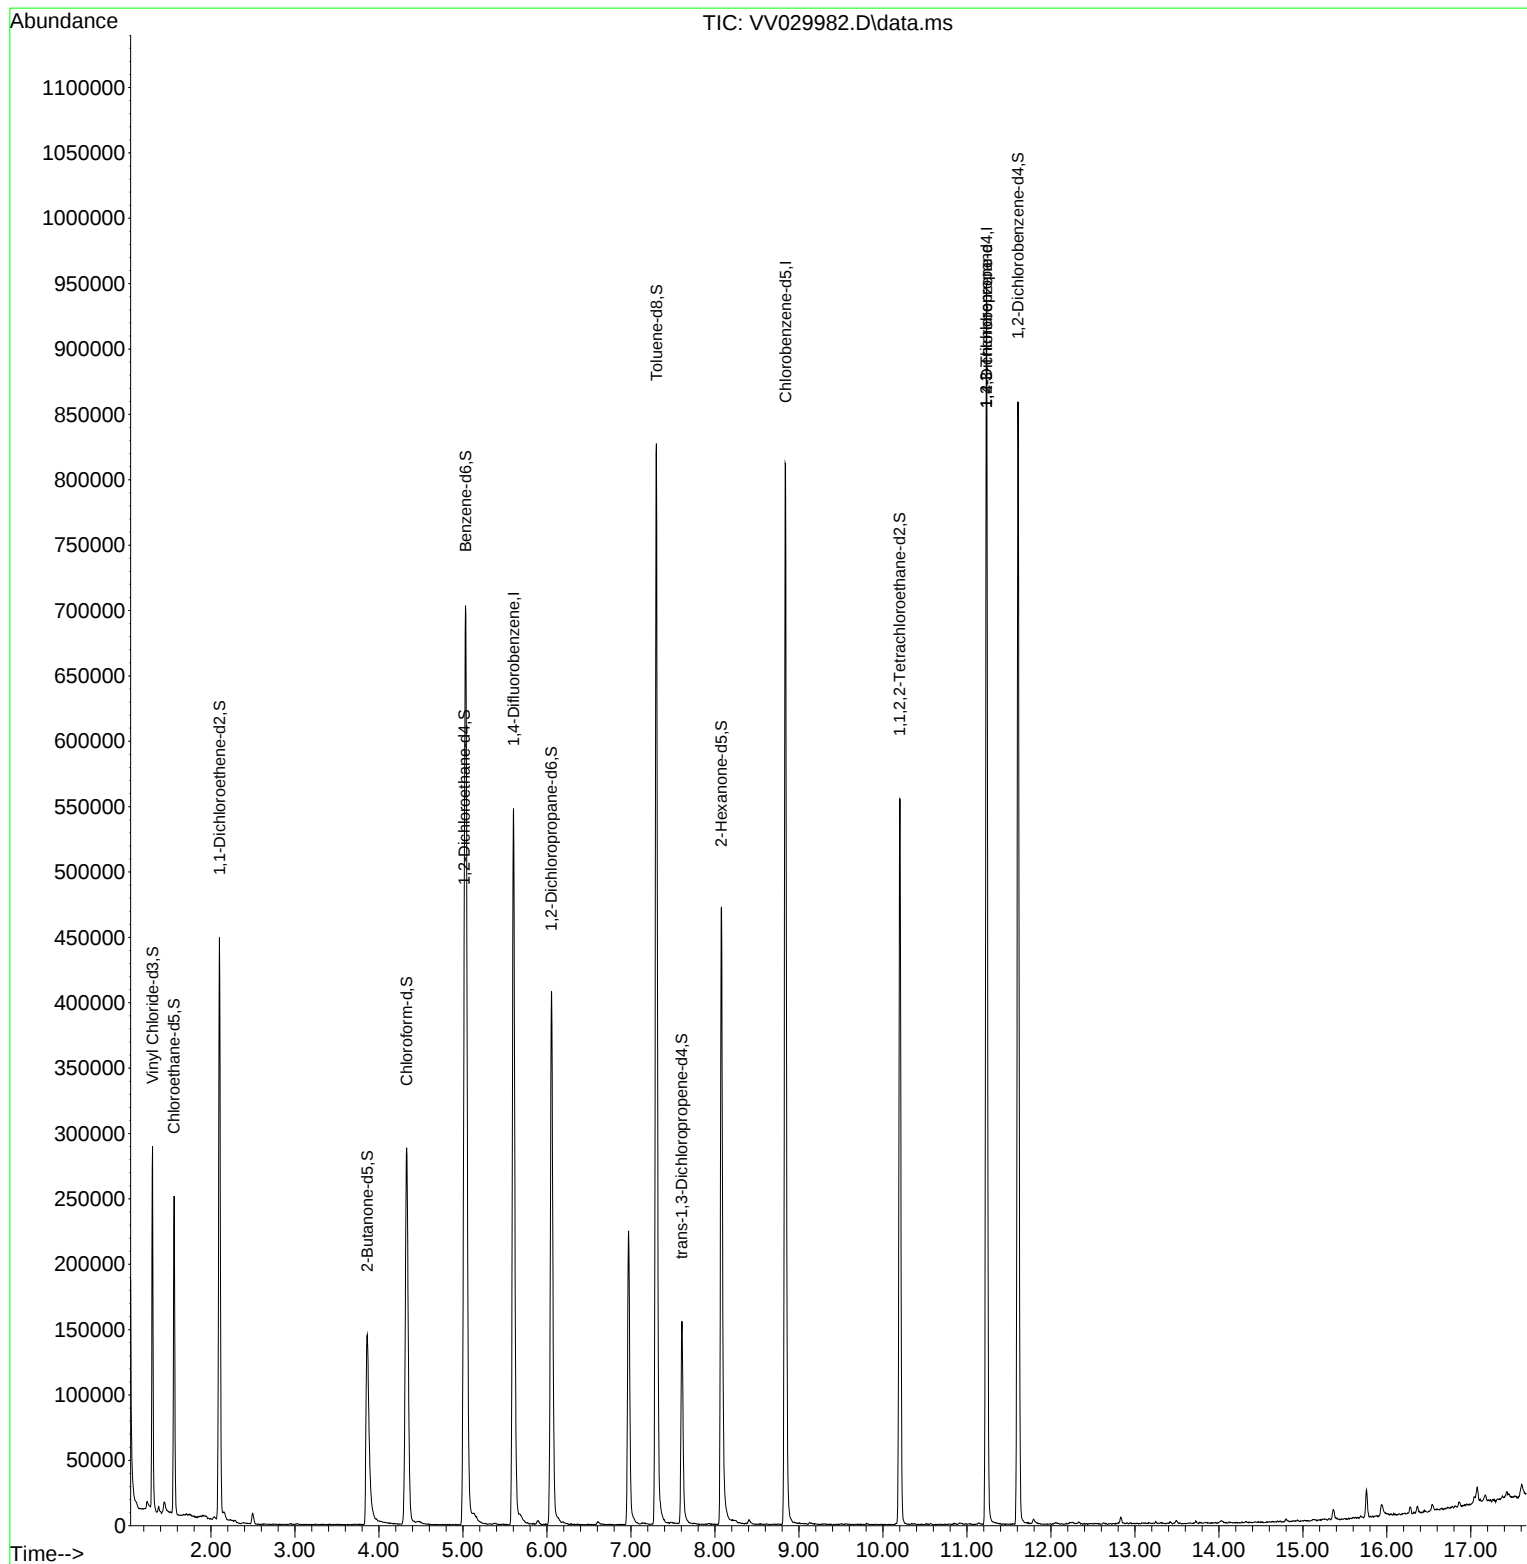

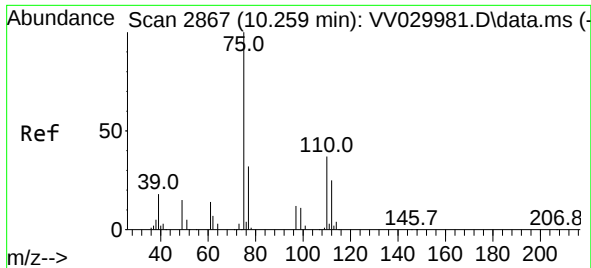

#61
 1,2,3-Trichloropropane
 Concen: 7.310 ug/L
 RT: 11.233 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV029982.D
 Acq: 30 Jan 2023 11:30

Instrument :
 MSVOA_V
 ClientSampleId :

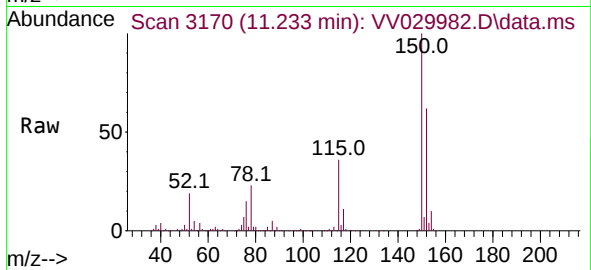

Tgt Ion: 75 Resp: 30224
 Ion Ratio Lower Upper
 75 100
 77 31.2 25.9 38.9
 110 2.3 32.3 48.5#

