

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013023\
 Data File : VW029996.D
 Acq On : 30 Jan 2023 16:59
 Operator : SY/MD
 Sample : 01314-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jan 31 02:20:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 31 02:16:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	491805	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	471014	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	252885	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	149778	43.707	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.420%
7) Chloroethane-d5	1.561	69	140309	48.671	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.340%
11) 1,1-Dichloroethene-d2	2.101	63	209301	34.369	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.740%
21) 2-Butanone-d5	3.866	46	222715	111.531	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.530%
24) Chloroform-d	4.336	84	280314	43.995	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	5.021	65	170243	47.726	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.460%
32) Benzene-d6	5.040	84	594274	47.159	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.320%
36) 1,2-Dichloropropane-d6	6.059	67	201873	52.043	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.080%
41) Toluene-d8	7.307	98	514828	44.580	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.160%
43) trans-1,3-Dichloroprop...	7.609	79	82996	48.171	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.340%
47) 2-Hexanone-d5	8.082	63	179697	107.742	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.740%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	285982	47.642	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.280%
66) 1,2-Dichlorobenzene-d4	11.612	152	211167	46.864	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.720%
Target Compounds						
61) 1,2,3-Trichloropropane	11.236	75	30205	7.334	ug/L	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029996.D
Acq On : 30 Jan 2023 16:59
Operator : SY/MD
Sample : 01314-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jan 31 02:20:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 31 02:16:13 2023
Response via : Initial Calibration

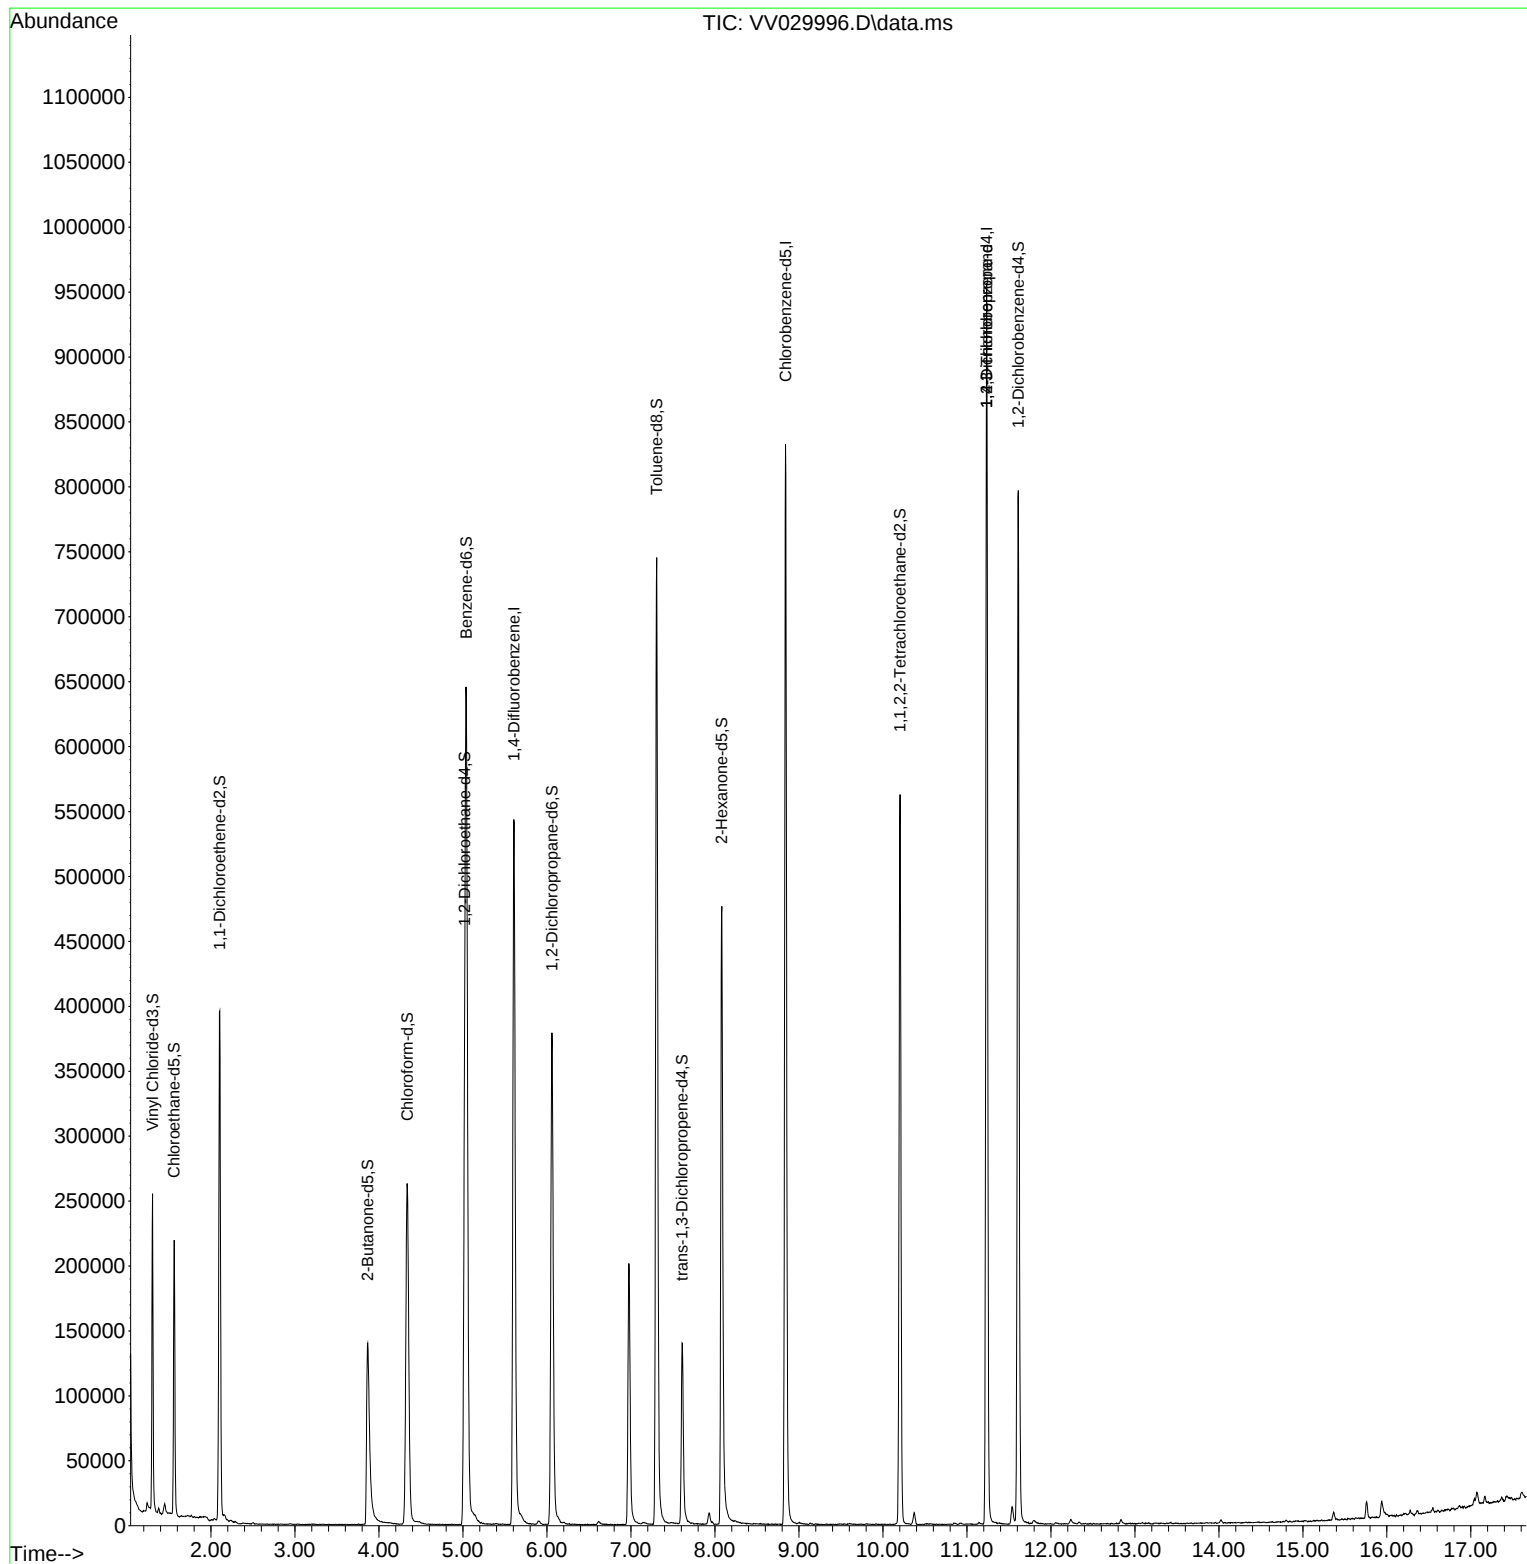

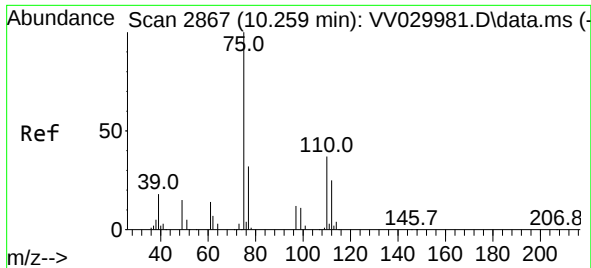

#61

1,2,3-Trichloropropane

Concen: 7.334 ug/L

RT: 11.236 min Scan# 31

Delta R.T. 0.977 min


Lab File: VV029996.D

Acq: 30 Jan 2023 16:59

Instrument :

MSVOA_V

ClientSampleId :

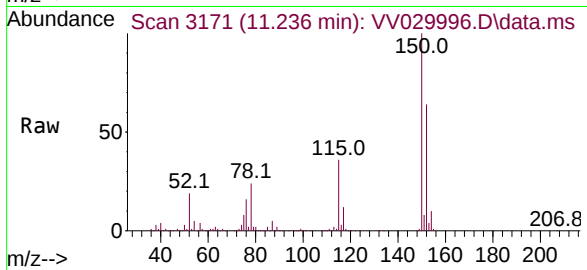

Tgt Ion: 75 Resp: 30205

Ion Ratio Lower Upper

75 100

77 30.2 25.9 38.9

110 2.1 32.3 48.5#

