




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029987.D
 Acq On : 30 Jan 2023 13:27
 Operator : SY/MD
 Sample : 01314-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L5

Manual IntegrationsAPPROVED

Quant Time: Jan 31 02:18:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 31 02:16:13 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/31/2023
 Supervised By :Mahesh Dadoda 01/31/2023

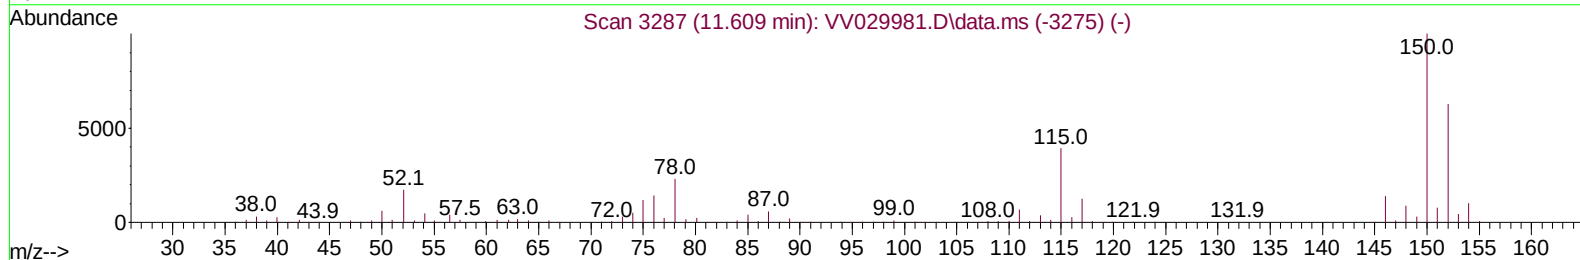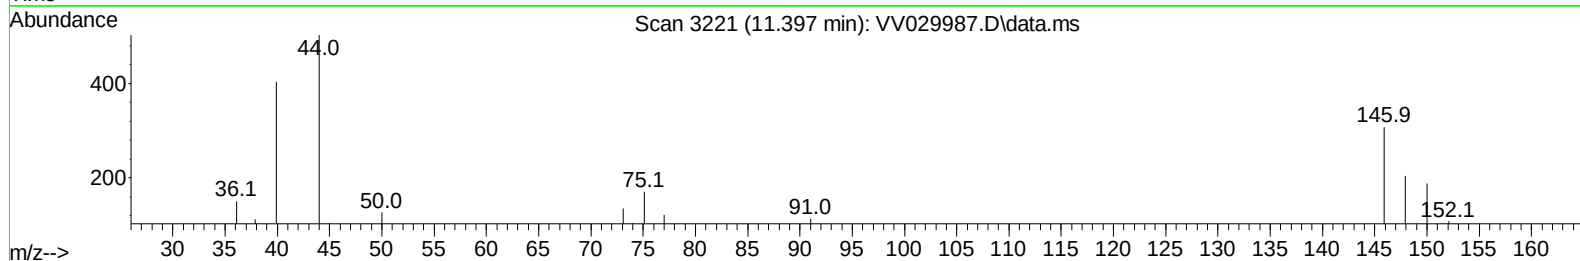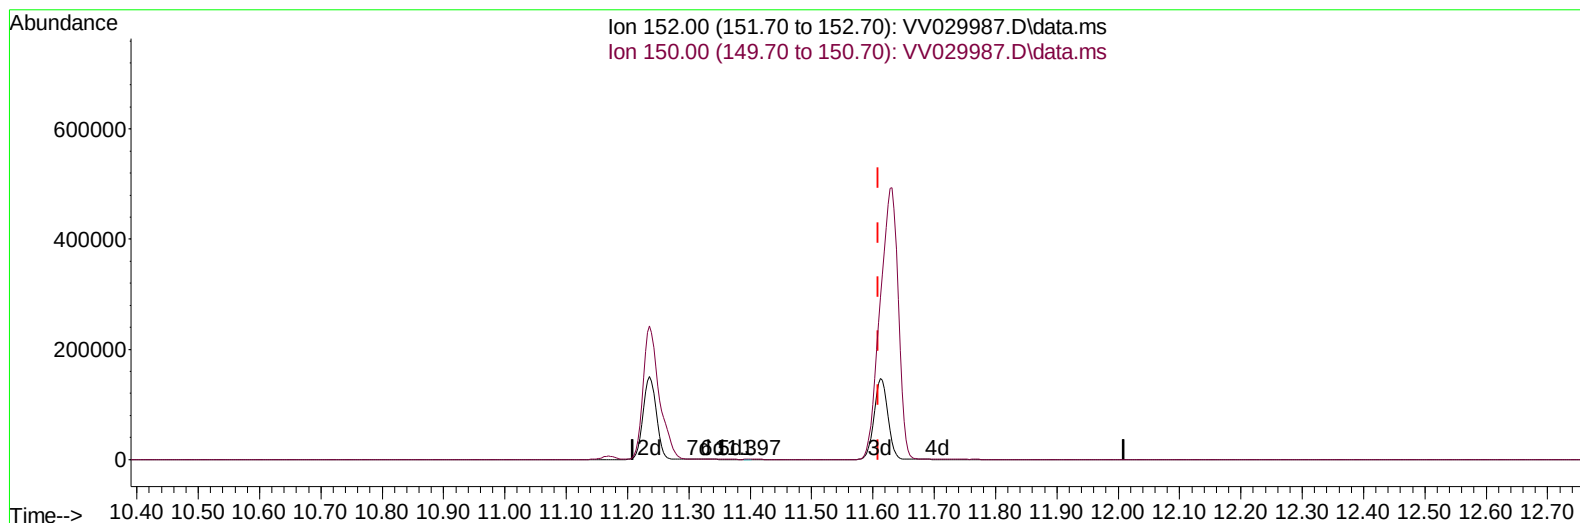

TIC: VV029987.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.397min (-0.212) 0.01 ug/L

response 41

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	174.20	141.46
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029987.D
 Acq On : 30 Jan 2023 13:27
 Operator : SY/MD
 Sample : 01314-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L5

Manual IntegrationsAPPROVED

Quant Time: Jan 31 02:18:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 31 02:16:13 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/31/2023
 Supervised By :Mahesh Dadoda 01/31/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	417488	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	404960	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	224919	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	162424	55.834	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	111.660%	
7) Chloroethane-d5	1.561	69	151539	61.924	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	123.840%	
11) 1,1-Dichloroethene-d2	2.101	63	228571	44.215	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	88.420%	
21) 2-Butanone-d5	3.863	46	213978	126.231	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	126.230%	
24) Chloroform-d	4.336	84	292353	54.052	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.100%	
26) 1,2-Dichloroethane-d4	5.018	65	174669	57.684	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	115.360%	
32) Benzene-d6	5.040	84	636553	58.754	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	117.500%	
36) 1,2-Dichloropropane-d6	6.059	67	210824	63.216	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	126.440%#	
41) Toluene-d8	7.307	98	546880	55.080	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	110.160%	
43) trans-1,3-Dichloroprop...	7.609	79	89322	60.299	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	120.600%	
47) 2-Hexanone-d5	8.079	63	174640	121.789	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	121.790%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	283768	54.984	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	109.960%	
66) 1,2-Dichlorobenzene-d4	11.612	152	232656m	58.054	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	116.100%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.240	50	5392	1.772	ug/L	99
5) Vinyl chloride	1.307	62	15068	4.303	ug/L	85
20) cis-1,2-Dichloroethene	3.902	96	66715	20.276	ug/L	94
33) Benzene	5.095	78	17055	1.401	ug/L	100
34) Trichloroethene	5.902	95	591770	193.123	ug/L	95
51) Chlorobenzene	8.870	112	170102	19.047	ug/L	97
64) 1,3-Dichlorobenzene	11.169	146	88887	13.113	ug/L	97
65) 1,4-Dichlorobenzene	11.259	146	851542	121.257	ug/L	99
67) 1,2-Dichlorobenzene	11.632	146	6204678	909.264	ug/L	97
70) 1,2,4-trichlorobenzene	13.246	180	45622	9.795	ug/L	97
72) 1,2,3-Trichlorobenzene	13.728	180	8227	1.812	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029987.D
Acq On : 30 Jan 2023 13:27
Operator : SY/MD
Sample : 01314-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L5

Manual IntegrationsAPPROVED

Quant Time: Jan 31 02:18:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 31 02:16:13 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 01/31/2023
Supervised By :Mahesh Dadoda 01/31/2023

