

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029983.D
 Acq On : 30 Jan 2023 11:54
 Operator : SY/MD
 Sample : 01314-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	278281	282497	15.33%	1.935%
2	1.561	156	162	179	rVB	240219	278695	15.13%	1.909%
3	2.105	321	331	343	rBV	441149	633979	34.41%	4.342%
4	2.860	563	566	569	rBV	278	183	0.01%	0.001%
5	2.989	602	606	609	rBV	240	232	0.01%	0.002%
6	3.198	668	671	675	rBV2	363	272	0.01%	0.002%
7	3.288	697	699	701	rBV	230	92	0.00%	0.001%
8	3.304	701	704	706	rBV2	321	196	0.01%	0.001%
9	3.355	716	720	721	rBV	178	145	0.01%	0.001%
10	3.420	737	740	744	rBV3	310	225	0.01%	0.002%
11	3.439	744	746	748	rBV2	215	114	0.01%	0.001%
12	3.455	748	751	753	rVB2	360	153	0.01%	0.001%
13	3.468	753	755	757	rVB	177	71	0.00%	0.000%
14	3.484	757	760	763	rBV	281	203	0.01%	0.001%
15	3.603	793	797	800	rBV2	339	289	0.02%	0.002%
16	3.667	814	817	819	rBV2	291	207	0.01%	0.001%
17	3.732	834	837	843	rVB3	424	416	0.02%	0.003%
18	3.777	848	851	854	rBV	350	226	0.01%	0.002%
19	3.863	867	878	913	rBV	160977	440830	23.93%	3.019%
20	4.336	1010	1025	1059	rVB	288497	700278	38.01%	4.796%
21	4.760	1154	1157	1160	rVB2	389	264	0.01%	0.002%
22	4.825	1176	1177	1181	rVB2	150	65	0.00%	0.000%
23	4.850	1181	1185	1187	rBV	271	150	0.01%	0.001%
24	4.860	1187	1188	1189	rBV	120	36	0.00%	0.000%
25	4.892	1195	1198	1201	rVB	268	136	0.01%	0.001%
26	4.934	1206	1211	1214	rBV3	348	288	0.02%	0.002%
27	4.960	1217	1219	1224	rBV2	197	151	0.01%	0.001%
28	5.037	1224	1243	1271	rBV2	706301	1842173	100.00%	12.615%
29	5.339	1335	1337	1340	rBV2	460	235	0.01%	0.002%
30	5.539	1398	1399	1401	rBV2	197	63	0.00%	0.000%
31	5.555	1401	1404	1406	rBV2	511	265	0.01%	0.002%
32	5.606	1406	1420	1442	rBV	550304	1095561	59.47%	7.502%
33	5.899	1502	1511	1520	rVB6	2112	4140	0.22%	0.028%
34	5.969	1529	1533	1536	rBV2	460	350	0.02%	0.002%
35	6.059	1546	1561	1587	rBV	416511	846388	45.95%	5.796%
36	6.288	1627	1632	1634	rBV4	569	482	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029983.D
 Acq On : 30 Jan 2023 11:54
 Operator : SY/MD
 Sample : 01314-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	6.301	1634	1636	1640	rBV3	458	342	0.02%	0.002%
38	6.423	1671	1674	1675	rBV2	245	116	0.01%	0.001%
39	6.465	1685	1687	1688	rBV	135	58	0.00%	0.000%
40	6.481	1688	1692	1693	rVV	335	202	0.01%	0.001%
41	6.503	1697	1699	1702	rVB	508	219	0.01%	0.001%
42	6.529	1705	1707	1709	rVB	110	44	0.00%	0.000%
43	6.539	1709	1710	1712	rBV	194	62	0.00%	0.000%
44	6.612	1721	1733	1742	rBV5	2492	5763	0.31%	0.039%
45	6.719	1764	1766	1769	rVB2	273	112	0.01%	0.001%
46	6.735	1769	1771	1772	rVV	138	35	0.00%	0.000%
47	6.744	1772	1774	1777	rVB2	247	156	0.01%	0.001%
48	6.764	1777	1780	1783	rVB	267	131	0.01%	0.001%
49	6.776	1783	1784	1786	rVB	144	54	0.00%	0.000%
50	6.799	1786	1791	1795	rVB3	371	266	0.01%	0.002%
51	6.821	1795	1798	1799	rBV	125	80	0.00%	0.001%
52	6.828	1799	1800	1802	rVB	192	51	0.00%	0.000%
53	6.857	1807	1809	1812	rVB2	201	115	0.01%	0.001%
54	6.873	1812	1814	1815	rBV2	217	82	0.00%	0.001%
55	6.976	1834	1846	1871	rBV	221999	409153	22.21%	2.802%
56	7.307	1936	1949	1967	rBV	844071	1462993	79.42%	10.019%
57	7.609	2033	2043	2068	rBV	158290	274974	14.93%	1.883%
58	7.847	2113	2117	2119	rBV2	642	459	0.02%	0.003%
59	7.870	2122	2124	2126	rBV2	458	191	0.01%	0.001%
60	7.931	2128	2143	2163	rBV2	54917	106152	5.76%	0.727%
61	8.079	2178	2189	2223	rBV	527832	905531	49.16%	6.201%
62	8.481	2313	2314	2317	rBV3	446	317	0.02%	0.002%
63	8.764	2398	2402	2404	rBV2	403	302	0.02%	0.002%
64	8.841	2414	2426	2453	rBV	841823	1353676	73.48%	9.270%
65	9.098	2505	2506	2507	rBV	279	104	0.01%	0.001%
66	9.130	2508	2516	2522	rVV3	3713	5182	0.28%	0.035%
67	9.297	2566	2568	2570	rBV2	314	173	0.01%	0.001%
68	9.326	2576	2577	2579	rVB	290	90	0.00%	0.001%
69	9.339	2579	2581	2588	rBV2	314	272	0.01%	0.002%
70	9.371	2588	2591	2593	rBV2	299	195	0.01%	0.001%
71	9.432	2608	2610	2611	rBV	168	57	0.00%	0.000%
72	9.477	2621	2624	2625	rBV	173	86	0.00%	0.001%
73	9.490	2625	2628	2630	rBV2	579	332	0.02%	0.002%
74	9.551	2635	2647	2658	rVV8	6430	12709	0.69%	0.087%
75	9.641	2672	2675	2677	rBV2	337	251	0.01%	0.002%
76	9.690	2684	2690	2691	rBV4	886	769	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029983.D
 Acq On : 30 Jan 2023 11:54
 Operator : SY/MD
 Sample : 01314-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	9.805	2719	2726	2736	rBV6	1586	2321	0.13%	0.016%
78	9.876	2745	2748	2750	rBV2	179	110	0.01%	0.001%
79	9.892	2750	2753	2755	rBV2	251	162	0.01%	0.001%
80	9.966	2772	2776	2777	rBV	486	324	0.02%	0.002%
81	10.040	2797	2799	2800	rBV	269	73	0.00%	0.000%
82	10.069	2805	2808	2809	rBV	384	164	0.01%	0.001%
83	10.204	2838	2850	2876	rVB	599281	929559	50.46%	6.366%
84	10.371	2890	2902	2916	rVB	54906	93273	5.06%	0.639%
85	10.567	2957	2963	2965	rBV2	683	531	0.03%	0.004%
86	10.731	3012	3014	3015	rBV2	311	121	0.01%	0.001%
87	10.792	3028	3033	3036	rBV3	327	299	0.02%	0.002%
88	10.837	3043	3047	3051	rBV4	1728	1907	0.10%	0.013%
89	10.902	3064	3067	3071	rBV4	900	914	0.05%	0.006%
90	11.098	3125	3128	3130	rBV	310	244	0.01%	0.002%
91	11.143	3135	3142	3149	rBV7	1959	3482	0.19%	0.024%
92	11.236	3158	3171	3195	rBV	959427	1461946	79.36%	10.011%
93	11.535	3255	3264	3275	rBV	22655	40849	2.22%	0.280%
94	11.609	3276	3287	3309	rVB	870575	1357105	73.67%	9.294%
95	11.979	3401	3402	3406	rVB2	472	233	0.01%	0.002%
96	12.062	3421	3428	3434	rBV5	1406	2479	0.13%	0.017%
97	12.239	3475	3483	3494	rVB2	17189	27251	1.48%	0.187%
98	12.336	3506	3513	3520	rVB6	4891	7256	0.39%	0.050%
99	12.474	3553	3556	3558	rBV2	370	214	0.01%	0.001%




Sum of corrected areas: 14602723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029983.D
Acq On : 30 Jan 2023 11:54
Operator : SY/MD
Sample : 01314-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

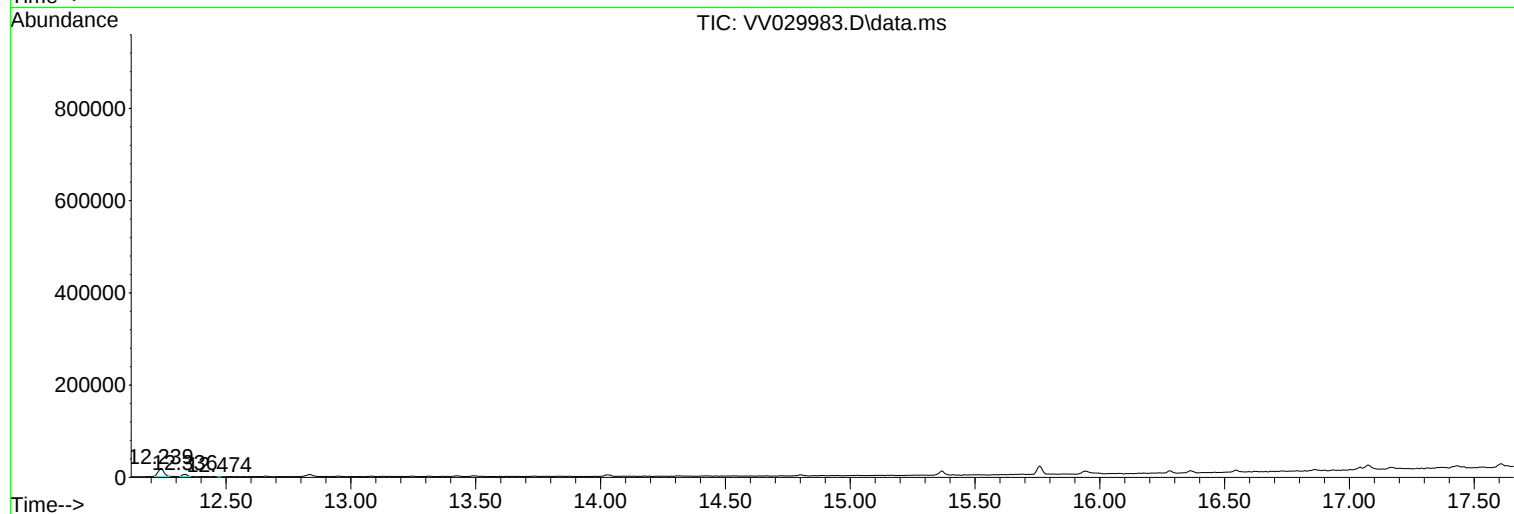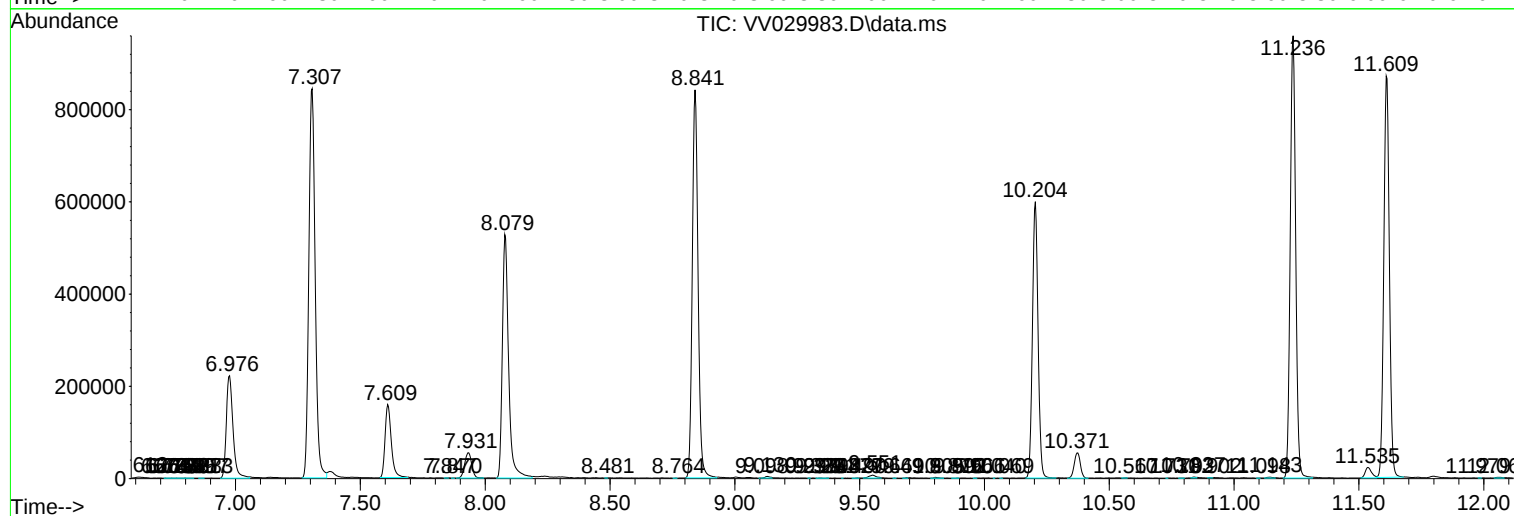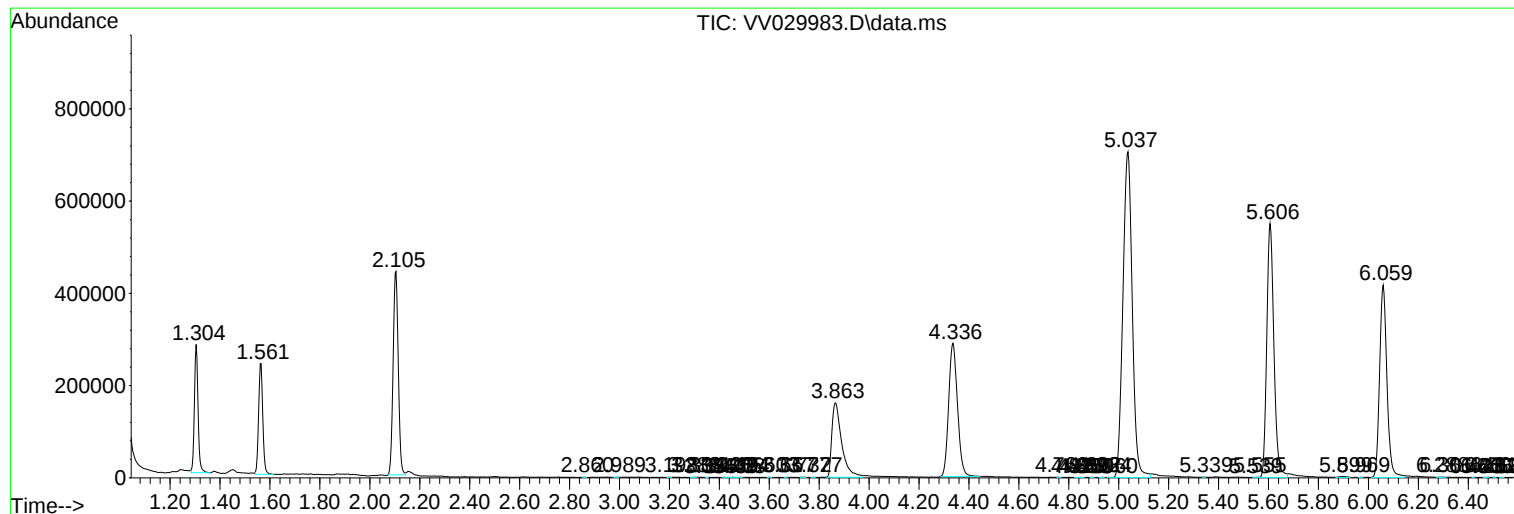

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029983.D
Acq On : 30 Jan 2023 11:54
Operator : SY/MD
Sample : 01314-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029983.D
Acq On : 30 Jan 2023 11:54
Operator : SY/MD
Sample : 01314-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc