

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029984.D
 Acq On : 30 Jan 2023 12:18
 Operator : SY/MD
 Sample : 01314-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	277933	276338	15.04%	1.957%
2	1.561	155	162	175	rVB	241806	275450	15.00%	1.951%
3	2.101	321	330	345	rBV	443518	625333	34.05%	4.428%
4	2.806	547	549	551	rBV	258	111	0.01%	0.001%
5	2.944	586	592	593	rBV4	658	641	0.03%	0.005%
6	3.002	607	610	614	rBV4	372	288	0.02%	0.002%
7	3.127	647	649	651	rBV2	407	229	0.01%	0.002%
8	3.214	675	676	679	rVB	273	97	0.01%	0.001%
9	3.230	679	681	683	rBV	282	152	0.01%	0.001%
10	3.256	688	689	690	rBV	201	65	0.00%	0.000%
11	3.281	695	697	700	rBV2	288	145	0.01%	0.001%
12	3.397	730	733	735	rBV	288	180	0.01%	0.001%
13	3.413	736	738	740	rVV2	363	146	0.01%	0.001%
14	3.436	742	745	747	rBV2	174	90	0.00%	0.001%
15	3.458	749	752	753	rBV2	233	108	0.01%	0.001%
16	3.494	759	763	766	rBV	255	214	0.01%	0.002%
17	3.558	781	783	786	rBV	250	184	0.01%	0.001%
18	3.619	799	802	806	rBV2	129	106	0.01%	0.001%
19	3.699	822	827	829	rBV2	278	250	0.01%	0.002%
20	3.818	860	864	865	rBV3	481	324	0.02%	0.002%
21	3.863	867	878	916	rBV	147449	395913	21.55%	2.804%
22	4.336	1009	1025	1050	rBV	287764	708181	38.56%	5.015%
23	4.686	1131	1134	1135	rBV	72	42	0.00%	0.000%
24	4.693	1135	1136	1138	rBV	234	89	0.00%	0.001%
25	4.728	1143	1147	1151	rBV3	389	330	0.02%	0.002%
26	4.773	1159	1161	1166	rVB2	201	111	0.01%	0.001%
27	4.838	1178	1181	1185	rBV2	302	269	0.01%	0.002%
28	4.908	1200	1203	1205	rBV2	134	93	0.01%	0.001%
29	4.928	1207	1209	1211	rBV2	137	38	0.00%	0.000%
30	4.957	1215	1218	1219	rBV	271	125	0.01%	0.001%
31	5.037	1223	1243	1270	rBV2	706679	1836782	100.00%	13.007%
32	5.452	1371	1372	1375	rBV2	451	221	0.01%	0.002%
33	5.471	1375	1378	1381	rVV3	654	449	0.02%	0.003%
34	5.513	1388	1391	1394	rBV	351	250	0.01%	0.002%
35	5.532	1394	1397	1402	rVB3	448	418	0.02%	0.003%
36	5.606	1405	1420	1459	rBV	539138	1101130	59.95%	7.797%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029984.D
 Acq On : 30 Jan 2023 12:18
 Operator : SY/MD
 Sample : 01314-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	5.973	1529	1534	1537	rBV2	509	476	0.03%	0.003%
38	6.059	1543	1561	1590	rBV	407594	844148	45.96%	5.978%
39	6.426	1673	1675	1677	rBV2	208	91	0.00%	0.001%
40	6.474	1688	1690	1693	rBV	265	121	0.01%	0.001%
41	6.535	1705	1709	1710	rBV	201	125	0.01%	0.001%
42	6.616	1725	1734	1741	rBV5	2144	3977	0.22%	0.028%
43	6.776	1782	1784	1785	rBV5	102	47	0.00%	0.000%
44	6.786	1785	1787	1789	rVV2	181	114	0.01%	0.001%
45	6.841	1800	1804	1806	rBV	249	181	0.01%	0.001%
46	6.886	1815	1818	1821	rBV	363	217	0.01%	0.002%
47	6.905	1821	1824	1825	rBV2	341	171	0.01%	0.001%
48	6.931	1830	1832	1834	rBV	145	65	0.00%	0.000%
49	6.976	1834	1846	1874	rBV	220497	406100	22.11%	2.876%
50	7.307	1935	1949	1980	rBV	827607	1455628	79.25%	10.308%
51	7.609	2033	2043	2070	rBV	154930	268046	14.59%	1.898%
52	7.931	2133	2143	2160	rVB2	21789	40045	2.18%	0.284%
53	7.995	2160	2163	2165	rBV2	560	311	0.02%	0.002%
54	8.079	2178	2189	2223	rBV	509034	875548	47.67%	6.200%
55	8.545	2331	2334	2339	rBV3	520	358	0.02%	0.003%
56	8.616	2354	2356	2357	rBV	359	184	0.01%	0.001%
57	8.744	2393	2396	2399	rBV3	715	477	0.03%	0.003%
58	8.783	2403	2408	2410	rBV2	308	180	0.01%	0.001%
59	8.841	2411	2426	2454	rBV	815517	1329269	72.37%	9.413%
60	9.198	2535	2537	2541	rVB3	512	304	0.02%	0.002%
61	9.294	2565	2567	2570	rBV2	292	233	0.01%	0.002%
62	9.342	2580	2582	2585	rBV2	353	183	0.01%	0.001%
63	9.387	2592	2596	2601	rVB2	841	510	0.03%	0.004%
64	9.410	2601	2603	2606	rBV	308	201	0.01%	0.001%
65	9.648	2674	2677	2679	rBV2	268	166	0.01%	0.001%
66	9.706	2691	2695	2696	rBV	670	494	0.03%	0.003%
67	9.805	2720	2726	2730	rBV4	1250	1302	0.07%	0.009%
68	9.857	2740	2742	2744	rBV2	457	221	0.01%	0.002%
69	9.911	2755	2759	2761	rBV	227	162	0.01%	0.001%
70	9.998	2781	2786	2788	rBV2	160	154	0.01%	0.001%
71	10.050	2801	2802	2803	rBV	103	25	0.00%	0.000%
72	10.062	2803	2806	2808	rBV2	152	101	0.01%	0.001%
73	10.075	2808	2810	2813	rBV2	198	127	0.01%	0.001%
74	10.120	2821	2824	2826	rBV	428	236	0.01%	0.002%
75	10.204	2831	2850	2867	rBV	577601	898361	48.91%	6.361%
76	10.371	2893	2902	2914	rVB2	19752	32537	1.77%	0.230%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029984.D
 Acq On : 30 Jan 2023 12:18
 Operator : SY/MD
 Sample : 01314-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	10.439	2921	2923	2925	rBV	301	146	0.01%	0.001%
78	10.477	2931	2935	2939	rBV2	591	417	0.02%	0.003%
79	10.509	2939	2945	2948	rBV2	883	955	0.05%	0.007%
80	10.635	2982	2984	2989	rVB2	319	195	0.01%	0.001%
81	10.664	2991	2993	2996	rBV2	372	204	0.01%	0.001%
82	10.812	3036	3039	3040	rBV	325	202	0.01%	0.001%
83	10.847	3045	3050	3053	rBV4	1044	1139	0.06%	0.008%
84	11.088	3123	3125	3129	rVB2	382	184	0.01%	0.001%
85	11.114	3129	3133	3136	rBV3	452	410	0.02%	0.003%
86	11.140	3137	3141	3142	rBV3	1349	920	0.05%	0.007%
87	11.236	3158	3171	3197	rBV	930597	1397445	76.08%	9.896%
88	11.541	3256	3266	3275	rBV3	11919	21103	1.15%	0.149%
89	11.609	3276	3287	3309	rVB	837148	1309995	71.32%	9.276%
90	11.995	3404	3407	3409	rBV3	547	344	0.02%	0.002%
91	12.185	3463	3466	3469	rBV3	609	476	0.03%	0.003%
92	12.442	3544	3546	3548	rBV	451	178	0.01%	0.001%
93	12.458	3549	3551	3555	rVB4	436	217	0.01%	0.002%
94	12.754	3641	3643	3645	rBV2	471	180	0.01%	0.001%
95	13.049	3730	3735	3738	rBV4	899	1057	0.06%	0.007%




Sum of corrected areas: 14121855

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029984.D
Acq On : 30 Jan 2023 12:18
Operator : SY/MD
Sample : 01314-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

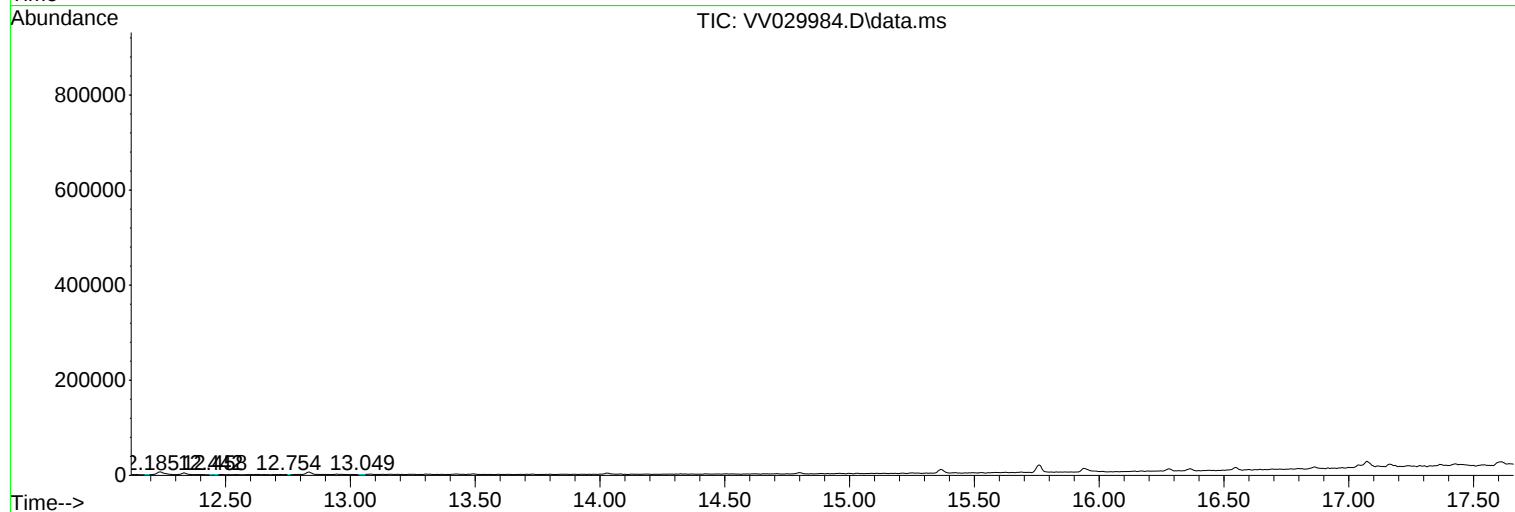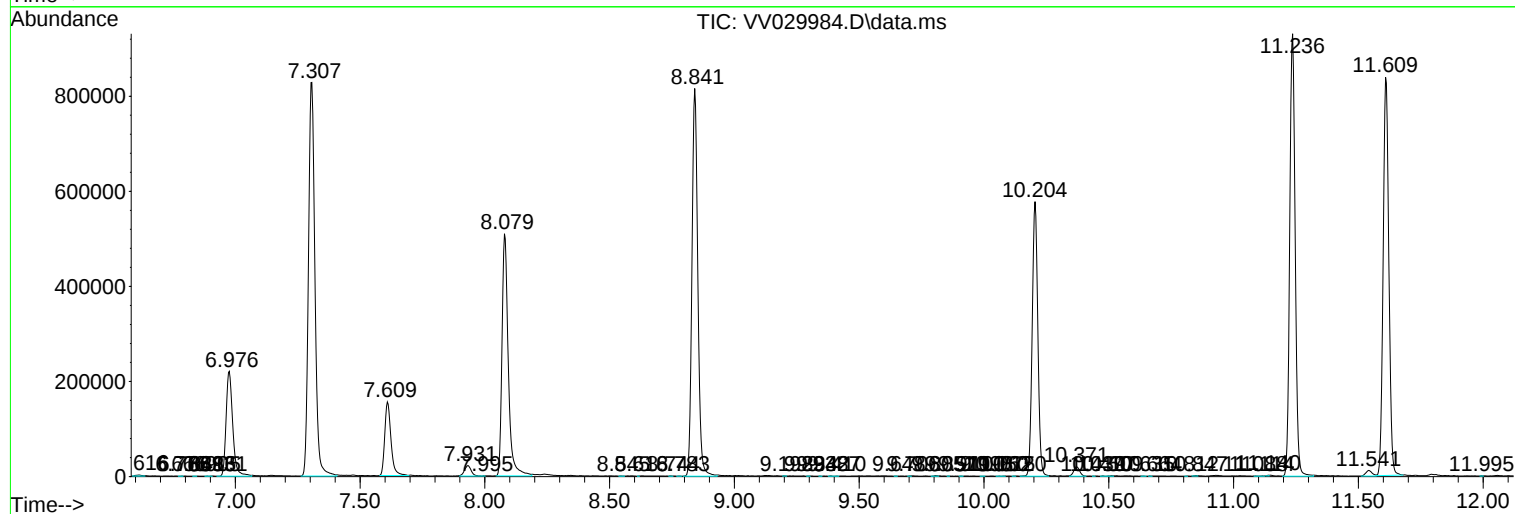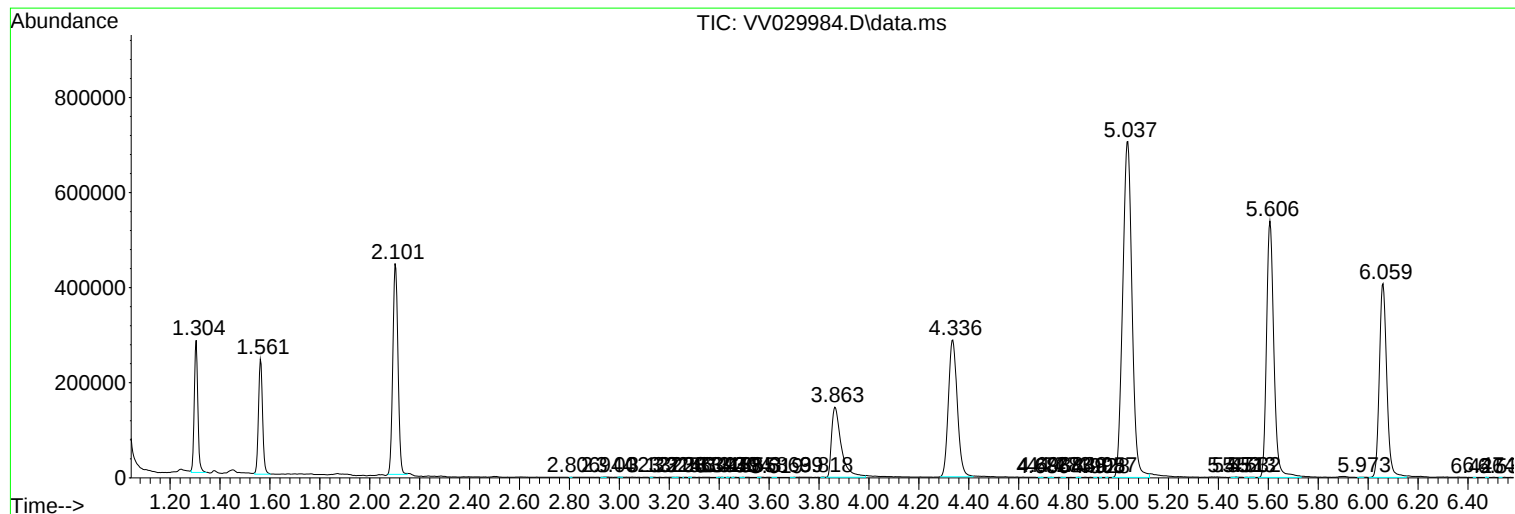

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029984.D
Acq On : 30 Jan 2023 12:18
Operator : SY/MD
Sample : 01314-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029984.D
Acq On : 30 Jan 2023 12:18
Operator : SY/MD
Sample : 01314-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------