

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029987.D
 Acq On : 30 Jan 2023 13:27
 Operator : SY/MD
 Sample : 01314-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	275710	287384	1.12%	0.633%
2	1.561	155	162	179	rVB	239931	269441	1.05%	0.594%
3	2.101	320	330	343	rBV	431241	613956	2.39%	1.353%
4	2.378	413	416	419	rBV2	669	649	0.00%	0.001%
5	2.500	445	454	466	rVV2	14574	23095	0.09%	0.051%
6	2.757	525	534	542	rBV4	2078	3469	0.01%	0.008%
7	2.947	587	593	602	rBV5	975	1423	0.01%	0.003%
8	3.088	634	637	644	rVB2	472	369	0.00%	0.001%
9	3.285	695	698	702	rVB3	471	351	0.00%	0.001%
10	3.648	807	811	815	rVB2	383	379	0.00%	0.001%
11	3.687	815	823	826	rBV2	475	372	0.00%	0.001%
12	3.867	867	879	883	rBV	143548	271439	1.06%	0.598%
13	4.336	1006	1025	1053	rBV	279146	690655	2.69%	1.522%
14	4.558	1091	1094	1098	rBV3	404	329	0.00%	0.001%
15	4.625	1110	1115	1118	rBV2	334	272	0.00%	0.001%
16	4.641	1118	1120	1124	rVB3	457	345	0.00%	0.001%
17	4.674	1124	1130	1135	rVB2	523	502	0.00%	0.001%
18	4.822	1168	1176	1180	rBV5	863	1386	0.01%	0.003%
19	5.037	1224	1243	1284	rBV2	670959	1813240	7.06%	3.996%
20	5.281	1317	1319	1325	rVB4	569	463	0.00%	0.001%
21	5.336	1333	1336	1338	rBV3	497	282	0.00%	0.001%
22	5.362	1341	1344	1346	rBV2	801	563	0.00%	0.001%
23	5.484	1379	1382	1383	rBV2	533	307	0.00%	0.001%
24	5.542	1398	1400	1406	rVB4	480	337	0.00%	0.001%
25	5.606	1406	1420	1447	rBV	473052	959347	3.74%	2.114%
26	5.902	1497	1512	1547	rBV	1665960	3265753	12.72%	7.198%
27	6.059	1548	1561	1584	rVV	398695	802122	3.12%	1.768%
28	6.326	1640	1644	1647	rBV5	491	426	0.00%	0.001%
29	6.416	1669	1672	1675	rBV	462	327	0.00%	0.001%
30	6.616	1725	1734	1743	rBV7	2024	4397	0.02%	0.010%
31	6.664	1747	1749	1754	rVV4	677	578	0.00%	0.001%
32	6.693	1754	1758	1762	rVB3	546	414	0.00%	0.001%
33	6.815	1792	1796	1800	rVB3	563	500	0.00%	0.001%
34	6.908	1822	1825	1830	rBV3	501	453	0.00%	0.001%
35	6.976	1830	1846	1878	rBV	213013	395865	1.54%	0.872%
36	7.137	1892	1896	1898	rBV3	957	666	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029987.D
 Acq On : 30 Jan 2023 13:27
 Operator : SY/MD
 Sample : 01314-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	7.191	1910	1913	1921	rVB6	447	536	0.00%	0.001%
38	7.223	1921	1923	1927	rVB3	605	319	0.00%	0.001%
39	7.256	1929	1933	1935	rBV2	470	308	0.00%	0.001%
40	7.307	1935	1949	1984	rBV	802595	1404048	5.47%	3.095%
41	7.609	2032	2043	2070	rVV	149051	261433	1.02%	0.576%
42	7.751	2086	2087	2092	rVB4	491	273	0.00%	0.001%
43	7.892	2127	2131	2134	rBV3	647	503	0.00%	0.001%
44	7.931	2134	2143	2153	rBV3	9345	16839	0.07%	0.037%
45	8.079	2178	2189	2229	rBV	469337	811526	3.16%	1.789%
46	8.300	2256	2258	2261	rBV3	682	362	0.00%	0.001%
47	8.349	2271	2273	2277	rVB3	614	321	0.00%	0.001%
48	8.493	2315	2318	2321	rBV2	336	277	0.00%	0.001%
49	8.554	2335	2337	2340	rVB3	534	297	0.00%	0.001%
50	8.664	2369	2371	2378	rVB2	565	505	0.00%	0.001%
51	8.693	2378	2380	2384	rBV2	431	327	0.00%	0.001%
52	8.841	2409	2426	2462	rBV2	727085	1671027	6.51%	3.683%
53	9.001	2474	2476	2484	rVB5	1871	2213	0.01%	0.005%
54	9.111	2507	2510	2512	rBV	643	449	0.00%	0.001%
55	9.133	2512	2517	2520	rVV4	1653	1777	0.01%	0.004%
56	9.252	2549	2554	2555	rBV2	395	291	0.00%	0.001%
57	9.362	2585	2588	2590	rBV3	445	300	0.00%	0.001%
58	9.503	2627	2632	2635	rBV2	724	718	0.00%	0.002%
59	9.535	2638	2642	2646	rVV5	946	1157	0.00%	0.003%
60	9.693	2687	2691	2694	rBV3	405	299	0.00%	0.001%
61	9.780	2715	2718	2720	rBV2	588	366	0.00%	0.001%
62	9.882	2749	2750	2755	rBV2	310	281	0.00%	0.001%
63	9.921	2760	2762	2768	rVB3	437	302	0.00%	0.001%
64	10.011	2786	2790	2797	rBV5	998	1292	0.01%	0.003%
65	10.059	2803	2805	2809	rVB	585	317	0.00%	0.001%
66	10.204	2837	2850	2870	rVB	555587	868560	3.38%	1.914%
67	10.374	2889	2903	2915	rBV2	10874	18504	0.07%	0.041%
68	10.448	2922	2926	2932	rBV4	446	613	0.00%	0.001%
69	10.522	2944	2949	2950	rBV2	686	551	0.00%	0.001%
70	10.706	2997	3006	3014	rBV4	2342	4151	0.02%	0.009%
71	10.837	3042	3047	3048	rBV2	811	593	0.00%	0.001%
72	10.915	3065	3071	3076	rBV5	798	1202	0.00%	0.003%
73	11.037	3106	3109	3112	rVV2	591	460	0.00%	0.001%
74	11.169	3137	3150	3160	rBV	215539	334974	1.30%	0.738%
75	11.259	3160	3178	3201	rVB2	2208295	4484159	17.47%	9.883%
76	11.442	3232	3235	3239	rVB3	636	437	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029987.D
 Acq On : 30 Jan 2023 13:27
 Operator : SY/MD
 Sample : 01314-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	11.471	3242	3244	3249	rVB4	643	404	0.00%	0.001%
78	11.542	3254	3266	3275	rBV3	10856	19969	0.08%	0.044%
79	11.632	3276	3294	3335	rVV	16569453	25674159	100.00%	56.586%
80	12.156	3452	3457	3458	rBV4	940	877	0.00%	0.002%
81	12.194	3466	3469	3471	rBV3	404	310	0.00%	0.001%
82	12.239	3471	3483	3494	rVV6	4845	10416	0.04%	0.023%
83	12.307	3500	3504	3506	rBV4	1042	822	0.00%	0.002%
84	12.384	3519	3528	3536	rBV3	6269	9049	0.04%	0.020%
85	12.567	3574	3585	3593	rVV10	3516	7604	0.03%	0.017%
86	12.625	3593	3603	3621	rVB2	21708	38701	0.15%	0.085%
87	12.731	3631	3636	3650	rVB7	2851	4385	0.02%	0.010%
88	12.799	3655	3657	3660	rVV4	571	415	0.00%	0.001%
89	12.834	3660	3668	3685	rVB8	4453	9032	0.04%	0.020%
90	12.940	3697	3701	3702	rBV3	905	575	0.00%	0.001%
91	13.030	3726	3729	3734	rVB3	429	298	0.00%	0.001%
92	13.246	3785	3796	3812	rVB	149953	226017	0.88%	0.498%
93	13.365	3829	3833	3837	rVB6	553	452	0.00%	0.001%
94	13.419	3845	3850	3851	rBV3	1068	807	0.00%	0.002%
95	13.493	3869	3873	3877	rBV4	1215	1011	0.00%	0.002%
96	13.638	3915	3918	3921	rBV3	495	353	0.00%	0.001%
97	13.728	3937	3946	3960	rBV3	25543	40364	0.16%	0.089%
98	13.882	3990	3994	3998	rBV4	686	815	0.00%	0.002%
99	14.664	4235	4237	4239	rBV2	788	478	0.00%	0.001%
100	15.757	4572	4577	4588	rVB3	14277	19676	0.08%	0.043%

Sum of corrected areas: 45371712




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029987.D
Acq On : 30 Jan 2023 13:27
Operator : SY/MD
Sample : 01314-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

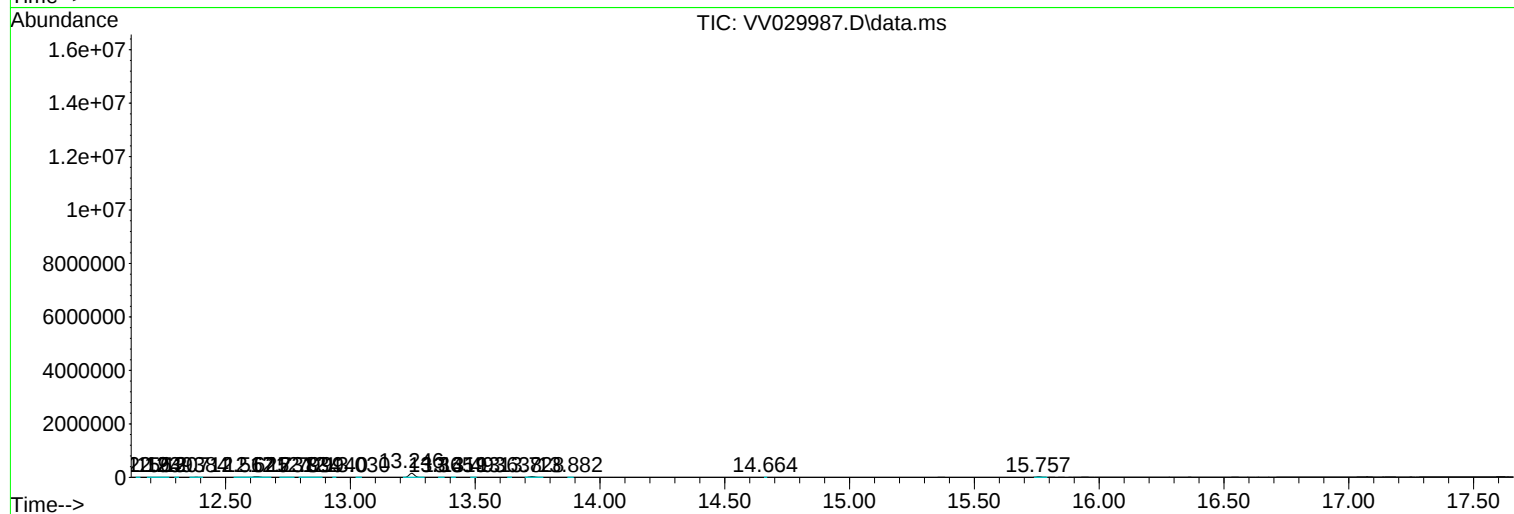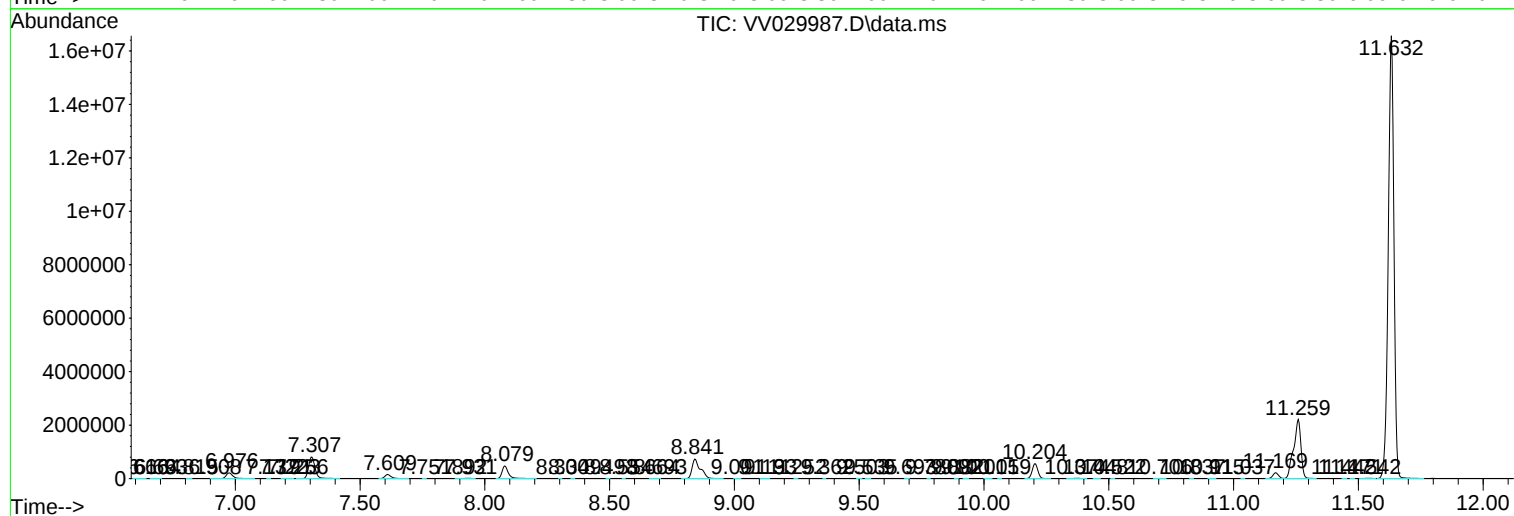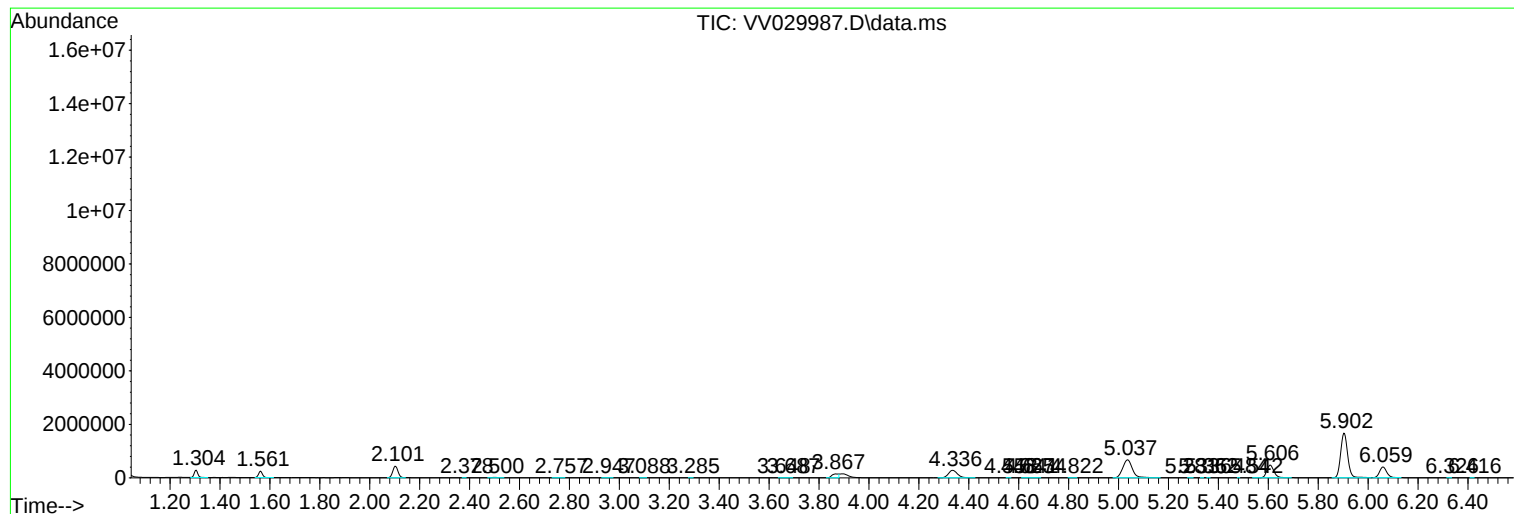

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029987.D
Acq On : 30 Jan 2023 13:27
Operator : SY/MD
Sample : 01314-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029987.D
Acq On : 30 Jan 2023 13:27
Operator : SY/MD
Sample : 01314-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc