

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029988.D
 Acq On : 30 Jan 2023 13:51
 Operator : SY/MD
 Sample : 01314-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	253719	253387	14.81%	1.906%
2	1.558	154	161	175	rVB	227262	257494	15.05%	1.937%
3	2.098	320	329	343	rBV	410098	584273	34.15%	4.396%
4	3.214	674	676	678	rVB	339	102	0.01%	0.001%
5	3.323	708	710	713	rVB	434	217	0.01%	0.002%
6	3.346	713	717	718	rBV	364	193	0.01%	0.001%
7	3.474	754	757	761	rVB2	355	252	0.01%	0.002%
8	3.497	761	764	768	rBV2	283	242	0.01%	0.002%
9	3.516	768	770	773	rBV2	304	146	0.01%	0.001%
10	3.600	793	796	799	rVB2	403	224	0.01%	0.002%
11	3.616	799	801	802	rBV	236	87	0.01%	0.001%
12	3.722	831	834	838	rBV3	325	216	0.01%	0.002%
13	3.780	850	852	854	rVB	182	74	0.00%	0.001%
14	3.860	867	877	912	rBV	134067	357533	20.90%	2.690%
15	4.333	1007	1024	1055	rBV	265686	652995	38.17%	4.913%
16	4.712	1140	1142	1145	rBV	209	84	0.00%	0.001%
17	4.745	1148	1152	1154	rBV	260	182	0.01%	0.001%
18	4.764	1154	1158	1159	rBV2	175	117	0.01%	0.001%
19	4.793	1163	1167	1169	rBV	316	237	0.01%	0.002%
20	4.806	1169	1171	1177	rVB3	390	318	0.02%	0.002%
21	4.838	1177	1181	1186	rBV2	497	497	0.03%	0.004%
22	4.860	1186	1188	1192	rVB2	189	94	0.01%	0.001%
23	4.899	1198	1200	1201	rBB2	119	46	0.00%	0.000%
24	4.915	1201	1205	1209	rBV3	270	287	0.02%	0.002%
25	4.960	1215	1219	1220	rBV2	224	143	0.01%	0.001%
26	5.034	1223	1242	1298	rBV2	649669	1710906	100.00%	12.871%
27	5.375	1347	1348	1350	rBV2	412	165	0.01%	0.001%
28	5.445	1367	1370	1372	rBV2	362	250	0.01%	0.002%
29	5.542	1398	1400	1401	rBV2	230	128	0.01%	0.001%
30	5.552	1401	1403	1406	rBV	263	119	0.01%	0.001%
31	5.606	1406	1420	1441	rBV	497293	1008605	58.95%	7.588%
32	5.812	1482	1484	1485	rBV	302	61	0.00%	0.000%
33	5.908	1503	1514	1532	rVB4	15472	33041	1.93%	0.249%
34	5.998	1540	1542	1544	rBV	319	151	0.01%	0.001%
35	6.056	1545	1560	1589	rBV	378960	783110	45.77%	5.891%
36	6.265	1624	1625	1628	rVB	264	138	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029988.D
 Acq On : 30 Jan 2023 13:51
 Operator : SY/MD
 Sample : 01314-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	6.397	1664	1666	1669	rVB2	199	104	0.01%	0.001%
38	6.449	1680	1682	1683	rBV	152	65	0.00%	0.000%
39	6.487	1690	1694	1698	rVB	472	338	0.02%	0.003%
40	6.571	1717	1720	1721	rBV	138	84	0.00%	0.001%
41	6.613	1725	1733	1742	rBV5	2177	4032	0.24%	0.030%
42	6.728	1767	1769	1773	rBV2	416	266	0.02%	0.002%
43	6.786	1786	1787	1792	rVB2	163	104	0.01%	0.001%
44	6.809	1792	1794	1795	rBV2	202	92	0.01%	0.001%
45	6.857	1807	1809	1812	rVB	104	57	0.00%	0.000%
46	6.870	1812	1813	1814	rBV	164	55	0.00%	0.000%
47	6.879	1814	1816	1819	rVB2	202	72	0.00%	0.001%
48	6.896	1819	1821	1824	rVB	207	91	0.01%	0.001%
49	6.931	1827	1832	1834	rVB2	401	362	0.02%	0.003%
50	6.976	1834	1846	1873	rBV	204110	377057	22.04%	2.837%
51	7.220	1920	1922	1928	rVB4	1119	893	0.05%	0.007%
52	7.259	1931	1934	1935	rBV2	556	296	0.02%	0.002%
53	7.304	1936	1948	1982	rVV	756969	1336742	78.13%	10.056%
54	7.564	2027	2029	2030	rBV2	676	328	0.02%	0.002%
55	7.609	2033	2043	2064	rVV	144071	248927	14.55%	1.873%
56	7.931	2135	2143	2153	rBV3	6979	11224	0.66%	0.084%
57	8.011	2167	2168	2169	rBV	276	71	0.00%	0.001%
58	8.079	2174	2189	2223	rBV	467130	809408	47.31%	6.089%
59	8.625	2355	2359	2360	rBV2	565	366	0.02%	0.003%
60	8.648	2364	2366	2368	rBV2	344	177	0.01%	0.001%
61	8.841	2412	2426	2451	rBV	773497	1252544	73.21%	9.423%
62	9.114	2508	2511	2512	rBV2	725	373	0.02%	0.003%
63	9.641	2673	2675	2676	rBV2	247	59	0.00%	0.000%
64	9.812	2721	2728	2730	rBV4	998	1085	0.06%	0.008%
65	9.915	2756	2760	2763	rBV2	599	515	0.03%	0.004%
66	9.979	2776	2780	2782	rBV5	400	301	0.02%	0.002%
67	9.992	2782	2784	2786	rVV2	533	242	0.01%	0.002%
68	10.008	2788	2789	2793	rVB	589	201	0.01%	0.002%
69	10.072	2807	2809	2811	rBV	420	239	0.01%	0.002%
70	10.204	2831	2850	2870	rBV	537866	852171	49.81%	6.411%
71	10.342	2888	2893	2894	rBV4	1106	848	0.05%	0.006%
72	10.510	2943	2945	2949	rVB3	689	421	0.02%	0.003%
73	10.529	2949	2951	2953	rBV2	472	236	0.01%	0.002%
74	10.587	2966	2969	2972	rBV4	325	201	0.01%	0.002%
75	10.677	2995	2997	2999	rBV2	365	160	0.01%	0.001%
76	10.754	3017	3021	3027	rBV2	510	535	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029988.D
 Acq On : 30 Jan 2023 13:51
 Operator : SY/MD
 Sample : 01314-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M

Title : VOC Analysis

77	10.844	3044	3049	3052	rBV4	1333	1402	0.08%	0.011%
78	11.098	3126	3128	3130	rBV	305	120	0.01%	0.001%
79	11.143	3138	3142	3146	rBV4	1187	1055	0.06%	0.008%
80	11.236	3158	3171	3194	rBV	861726	1344106	78.56%	10.112%
81	11.423	3227	3229	3230	rBV	341	117	0.01%	0.001%
82	11.493	3248	3251	3255	rBV2	447	420	0.02%	0.003%
83	11.535	3255	3264	3276	rBV	22383	41603	2.43%	0.313%
84	11.609	3276	3287	3310	rVB	809758	1344150	78.56%	10.112%
85	12.024	3413	3416	3420	rBV3	591	526	0.03%	0.004%
86	12.130	3447	3449	3452	rBV3	421	257	0.02%	0.002%
87	12.333	3505	3512	3520	rBV8	1949	3329	0.19%	0.025%
88	12.834	3659	3668	3679	rBV6	4198	7467	0.44%	0.056%
89	13.304	3812	3814	3815	rBV	904	380	0.02%	0.003%




Sum of corrected areas: 13292388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029988.D
Acq On : 30 Jan 2023 13:51
Operator : SY/MD
Sample : 01314-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

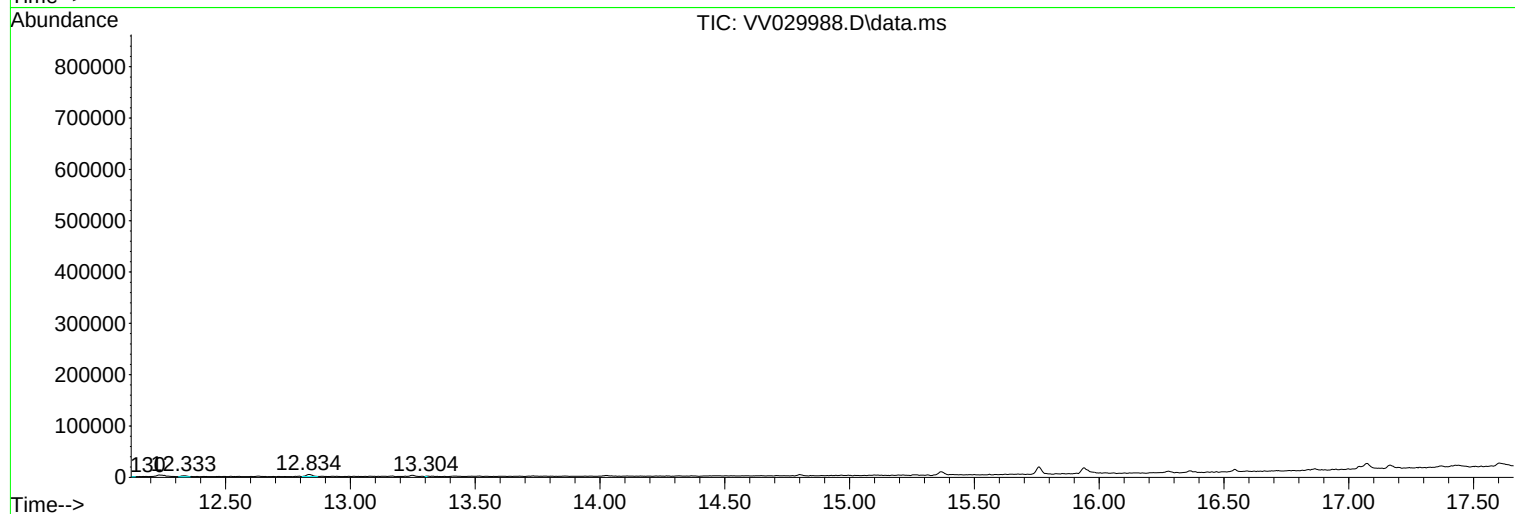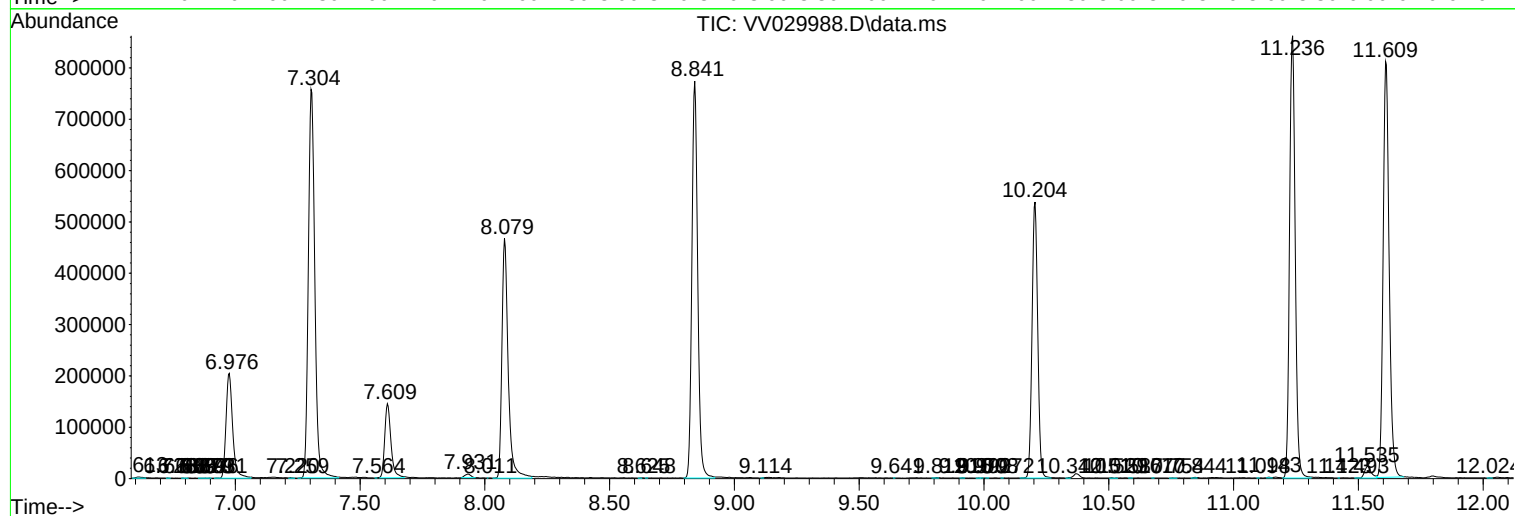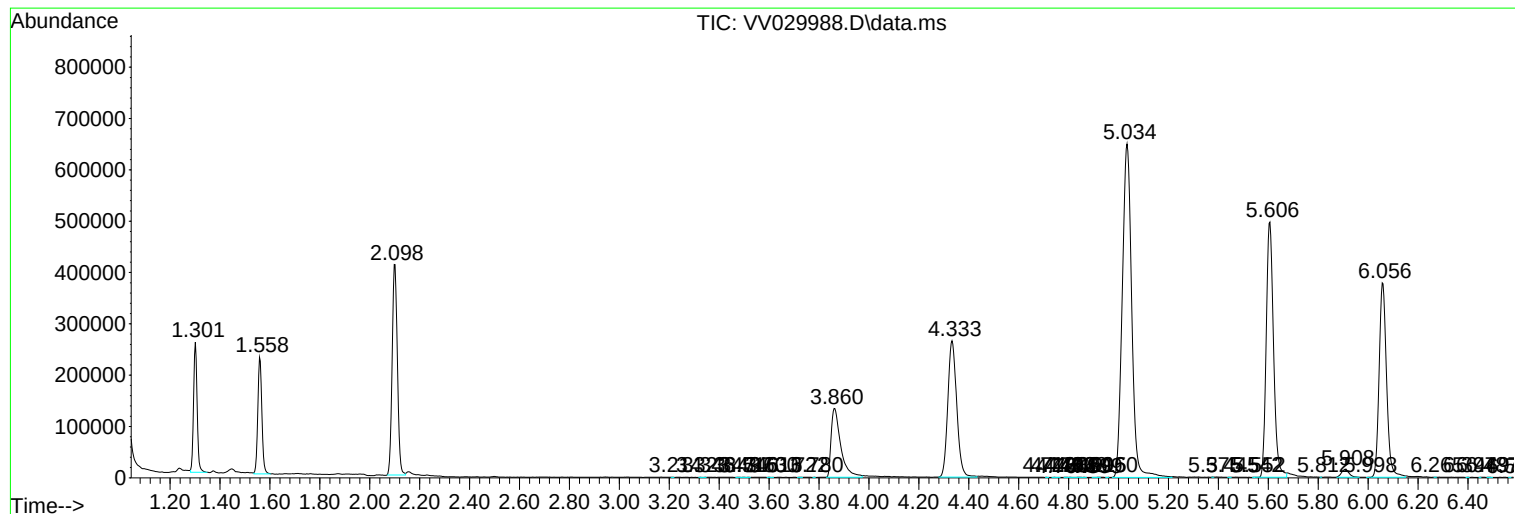

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029988.D
Acq On : 30 Jan 2023 13:51
Operator : SY/MD
Sample : 01314-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029988.D
Acq On : 30 Jan 2023 13:51
Operator : SY/MD
Sample : 01314-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------