

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029989.D
 Acq On : 30 Jan 2023 14:15
 Operator : SY/MD
 Sample : 01314-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	254986	258124	7.40%	1.534%
2	1.561	155	162	180	rVB	224738	255139	7.31%	1.516%
3	2.101	320	330	343	rBV	409548	586095	16.80%	3.484%
4	2.754	526	533	541	rVB5	1473	2331	0.07%	0.014%
5	2.815	544	552	555	rBV3	409	485	0.01%	0.003%
6	2.953	590	595	597	rBV3	445	438	0.01%	0.003%
7	3.034	618	620	624	rVB3	407	300	0.01%	0.002%
8	3.063	624	629	631	rBV4	386	294	0.01%	0.002%
9	3.224	674	679	683	rBV2	311	367	0.01%	0.002%
10	3.471	750	756	757	rBV3	346	389	0.01%	0.002%
11	3.632	801	806	812	rVB3	331	350	0.01%	0.002%
12	3.863	867	878	911	rBV	137934	404544	11.59%	2.404%
13	4.233	990	993	996	rBV4	393	328	0.01%	0.002%
14	4.336	1007	1025	1054	rBV	266263	655351	18.78%	3.895%
15	4.728	1143	1147	1152	rBV2	504	502	0.01%	0.003%
16	4.841	1177	1182	1187	rVB4	362	481	0.01%	0.003%
17	5.037	1222	1243	1270	rBV2	648946	1699344	48.70%	10.100%
18	5.368	1344	1346	1349	rBV2	709	446	0.01%	0.003%
19	5.387	1349	1352	1354	rBV3	638	372	0.01%	0.002%
20	5.465	1370	1376	1378	rBV3	756	745	0.02%	0.004%
21	5.519	1390	1393	1398	rBV3	360	296	0.01%	0.002%
22	5.606	1404	1420	1447	rBV	511957	1026632	29.42%	6.102%
23	5.783	1473	1475	1479	rVB3	774	373	0.01%	0.002%
24	5.905	1500	1513	1539	rVV	220847	443264	12.70%	2.635%
25	6.059	1547	1561	1597	rBV	380170	780122	22.36%	4.637%
26	6.284	1626	1631	1633	rBV3	526	358	0.01%	0.002%
27	6.317	1638	1641	1644	rVV2	437	302	0.01%	0.002%
28	6.355	1648	1653	1656	rVV3	435	397	0.01%	0.002%
29	6.416	1667	1672	1679	rBV2	336	428	0.01%	0.003%
30	6.619	1727	1735	1747	rBV6	1884	3951	0.11%	0.023%
31	6.735	1766	1771	1774	rBV3	372	356	0.01%	0.002%
32	6.812	1791	1795	1798	rVB3	385	282	0.01%	0.002%
33	6.902	1820	1823	1827	rVB3	446	362	0.01%	0.002%
34	6.976	1833	1846	1875	rBV	205936	377990	10.83%	2.247%
35	7.149	1895	1900	1901	rBV3	568	525	0.02%	0.003%
36	7.239	1925	1928	1931	rBV2	659	452	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029989.D
 Acq On : 30 Jan 2023 14:15
 Operator : SY/MD
 Sample : 01314-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	7.307	1935	1949	1974	rBV	770939	1343821	38.51%	7.987%
38	7.538	2016	2021	2025	rVB5	703	728	0.02%	0.004%
39	7.609	2032	2043	2069	rBV	145491	252823	7.24%	1.503%
40	7.876	2122	2126	2129	rBV2	464	373	0.01%	0.002%
41	7.892	2129	2131	2134	rVV2	385	294	0.01%	0.002%
42	7.931	2134	2143	2157	rVV3	6491	12636	0.36%	0.075%
43	8.040	2172	2177	2178	rBV2	488	323	0.01%	0.002%
44	8.079	2178	2189	2221	rBV	469656	821953	23.55%	4.885%
45	8.452	2303	2305	2310	rVB5	390	310	0.01%	0.002%
46	8.561	2336	2339	2345	rVB4	593	570	0.02%	0.003%
47	8.722	2387	2389	2393	rVB4	466	307	0.01%	0.002%
48	8.776	2403	2406	2410	rVB2	457	352	0.01%	0.002%
49	8.841	2410	2426	2431	rBV	810506	1312893	37.62%	7.803%
50	9.095	2502	2505	2507	rBV	597	312	0.01%	0.002%
51	9.124	2511	2514	2515	rBV3	884	436	0.01%	0.003%
52	9.181	2527	2532	2536	rBV5	548	457	0.01%	0.003%
53	9.317	2570	2574	2578	rBV3	403	304	0.01%	0.002%
54	9.458	2614	2618	2622	rBV2	649	575	0.02%	0.003%
55	9.497	2622	2630	2632	rBV3	734	820	0.02%	0.005%
56	9.545	2639	2645	2646	rBV3	373	367	0.01%	0.002%
57	9.622	2665	2669	2675	rVB3	304	283	0.01%	0.002%
58	9.751	2704	2709	2712	rVB	427	347	0.01%	0.002%
59	9.808	2721	2727	2732	rBV5	851	1079	0.03%	0.006%
60	9.924	2758	2763	2768	rVB3	560	621	0.02%	0.004%
61	9.966	2771	2776	2780	rVB2	319	289	0.01%	0.002%
62	10.149	2828	2833	2834	rBV	543	364	0.01%	0.002%
63	10.204	2835	2850	2875	rVV	553554	858238	24.59%	5.101%
64	10.371	2892	2902	2918	rVB2	8508	14053	0.40%	0.084%
65	10.435	2918	2922	2927	rBV2	626	655	0.02%	0.004%
66	10.513	2942	2946	2949	rBV5	781	592	0.02%	0.004%
67	10.561	2956	2961	2966	rBV6	731	840	0.02%	0.005%
68	10.728	3010	3013	3020	rBV3	395	391	0.01%	0.002%
69	10.841	3044	3048	3052	rBV3	700	665	0.02%	0.004%
70	10.905	3061	3068	3069	rBV3	830	710	0.02%	0.004%
71	11.034	3106	3108	3111	rBV	600	419	0.01%	0.002%
72	11.050	3111	3113	3120	rVB4	406	339	0.01%	0.002%
73	11.169	3134	3150	3160	rBV	89925	142158	4.07%	0.845%
74	11.236	3160	3171	3199	rVB2	937613	1929427	55.29%	11.468%
75	11.542	3256	3266	3276	rBV3	11813	21387	0.61%	0.127%
76	11.625	3276	3292	3320	rVB2	1646697	3489629	100.00%	20.741%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029989.D
 Acq On : 30 Jan 2023 14:15
 Operator : SY/MD
 Sample : 01314-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	11.799	3336	3346	3352	rBV5	3290	5713	0.16%	0.034%
78	11.857	3362	3364	3368	rVB4	713	447	0.01%	0.003%
79	12.056	3419	3426	3430	rBV6	1647	2045	0.06%	0.012%
80	12.098	3435	3439	3444	rVV4	1291	1183	0.03%	0.007%
81	12.172	3459	3462	3465	rBV2	474	380	0.01%	0.002%
82	12.249	3474	3486	3494	rBV6	2757	6479	0.19%	0.039%
83	12.336	3502	3513	3520	rBV6	1804	2952	0.08%	0.018%
84	12.413	3533	3537	3540	rBV3	297	283	0.01%	0.002%
85	12.435	3540	3544	3546	rBV3	642	498	0.01%	0.003%
86	12.522	3568	3571	3577	rVB5	518	417	0.01%	0.002%
87	12.606	3595	3597	3599	rBV3	466	288	0.01%	0.002%
88	12.632	3599	3605	3611	rVB5	1309	1802	0.05%	0.011%
89	12.686	3617	3622	3627	rBV5	439	628	0.02%	0.004%
90	12.760	3641	3645	3646	rBV	463	321	0.01%	0.002%
91	12.834	3661	3668	3680	rVB7	3919	6106	0.17%	0.036%
92	12.998	3715	3719	3722	rBV4	554	474	0.01%	0.003%
93	13.246	3787	3796	3808	rVB2	29792	46419	1.33%	0.276%
94	13.361	3828	3832	3840	rVB5	681	820	0.02%	0.005%
95	13.419	3844	3850	3856	rBV9	1174	1596	0.05%	0.009%
96	13.731	3939	3947	3956	rBV3	5174	6958	0.20%	0.041%
97	14.027	4036	4039	4045	rVB4	1856	1849	0.05%	0.011%
98	14.130	4069	4071	4076	rVB4	596	369	0.01%	0.002%
99	14.805	4276	4281	4284	rBV5	1643	1769	0.05%	0.011%
100	15.760	4571	4578	4588	rVB2	13330	19201	0.55%	0.114%




Sum of corrected areas: 16824652

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029989.D
Acq On : 30 Jan 2023 14:15
Operator : SY/MD
Sample : 01314-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

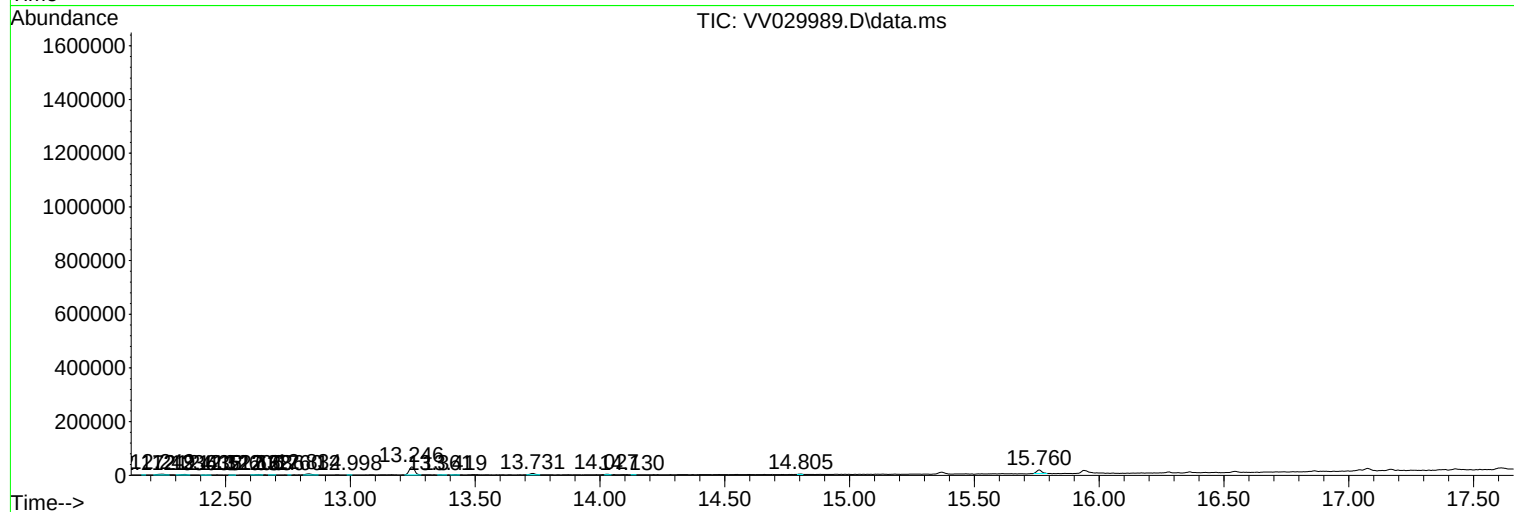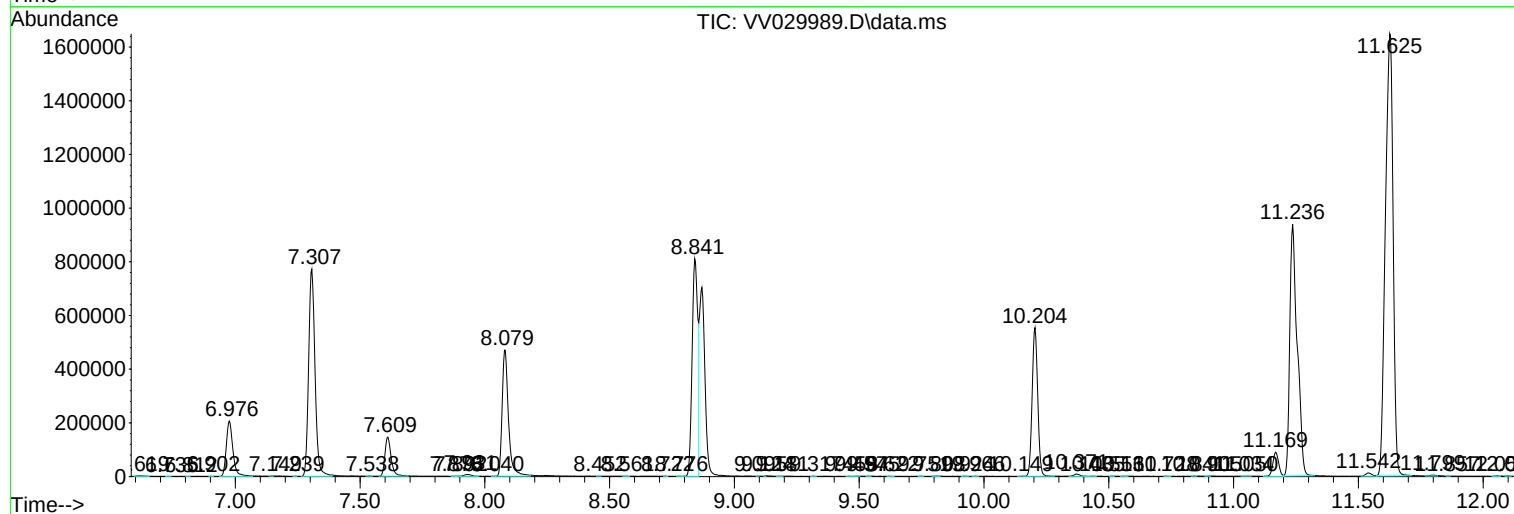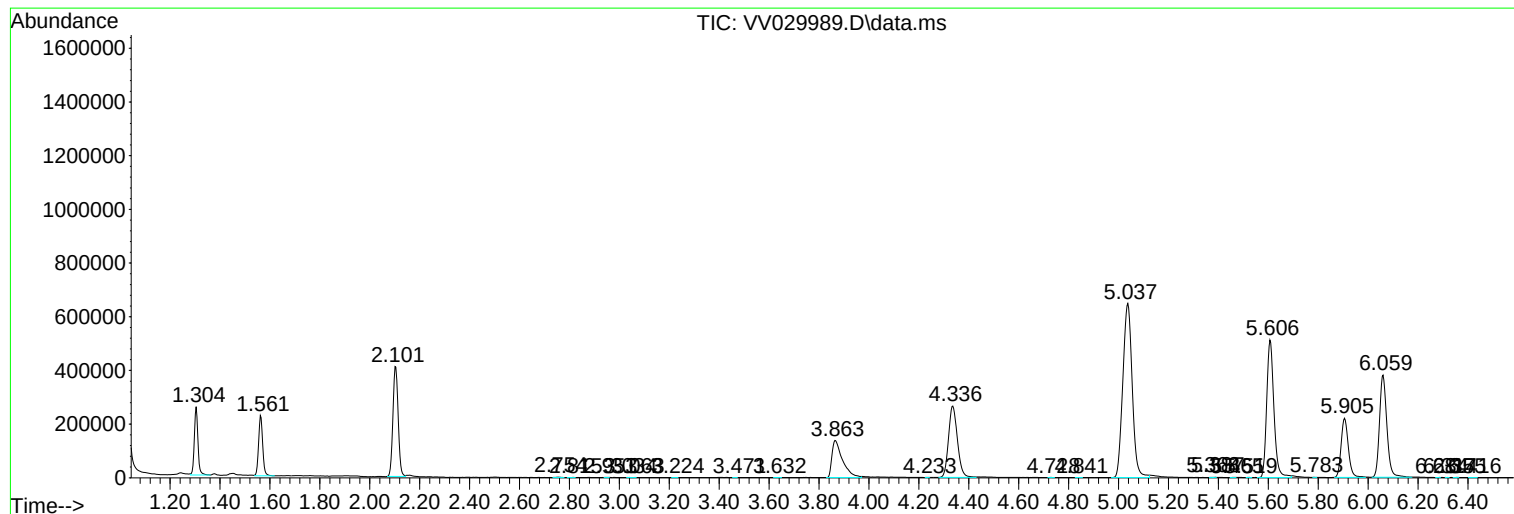

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029989.D
Acq On : 30 Jan 2023 14:15
Operator : SY/MD
Sample : 01314-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029989.D
Acq On : 30 Jan 2023 14:15
Operator : SY/MD
Sample : 01314-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc