

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029990.D
 Acq On : 30 Jan 2023 14:38
 Operator : SY/MD
 Sample : 01314-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	261826	262512	15.42%	1.852%
2	1.561	155	162	177	rVB	229028	258670	15.19%	1.825%
3	2.101	320	330	343	rBV	406623	588511	34.56%	4.152%
4	2.503	450	455	463	rVB6	1251	1479	0.09%	0.010%
5	2.754	524	533	544	rVB4	3393	6219	0.37%	0.044%
6	3.159	655	659	662	rVB2	479	335	0.02%	0.002%
7	3.204	670	673	679	rBV2	327	334	0.02%	0.002%
8	3.625	799	804	809	rVB3	296	323	0.02%	0.002%
9	3.735	832	838	840	rBV3	365	357	0.02%	0.003%
10	3.867	868	879	915	rBV3	136305	459308	26.97%	3.240%
11	4.336	1007	1025	1057	rBV	269111	661283	38.83%	4.665%
12	4.635	1115	1118	1125	rVB4	433	495	0.03%	0.003%
13	4.667	1125	1128	1139	rVB3	700	929	0.05%	0.007%
14	4.715	1139	1143	1145	rBV3	427	305	0.02%	0.002%
15	5.037	1224	1243	1269	rBV2	653644	1702920	100.00%	12.013%
16	5.320	1327	1331	1336	rBV3	582	644	0.04%	0.005%
17	5.606	1406	1420	1465	rBV	520542	1065503	62.57%	7.517%
18	5.844	1492	1494	1500	rVB4	428	365	0.02%	0.003%
19	5.905	1500	1513	1540	rBV	254180	503307	29.56%	3.551%
20	6.059	1547	1561	1597	rVB	381217	784850	46.09%	5.537%
21	6.265	1621	1625	1627	rBV3	440	310	0.02%	0.002%
22	6.297	1632	1635	1638	rBV4	353	306	0.02%	0.002%
23	6.419	1670	1673	1678	rVB3	347	300	0.02%	0.002%
24	6.616	1725	1734	1744	rBV6	2369	4668	0.27%	0.033%
25	6.821	1796	1798	1803	rVB2	429	359	0.02%	0.003%
26	6.850	1803	1807	1811	rBV2	454	317	0.02%	0.002%
27	6.976	1834	1846	1873	rBV	204534	375032	22.02%	2.646%
28	7.149	1894	1900	1901	rBV4	833	889	0.05%	0.006%
29	7.307	1935	1949	1982	rVV	772527	1356666	79.67%	9.571%
30	7.464	1995	1998	1999	rBV3	746	413	0.02%	0.003%
31	7.474	1999	2001	2011	rVB8	1750	1995	0.12%	0.014%
32	7.516	2011	2014	2019	rBV4	563	371	0.02%	0.003%
33	7.609	2032	2043	2066	rBV	144547	255605	15.01%	1.803%
34	7.870	2119	2124	2125	rBV2	576	345	0.02%	0.002%
35	7.934	2135	2144	2158	rVB3	5516	10375	0.61%	0.073%
36	8.079	2176	2189	2215	rBV	454184	800518	47.01%	5.647%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029990.D
 Acq On : 30 Jan 2023 14:38
 Operator : SY/MD
 Sample : 01314-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	8.439	2299	2301	2306	rVB5	901	699	0.04%	0.005%
38	8.464	2306	2309	2312	rBV2	409	336	0.02%	0.002%
39	8.558	2335	2338	2340	rBV2	688	483	0.03%	0.003%
40	8.657	2362	2369	2373	rVB5	348	419	0.02%	0.003%
41	8.686	2373	2378	2382	rVB3	568	437	0.03%	0.003%
42	8.709	2382	2385	2389	rBV3	399	369	0.02%	0.003%
43	8.747	2392	2397	2399	rBV4	561	473	0.03%	0.003%
44	8.841	2413	2426	2455	rBV	802916	1312899	77.10%	9.262%
45	9.130	2512	2516	2517	rBV4	822	559	0.03%	0.004%
46	9.172	2527	2529	2534	rVB3	462	393	0.02%	0.003%
47	9.316	2569	2574	2577	rBV4	527	493	0.03%	0.003%
48	9.426	2606	2608	2612	rVB2	803	495	0.03%	0.003%
49	9.461	2612	2619	2620	rBV2	431	383	0.02%	0.003%
50	9.564	2648	2651	2656	rVB4	730	518	0.03%	0.004%
51	9.696	2686	2692	2694	rBV3	838	811	0.05%	0.006%
52	9.805	2722	2726	2729	rBV4	986	819	0.05%	0.006%
53	10.014	2788	2791	2796	rVB4	548	509	0.03%	0.004%
54	10.162	2834	2837	2838	rVV2	980	650	0.04%	0.005%
55	10.204	2838	2850	2876	rVV	559702	866116	50.86%	6.110%
56	10.307	2880	2882	2887	rVB3	714	571	0.03%	0.004%
57	10.371	2887	2902	2912	rBV3	6740	12185	0.72%	0.086%
58	10.561	2957	2961	2964	rBV2	524	445	0.03%	0.003%
59	10.577	2964	2966	2971	rVB5	767	488	0.03%	0.003%
60	10.609	2971	2976	2981	rBV4	496	548	0.03%	0.004%
61	10.715	3006	3009	3010	rBV2	729	399	0.02%	0.003%
62	10.847	3041	3050	3058	rBV6	1383	2322	0.14%	0.016%
63	10.918	3067	3072	3075	rBV3	825	725	0.04%	0.005%
64	11.001	3090	3098	3103	rBV6	788	1006	0.06%	0.007%
65	11.140	3136	3141	3142	rVV3	1568	1216	0.07%	0.009%
66	11.172	3143	3151	3159	rVB3	8792	13237	0.78%	0.093%
67	11.236	3159	3171	3198	rBV	912091	1409748	82.78%	9.945%
68	11.496	3248	3252	3255	rBV3	399	395	0.02%	0.003%
69	11.541	3255	3266	3275	rVV2	10440	19213	1.13%	0.136%
70	11.609	3275	3287	3317	rVB	819776	1317883	77.39%	9.297%
71	11.734	3323	3326	3328	rBV3	567	440	0.03%	0.003%
72	11.747	3328	3330	3333	rVB3	985	494	0.03%	0.003%
73	11.799	3339	3346	3359	rBV4	2885	5248	0.31%	0.037%
74	12.030	3415	3418	3421	rBV2	549	391	0.02%	0.003%
75	12.101	3436	3440	3449	rVB7	1229	1645	0.10%	0.012%
76	12.194	3467	3469	3473	rVB2	736	426	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029990.D
 Acq On : 30 Jan 2023 14:38
 Operator : SY/MD
 Sample : 01314-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	12.220	3473	3477	3478	rBV2	1351	919	0.05%	0.006%
78	12.239	3478	3483	3490	rVV6	1855	2628	0.15%	0.019%
79	12.332	3509	3512	3518	rVB5	1964	2055	0.12%	0.014%
80	12.455	3548	3550	3553	rBV3	592	367	0.02%	0.003%
81	12.583	3586	3590	3594	rBV3	446	412	0.02%	0.003%
82	12.628	3596	3604	3618	rVV5	2986	5020	0.29%	0.035%
83	12.705	3626	3628	3632	rBV4	495	353	0.02%	0.002%
84	12.763	3641	3646	3649	rBV4	954	728	0.04%	0.005%
85	12.834	3662	3668	3678	rVB7	3982	5895	0.35%	0.042%
86	12.873	3678	3680	3685	rVB4	648	409	0.02%	0.003%
87	12.947	3701	3703	3707	rVB2	917	605	0.04%	0.004%
88	13.017	3717	3725	3727	rBV5	540	686	0.04%	0.005%
89	13.249	3788	3797	3810	rVB3	9428	13615	0.80%	0.096%
90	13.297	3810	3812	3813	rBV	577	305	0.02%	0.002%
91	13.422	3849	3851	3853	rVB2	889	381	0.02%	0.003%
92	13.487	3866	3871	3874	rBV5	1019	1047	0.06%	0.007%
93	13.731	3944	3947	3953	rVB5	1285	1393	0.08%	0.010%
94	13.853	3981	3985	3989	rBV5	874	932	0.05%	0.007%
95	13.975	4021	4023	4027	rVB3	1002	610	0.04%	0.004%
96	14.210	4094	4096	4100	rBV4	678	561	0.03%	0.004%
97	14.802	4275	4280	4288	rVB7	2635	3105	0.18%	0.022%
98	15.364	4449	4455	4464	rBV10	6976	10962	0.64%	0.077%
99	15.757	4571	4577	4592	rVB4	13562	19994	1.17%	0.141%
100	15.937	4627	4633	4641	rBV7	10552	18454	1.08%	0.130%




Sum of corrected areas: 14175440

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029990.D
Acq On : 30 Jan 2023 14:38
Operator : SY/MD
Sample : 01314-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

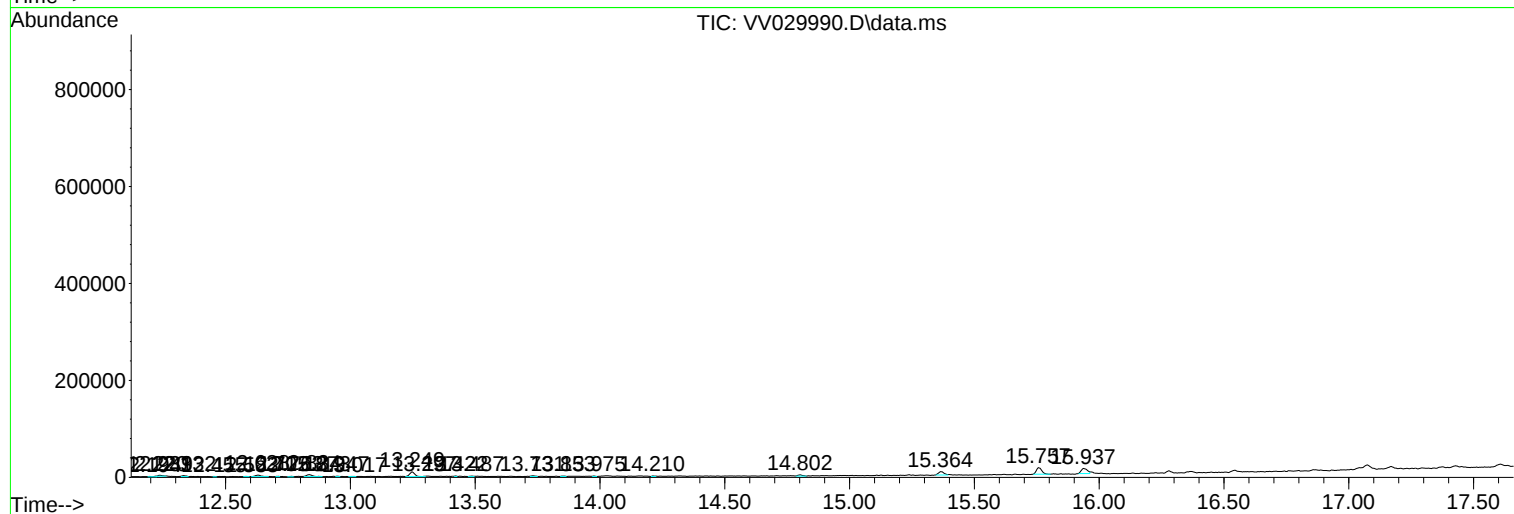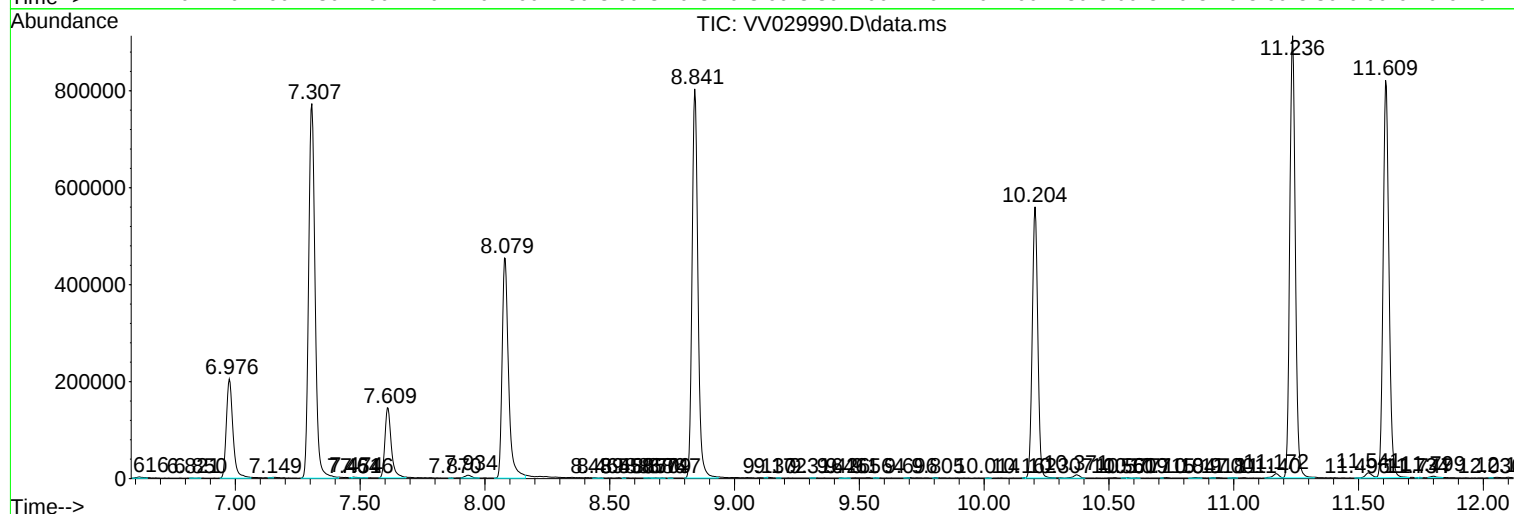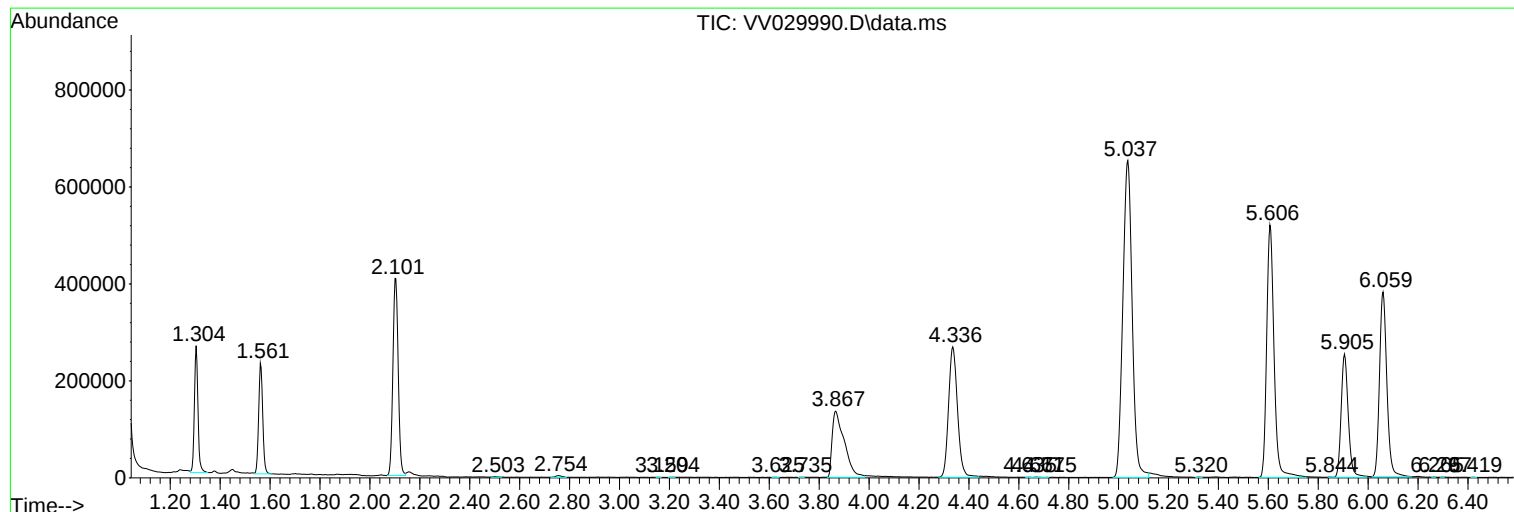

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029990.D
Acq On : 30 Jan 2023 14:38
Operator : SY/MD
Sample : 01314-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029990.D
Acq On : 30 Jan 2023 14:38
Operator : SY/MD
Sample : 01314-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc