

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029991.D
 Acq On : 30 Jan 2023 15:02
 Operator : SY/MD
 Sample : 01314-24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.198	43	49	57	rBV	156482	144563	6.55%	0.850%
2	1.304	76	82	100	rVB	255698	265203	12.02%	1.560%
3	1.561	155	162	180	rVB	230379	263015	11.92%	1.547%
4	2.101	320	330	342	rBV	414889	596894	27.05%	3.510%
5	2.497	448	453	465	rVB5	2352	3760	0.17%	0.022%
6	2.751	528	532	537	rBV4	495	462	0.02%	0.003%
7	3.240	681	684	686	rVV3	373	280	0.01%	0.002%
8	3.314	704	707	711	rVV2	315	312	0.01%	0.002%
9	3.346	712	717	720	rVB3	335	362	0.02%	0.002%
10	3.442	744	747	751	rVB3	455	376	0.02%	0.002%
11	3.622	800	803	809	rVB3	242	286	0.01%	0.002%
12	3.677	815	820	824	rBV	265	319	0.01%	0.002%
13	3.867	868	879	913	rBV	140873	401971	18.22%	2.364%
14	4.336	1004	1025	1052	rBV	273904	668887	30.32%	3.933%
15	4.539	1086	1088	1093	rVB5	445	287	0.01%	0.002%
16	4.719	1142	1144	1151	rVB4	298	296	0.01%	0.002%
17	4.760	1151	1157	1158	rBV3	367	276	0.01%	0.002%
18	4.924	1204	1208	1212	rBV2	236	281	0.01%	0.002%
19	5.037	1223	1243	1271	rBV2	668844	1733753	78.58%	10.195%
20	5.339	1335	1337	1342	rVB3	552	372	0.02%	0.002%
21	5.368	1342	1346	1351	rVV4	485	571	0.03%	0.003%
22	5.397	1351	1355	1361	rVB3	602	718	0.03%	0.004%
23	5.500	1382	1387	1394	rVB5	600	687	0.03%	0.004%
24	5.539	1396	1399	1401	rBV	632	309	0.01%	0.002%
25	5.606	1406	1420	1444	rBV	547721	1101391	49.92%	6.477%
26	5.902	1498	1512	1546	rVV	1118818	2206227	100.00%	12.974%
27	6.059	1548	1561	1594	rVB	397529	810107	36.72%	4.764%
28	6.403	1665	1668	1671	rBV2	504	381	0.02%	0.002%
29	6.510	1698	1701	1704	rBV2	445	278	0.01%	0.002%
30	6.532	1704	1708	1710	rBV2	436	332	0.02%	0.002%
31	6.725	1763	1768	1774	rBV5	643	652	0.03%	0.004%
32	6.876	1812	1815	1818	rVB	528	345	0.02%	0.002%
33	6.976	1832	1846	1878	rBV	212886	389822	17.67%	2.292%
34	7.207	1915	1918	1920	rBV2	610	314	0.01%	0.002%
35	7.307	1935	1949	1981	rBV	778310	1370822	62.13%	8.061%
36	7.609	2033	2043	2064	rBV	146512	256539	11.63%	1.509%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029991.D
 Acq On : 30 Jan 2023 15:02
 Operator : SY/MD
 Sample : 01314-24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	7.841	2113	2115	2121	rBV3	474	365	0.02%	0.002%
38	7.931	2133	2143	2153	rBV2	4721	8184	0.37%	0.048%
39	7.989	2159	2161	2165	rVB2	481	312	0.01%	0.002%
40	8.079	2178	2189	2226	rBV	495227	859592	38.96%	5.055%
41	8.374	2278	2281	2284	rBV4	545	345	0.02%	0.002%
42	8.445	2301	2303	2308	rVB4	869	569	0.03%	0.003%
43	8.487	2312	2316	2319	rBV4	356	333	0.02%	0.002%
44	8.603	2349	2352	2355	rVB3	448	310	0.01%	0.002%
45	8.632	2355	2361	2365	rVB3	624	584	0.03%	0.003%
46	8.670	2365	2373	2375	rBV3	611	757	0.03%	0.004%
47	8.754	2396	2399	2407	rBV5	370	344	0.02%	0.002%
48	8.841	2412	2426	2459	rBV	845049	1465430	66.42%	8.618%
49	9.136	2515	2518	2522	rVB3	834	642	0.03%	0.004%
50	9.226	2543	2546	2550	rVB4	371	322	0.01%	0.002%
51	9.259	2552	2556	2558	rBV3	422	289	0.01%	0.002%
52	9.278	2560	2562	2567	rVB3	571	308	0.01%	0.002%
53	9.349	2579	2584	2586	rVB3	634	554	0.03%	0.003%
54	9.378	2586	2593	2596	rVB3	281	325	0.01%	0.002%
55	9.413	2599	2604	2609	rVB2	491	395	0.02%	0.002%
56	9.458	2615	2618	2623	rBV3	378	287	0.01%	0.002%
57	9.487	2623	2627	2630	rBV4	468	430	0.02%	0.003%
58	9.561	2648	2650	2655	rVB2	556	389	0.02%	0.002%
59	9.583	2655	2657	2659	rVV2	491	311	0.01%	0.002%
60	9.696	2688	2692	2694	rBV	522	334	0.02%	0.002%
61	9.767	2710	2714	2719	rBV3	393	378	0.02%	0.002%
62	9.796	2719	2723	2724	rBV3	643	405	0.02%	0.002%
63	10.152	2831	2834	2836	rBV2	606	489	0.02%	0.003%
64	10.204	2836	2850	2869	rBV	578380	897166	40.67%	5.276%
65	10.368	2893	2901	2916	rVB2	5303	9279	0.42%	0.055%
66	10.525	2946	2950	2953	rBV3	444	414	0.02%	0.002%
67	10.680	2994	2998	3002	rVB3	665	479	0.02%	0.003%
68	10.837	3044	3047	3048	rBV2	651	388	0.02%	0.002%
69	10.847	3048	3050	3053	rVB3	590	358	0.02%	0.002%
70	11.098	3125	3128	3133	rBV2	428	324	0.01%	0.002%
71	11.169	3135	3150	3159	rBV2	13827	23896	1.08%	0.141%
72	11.236	3159	3171	3196	rBV	978241	1579819	71.61%	9.290%
73	11.541	3257	3266	3275	rBV4	7045	12160	0.55%	0.072%
74	11.612	3275	3288	3309	rVV2	883005	1750182	79.33%	10.292%
75	11.799	3337	3346	3356	rBV6	2938	6214	0.28%	0.037%
76	11.998	3406	3408	3412	rVV3	459	350	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029991.D
 Acq On : 30 Jan 2023 15:02
 Operator : SY/MD
 Sample : 01314-24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	12.062	3417	3428	3432	rBV6	1167	2109	0.10%	0.012%
78	12.143	3451	3453	3459	rBV4	408	418	0.02%	0.002%
79	12.242	3474	3484	3489	rBV7	1731	3410	0.15%	0.020%
80	12.332	3504	3512	3521	rBV7	2823	4622	0.21%	0.027%
81	12.477	3555	3557	3561	rVB2	523	346	0.02%	0.002%
82	12.522	3563	3571	3573	rBV3	735	877	0.04%	0.005%
83	12.622	3592	3602	3630	rVB2	42022	74809	3.39%	0.440%
84	12.757	3639	3644	3646	rBV2	629	633	0.03%	0.004%
85	12.831	3657	3667	3684	rVB9	4400	8480	0.38%	0.050%
86	12.895	3684	3687	3689	rBV3	372	318	0.01%	0.002%
87	13.246	3790	3796	3806	rVB3	6767	9061	0.41%	0.053%
88	13.307	3812	3815	3819	rVB3	763	511	0.02%	0.003%
89	13.416	3846	3849	3856	rVB6	1231	1535	0.07%	0.009%
90	13.538	3885	3887	3892	rBV4	362	352	0.02%	0.002%
91	13.728	3944	3946	3953	rVB4	1402	1072	0.05%	0.006%
92	13.786	3961	3964	3967	rVB3	572	431	0.02%	0.003%
93	13.850	3982	3984	3987	rVB2	713	400	0.02%	0.002%
94	13.866	3987	3989	3993	rBV2	463	344	0.02%	0.002%
95	14.027	4034	4039	4045	rVB5	1293	1513	0.07%	0.009%
96	14.310	4122	4127	4132	rBV6	880	1280	0.06%	0.008%
97	14.625	4222	4225	4229	rBV3	926	659	0.03%	0.004%
98	15.364	4449	4455	4464	rBV10	6754	10484	0.48%	0.062%
99	15.760	4571	4578	4586	rVB2	13219	17394	0.79%	0.102%
100	15.937	4627	4633	4642	rBV8	11155	18635	0.84%	0.110%




Sum of corrected areas: 17005155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029991.D
Acq On : 30 Jan 2023 15:02
Operator : SY/MD
Sample : 01314-24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44Q7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

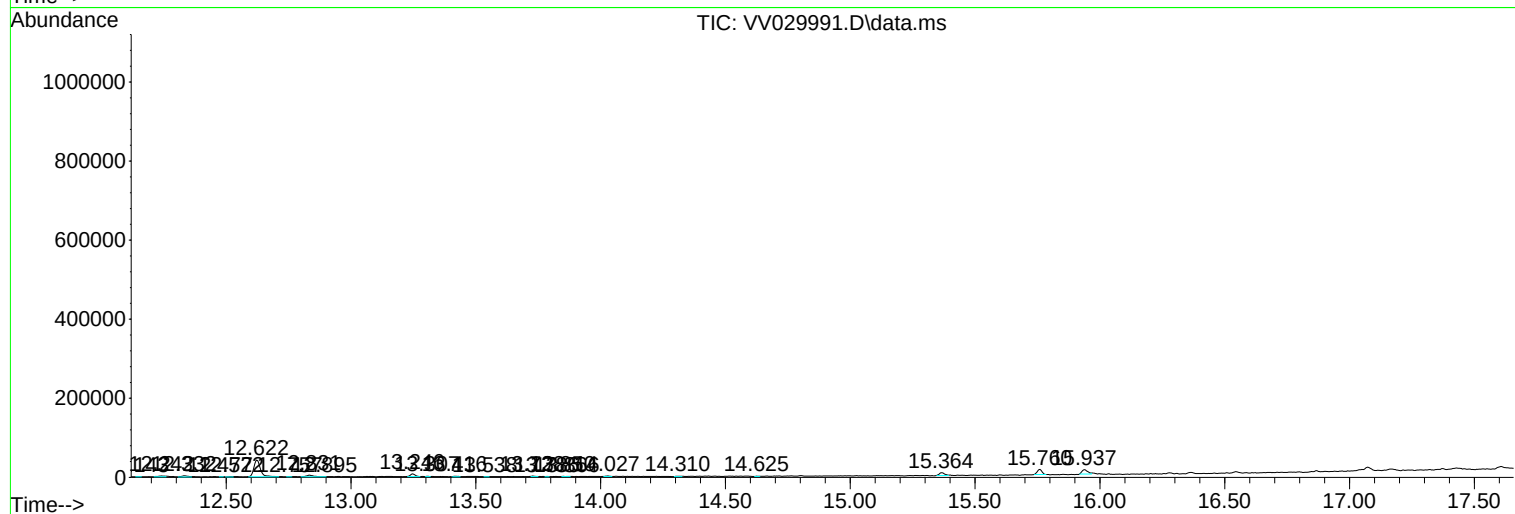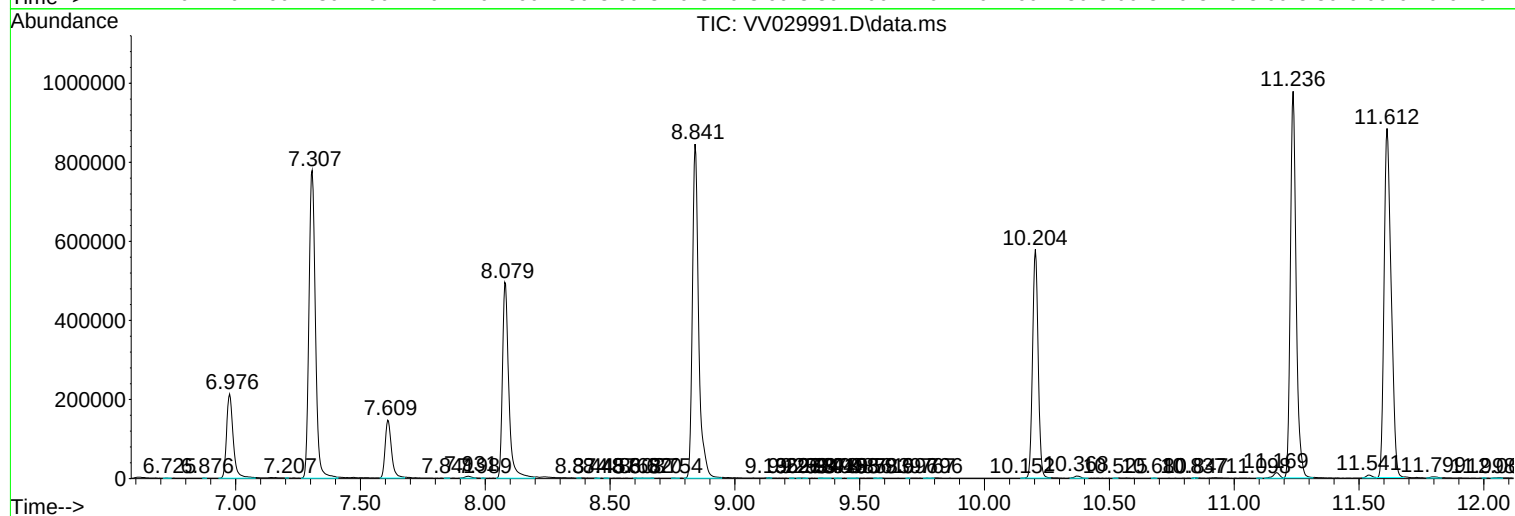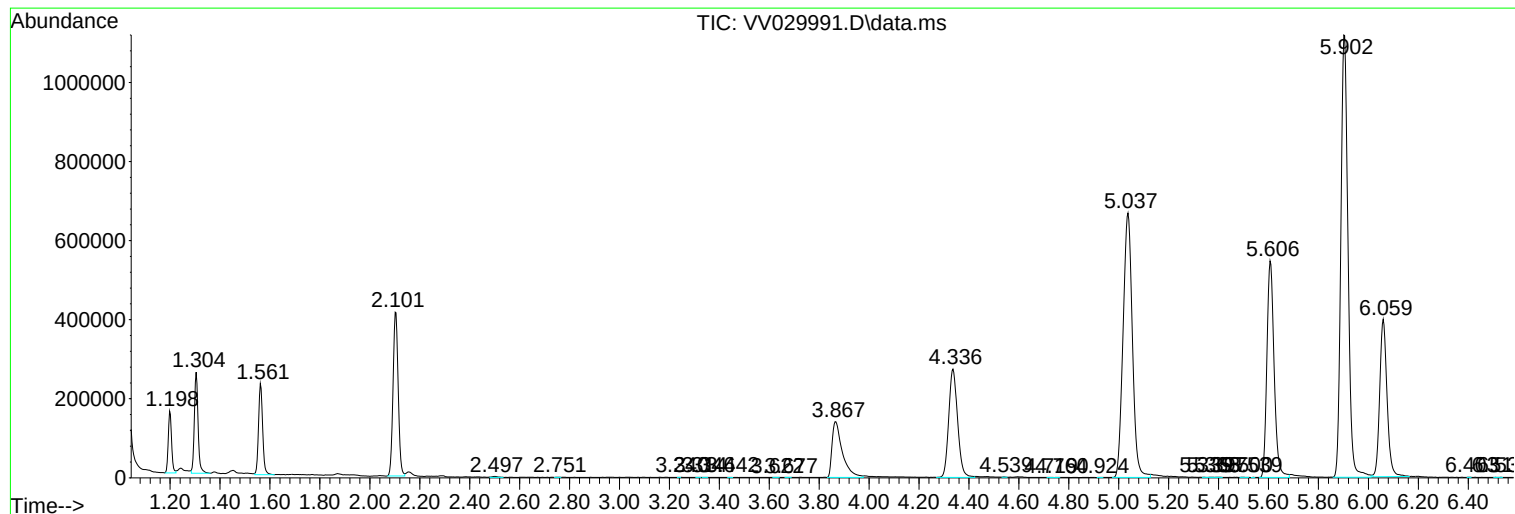

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013023\
Data File : VW029991.D
Acq On : 30 Jan 2023 15:02
Operator : SY/MD
Sample : 01314-24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44Q7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029991.D
Acq On : 30 Jan 2023 15:02
Operator : SY/MD
Sample : 01314-24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44Q7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc