

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029996.D
 Acq On : 30 Jan 2023 16:59
 Operator : SY/MD
 Sample : 01314-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	245104	242655	14.54%	1.797%
2	1.561	155	162	182	rVB	213176	249135	14.93%	1.845%
3	2.104	320	331	344	rBV	391480	563915	33.78%	4.177%
4	2.506	448	456	460	rVB4	1101	1724	0.10%	0.013%
5	2.754	529	533	538	rVB2	489	514	0.03%	0.004%
6	2.780	538	541	545	rBV2	388	419	0.03%	0.003%
7	3.008	608	612	616	rVV2	247	283	0.02%	0.002%
8	3.030	616	619	625	rVV4	468	483	0.03%	0.004%
9	3.297	698	702	705	rVB	398	256	0.02%	0.002%
10	3.760	843	846	849	rVB2	530	299	0.02%	0.002%
11	3.825	858	866	868	rBV2	389	503	0.03%	0.004%
12	3.866	868	879	913	rBV	139127	366560	21.96%	2.715%
13	4.262	999	1002	1006	rBV4	478	348	0.02%	0.003%
14	4.336	1006	1025	1056	rBV	262406	651327	39.02%	4.824%
15	4.760	1153	1157	1163	rVB3	586	542	0.03%	0.004%
16	4.792	1163	1167	1170	rBV2	384	267	0.02%	0.002%
17	5.037	1223	1243	1273	rBV2	645196	1669167	100.00%	12.363%
18	5.243	1305	1307	1312	rVB4	623	437	0.03%	0.003%
19	5.300	1322	1325	1328	rBV3	424	319	0.02%	0.002%
20	5.323	1328	1332	1336	rVB4	513	451	0.03%	0.003%
21	5.362	1341	1344	1346	rVB2	563	278	0.02%	0.002%
22	5.606	1402	1420	1462	rBV	542925	1114439	66.77%	8.254%
23	5.895	1502	1510	1513	rBV5	2470	3121	0.19%	0.023%
24	6.059	1547	1561	1582	rBV	378470	775414	46.46%	5.743%
25	6.188	1599	1601	1605	rBV3	681	536	0.03%	0.004%
26	6.268	1624	1626	1632	rVB3	731	478	0.03%	0.004%
27	6.300	1632	1636	1638	rBV4	442	371	0.02%	0.003%
28	6.455	1677	1684	1687	rBV2	419	480	0.03%	0.004%
29	6.609	1724	1732	1733	rBV3	2018	1904	0.11%	0.014%
30	6.689	1755	1757	1761	rVB2	393	252	0.02%	0.002%
31	6.760	1776	1779	1789	rVB2	460	581	0.03%	0.004%
32	6.976	1834	1846	1873	rBV	201134	368810	22.10%	2.732%
33	7.143	1892	1898	1902	rBV6	1178	1321	0.08%	0.010%
34	7.307	1936	1949	1981	rBV	744476	1315196	78.79%	9.741%
35	7.609	2033	2043	2064	rBV	138691	243917	14.61%	1.807%
36	7.824	2108	2110	2115	rVB3	564	419	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029996.D
 Acq On : 30 Jan 2023 16:59
 Operator : SY/MD
 Sample : 01314-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	7.850	2115	2118	2119	rBV	537	281	0.02%	0.002%
38	7.931	2134	2143	2152	rBV2	8458	15201	0.91%	0.113%
39	8.008	2162	2167	2170	rBV4	343	334	0.02%	0.002%
40	8.082	2179	2190	2226	rBV	475536	837801	50.19%	6.205%
41	8.381	2280	2283	2287	rBV5	603	454	0.03%	0.003%
42	8.471	2308	2311	2314	rVV3	326	293	0.02%	0.002%
43	8.548	2333	2335	2338	rVB2	535	266	0.02%	0.002%
44	8.673	2368	2374	2376	rBV4	375	363	0.02%	0.003%
45	8.841	2414	2426	2460	rBV	831985	1353293	81.08%	10.024%
46	8.988	2469	2472	2473	rBV2	497	289	0.02%	0.002%
47	9.005	2475	2477	2480	rVB4	691	321	0.02%	0.002%
48	9.069	2495	2497	2501	rVB3	553	376	0.02%	0.003%
49	9.133	2512	2517	2518	rBV3	942	769	0.05%	0.006%
50	9.197	2532	2537	2543	rBV4	600	715	0.04%	0.005%
51	9.326	2571	2577	2579	rBV3	499	467	0.03%	0.003%
52	9.406	2596	2602	2606	rBV3	409	468	0.03%	0.003%
53	9.541	2639	2644	2646	rBV2	437	362	0.02%	0.003%
54	9.599	2658	2662	2663	rBV2	447	318	0.02%	0.002%
55	9.712	2692	2697	2700	rBV2	359	292	0.02%	0.002%
56	9.805	2719	2726	2729	rBV3	648	819	0.05%	0.006%
57	9.921	2756	2762	2765	rBV2	665	708	0.04%	0.005%
58	10.085	2808	2813	2817	rVB3	531	404	0.02%	0.003%
59	10.204	2832	2850	2871	rBV	561988	877723	52.58%	6.501%
60	10.371	2891	2902	2911	rBV	8957	14975	0.90%	0.111%
61	10.506	2939	2944	2946	rBV3	533	460	0.03%	0.003%
62	10.638	2982	2985	2988	rVB2	458	271	0.02%	0.002%
63	10.670	2991	2995	3000	rBV3	450	473	0.03%	0.004%
64	10.773	3023	3027	3030	rBV3	288	273	0.02%	0.002%
65	10.844	3046	3049	3065	rVB5	1084	2087	0.13%	0.015%
66	10.911	3065	3070	3071	rBV2	884	621	0.04%	0.005%
67	11.123	3131	3136	3138	rBV2	449	374	0.02%	0.003%
68	11.146	3138	3143	3147	rVV6	1266	1285	0.08%	0.010%
69	11.236	3158	3171	3195	rBV	955443	1449614	86.85%	10.737%
70	11.538	3255	3265	3275	rBV5	13448	24901	1.49%	0.184%
71	11.612	3276	3288	3312	rVB	794818	1261200	75.56%	9.342%
72	11.795	3340	3345	3348	rBV4	1867	2250	0.13%	0.017%
73	11.879	3368	3371	3374	rBV4	519	336	0.02%	0.002%
74	11.937	3386	3389	3392	rBV3	421	266	0.02%	0.002%
75	12.056	3418	3426	3430	rBV5	1171	1565	0.09%	0.012%
76	12.239	3472	3483	3492	rBV2	3725	7107	0.43%	0.053%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029996.D
 Acq On : 30 Jan 2023 16:59
 Operator : SY/MD
 Sample : 01314-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	12.336	3508	3513	3522	rVB7	1621	2297	0.14%	0.017%
78	12.471	3553	3555	3563	rVB3	648	481	0.03%	0.004%
79	12.506	3563	3566	3569	rBV3	624	496	0.03%	0.004%
80	12.586	3588	3591	3592	rBV2	572	326	0.02%	0.002%
81	12.718	3630	3632	3635	rBV2	573	361	0.02%	0.003%
82	12.779	3649	3651	3653	rVB2	709	325	0.02%	0.002%
83	12.834	3662	3668	3677	rVV6	3065	4446	0.27%	0.033%
84	12.905	3687	3690	3692	rBV3	788	556	0.03%	0.004%
85	12.972	3709	3711	3713	rVV2	613	277	0.02%	0.002%
86	12.991	3713	3717	3720	rVV4	569	401	0.02%	0.003%
87	13.130	3759	3760	3763	rVV2	643	302	0.02%	0.002%
88	13.162	3767	3770	3777	rVB5	945	1005	0.06%	0.007%
89	13.229	3787	3791	3792	rBV3	572	365	0.02%	0.003%
90	13.310	3813	3816	3818	rVV2	604	354	0.02%	0.003%
91	13.377	3834	3837	3842	rBV4	508	467	0.03%	0.003%
92	13.429	3849	3853	3858	rVB5	1049	949	0.06%	0.007%
93	13.467	3862	3865	3867	rBV4	526	334	0.02%	0.002%
94	13.583	3899	3901	3906	rVB2	545	337	0.02%	0.002%
95	13.612	3906	3910	3912	rBV3	525	513	0.03%	0.004%
96	14.065	4048	4051	4055	rBV5	809	716	0.04%	0.005%
97	14.146	4074	4076	4079	rBV2	560	410	0.02%	0.003%
98	15.368	4449	4456	4464	rBV9	5735	8572	0.51%	0.063%
99	15.760	4570	4578	4591	rBV5	12701	19814	1.19%	0.147%
100	15.940	4627	4634	4643	rBV8	11046	19403	1.16%	0.144%




Sum of corrected areas: 13501003

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029996.D
Acq On : 30 Jan 2023 16:59
Operator : SY/MD
Sample : 01314-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44N9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

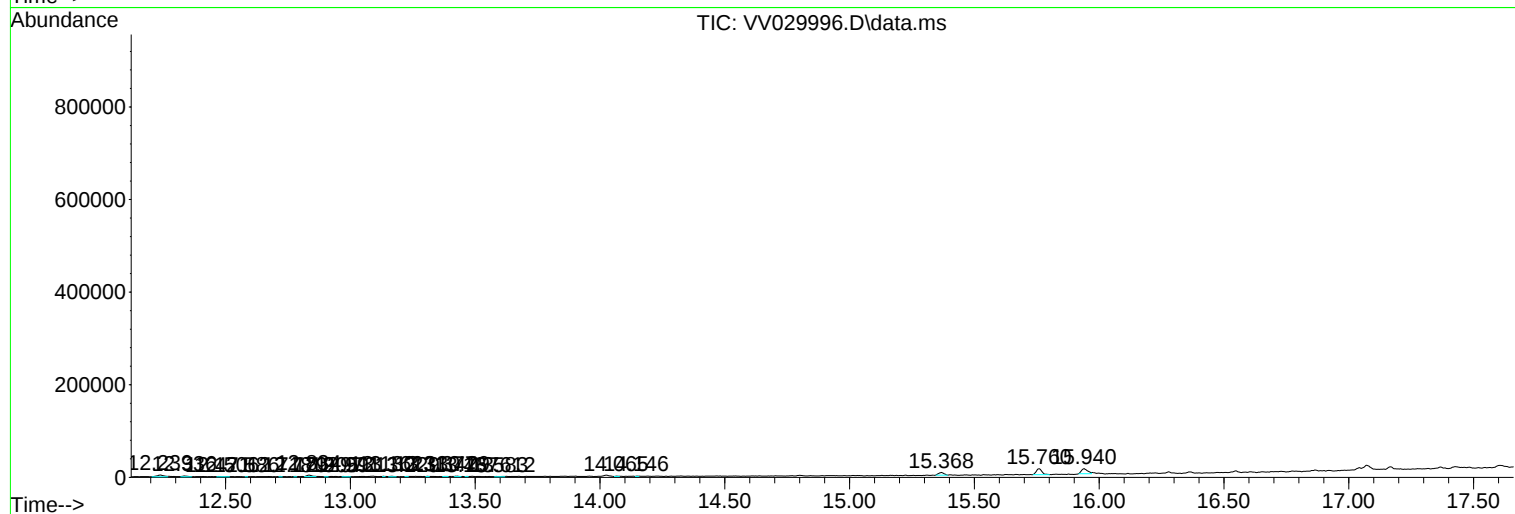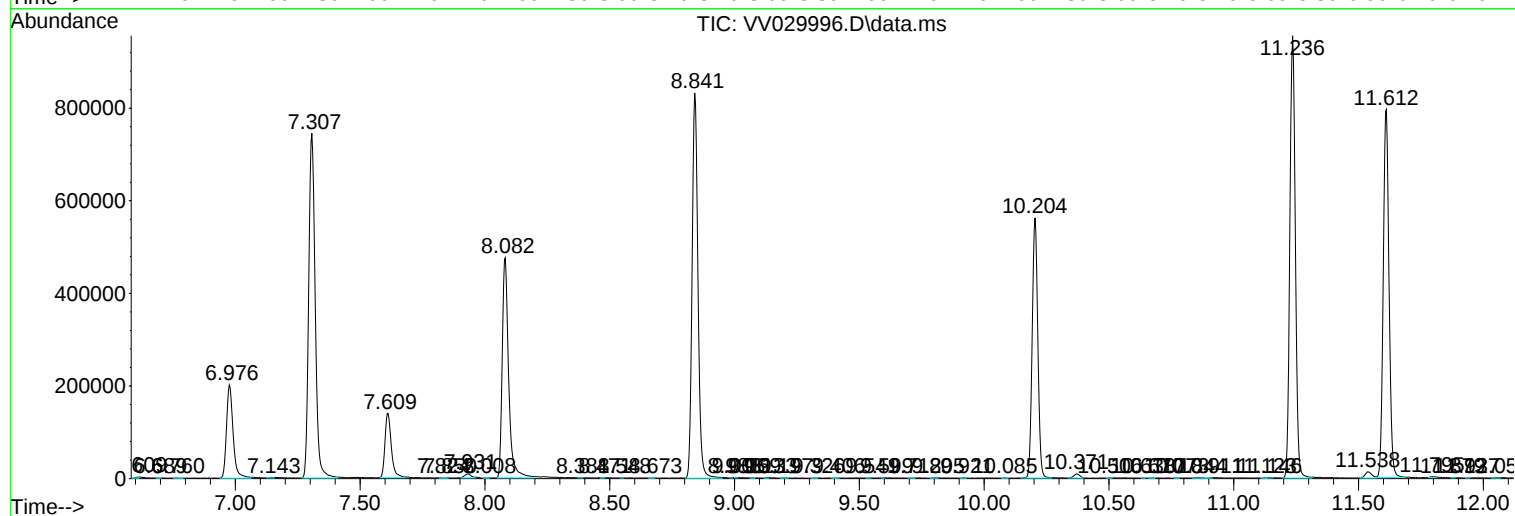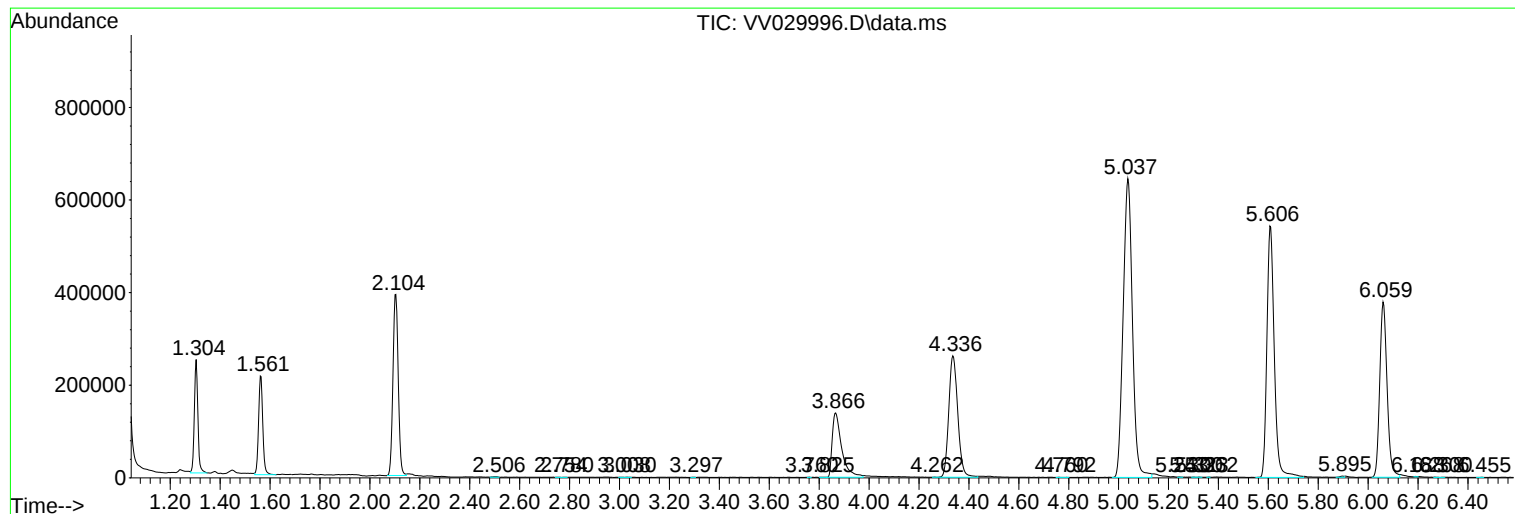

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029996.D
Acq On : 30 Jan 2023 16:59
Operator : SY/MD
Sample : 01314-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44N9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029996.D
Acq On : 30 Jan 2023 16:59
Operator : SY/MD
Sample : 01314-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44N9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc