

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029997.D
 Acq On : 30 Jan 2023 17:23
 Operator : SY/MD
 Sample : 01314-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	230011	235148	8.40%	1.471%
2	1.561	155	162	179	rVB	212772	243737	8.70%	1.524%
3	2.102	321	330	342	rBV	379226	539027	19.25%	3.371%
4	2.500	448	454	461	rVB4	1633	2363	0.08%	0.015%
5	2.899	576	578	583	rVB	347	205	0.01%	0.001%
6	2.928	584	587	588	rBV	326	180	0.01%	0.001%
7	2.963	595	598	602	rVB3	584	324	0.01%	0.002%
8	3.076	631	633	635	rVB	308	110	0.00%	0.001%
9	3.137	649	652	653	rBV	173	102	0.00%	0.001%
10	3.278	691	696	699	rBV2	314	267	0.01%	0.002%
11	3.304	699	704	705	rBV2	287	248	0.01%	0.002%
12	3.336	710	714	715	rBV	285	208	0.01%	0.001%
13	3.423	737	741	743	rBV2	246	191	0.01%	0.001%
14	3.558	778	783	787	rBV3	340	309	0.01%	0.002%
15	3.590	790	793	799	rVB2	401	391	0.01%	0.002%
16	3.626	799	804	810	rBV3	332	425	0.02%	0.003%
17	3.696	823	826	833	rVB3	261	231	0.01%	0.001%
18	3.728	834	836	839	rBV2	297	106	0.00%	0.001%
19	3.745	839	841	844	rBV2	207	144	0.01%	0.001%
20	3.786	852	854	859	rVB2	384	209	0.01%	0.001%
21	3.828	860	867	868	rBV2	510	463	0.02%	0.003%
22	3.867	868	879	916	rBV	131618	393417	14.05%	2.461%
23	4.336	1009	1025	1052	rBV	252863	620679	22.16%	3.882%
24	4.600	1093	1107	1119	rVB4	3567	8912	0.32%	0.056%
25	4.648	1119	1122	1128	rBV3	309	324	0.01%	0.002%
26	4.674	1128	1130	1132	rVB	311	117	0.00%	0.001%
27	4.693	1132	1136	1137	rBV	183	107	0.00%	0.001%
28	4.764	1156	1158	1161	rVB2	395	206	0.01%	0.001%
29	4.786	1161	1165	1167	rBV	243	216	0.01%	0.001%
30	4.831	1177	1179	1180	rVB	128	28	0.00%	0.000%
31	4.841	1180	1182	1187	rVB	282	223	0.01%	0.001%
32	4.867	1187	1190	1194	rBV2	424	367	0.01%	0.002%
33	4.899	1194	1200	1205	rBV4	367	461	0.02%	0.003%
34	4.944	1212	1214	1218	rVB	173	115	0.00%	0.001%
35	4.973	1218	1223	1224	rBV	300	239	0.01%	0.001%
36	5.037	1224	1243	1267	rBV2	615977	1596535	57.01%	9.985%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029997.D
 Acq On : 30 Jan 2023 17:23
 Operator : SY/MD
 Sample : 01314-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	5.346	1335	1339	1341	rBV2	441	368	0.01%	0.002%
38	5.391	1346	1353	1355	rBV3	721	881	0.03%	0.006%
39	5.442	1367	1369	1370	rBV2	154	73	0.00%	0.000%
40	5.507	1387	1389	1391	rBV2	292	111	0.00%	0.001%
41	5.523	1391	1394	1397	rVB3	410	226	0.01%	0.001%
42	5.539	1397	1399	1400	rBV	127	63	0.00%	0.000%
43	5.558	1403	1405	1406	rVB	173	49	0.00%	0.000%
44	5.606	1406	1420	1444	rBV	530228	1069987	38.21%	6.692%
45	5.902	1498	1512	1547	rBV	1436839	2800356	100.00%	17.514%
46	6.060	1549	1561	1580	rVV	363867	720816	25.74%	4.508%
47	6.310	1637	1639	1641	rBV2	364	163	0.01%	0.001%
48	6.397	1663	1666	1669	rBV3	300	182	0.01%	0.001%
49	6.613	1726	1733	1735	rBV5	1770	2253	0.08%	0.014%
50	6.719	1764	1766	1768	rBV2	290	170	0.01%	0.001%
51	6.767	1778	1781	1784	rBV2	232	130	0.00%	0.001%
52	6.844	1802	1805	1807	rBV	169	86	0.00%	0.001%
53	6.857	1807	1809	1811	rBV2	169	98	0.00%	0.001%
54	6.896	1817	1821	1824	rBV3	350	331	0.01%	0.002%
55	6.976	1834	1846	1871	rBV	195048	352933	12.60%	2.207%
56	7.140	1892	1897	1898	rBV3	1197	845	0.03%	0.005%
57	7.307	1935	1949	1974	rBV	713499	1254482	44.80%	7.846%
58	7.609	2033	2043	2065	rBV	135104	236646	8.45%	1.480%
59	7.928	2131	2142	2154	rBV4	9794	19318	0.69%	0.121%
60	8.079	2178	2189	2224	rBV	446890	791888	28.28%	4.953%
61	8.609	2351	2354	2355	rBV2	369	207	0.01%	0.001%
62	8.728	2386	2391	2394	rBV3	665	617	0.02%	0.004%
63	8.841	2411	2426	2450	rBV	821357	1344878	48.03%	8.411%
64	9.053	2489	2492	2493	rBV2	633	374	0.01%	0.002%
65	9.236	2547	2549	2552	rVB2	403	162	0.01%	0.001%
66	9.281	2562	2563	2569	rVB3	382	227	0.01%	0.001%
67	9.310	2569	2572	2575	rBV3	275	193	0.01%	0.001%
68	9.365	2585	2589	2591	rVB	359	166	0.01%	0.001%
69	9.526	2636	2639	2643	rBV3	652	545	0.02%	0.003%
70	9.616	2665	2667	2668	rBV	408	145	0.01%	0.001%
71	9.651	2675	2678	2683	rBV3	648	685	0.02%	0.004%
72	9.699	2691	2693	2696	rBV2	412	317	0.01%	0.002%
73	9.870	2744	2746	2749	rVB2	728	367	0.01%	0.002%
74	10.014	2789	2791	2794	rBV3	389	218	0.01%	0.001%
75	10.082	2808	2812	2814	rBV4	306	243	0.01%	0.002%
76	10.204	2837	2850	2872	rVB	538460	840361	30.01%	5.256%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029997.D
 Acq On : 30 Jan 2023 17:23
 Operator : SY/MD
 Sample : 01314-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	10.371	2892	2902	2913	rVB2	11773	19495	0.70%	0.122%
78	10.564	2958	2962	2964	rBV2	566	500	0.02%	0.003%
79	10.728	3011	3013	3018	rBV3	425	392	0.01%	0.002%
80	11.169	3143	3150	3159	rVB3	11951	18117	0.65%	0.113%
81	11.236	3159	3171	3197	rBV	933229	1440182	51.43%	9.007%
82	11.493	3248	3251	3252	rBV	352	145	0.01%	0.001%
83	11.535	3255	3264	3275	rBV3	16112	29607	1.06%	0.185%
84	11.612	3276	3288	3312	rVB	776540	1331368	47.54%	8.327%
85	12.407	3532	3535	3537	rBV	259	167	0.01%	0.001%
86	12.419	3537	3539	3540	rBV	346	129	0.00%	0.001%
87	12.622	3593	3602	3619	rBV	31389	53651	1.92%	0.336%
88	13.249	3791	3797	3804	rVB6	4911	6787	0.24%	0.042%




Sum of corrected areas: 15989034

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029997.D
Acq On : 30 Jan 2023 17:23
Operator : SY/MD
Sample : 01314-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

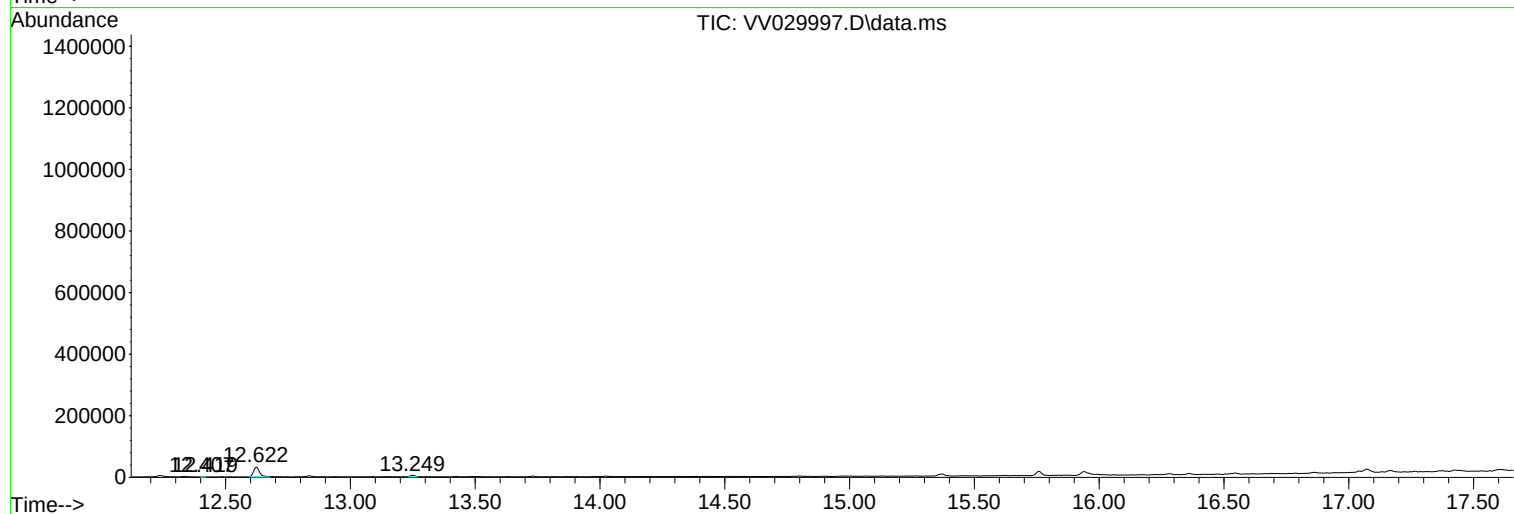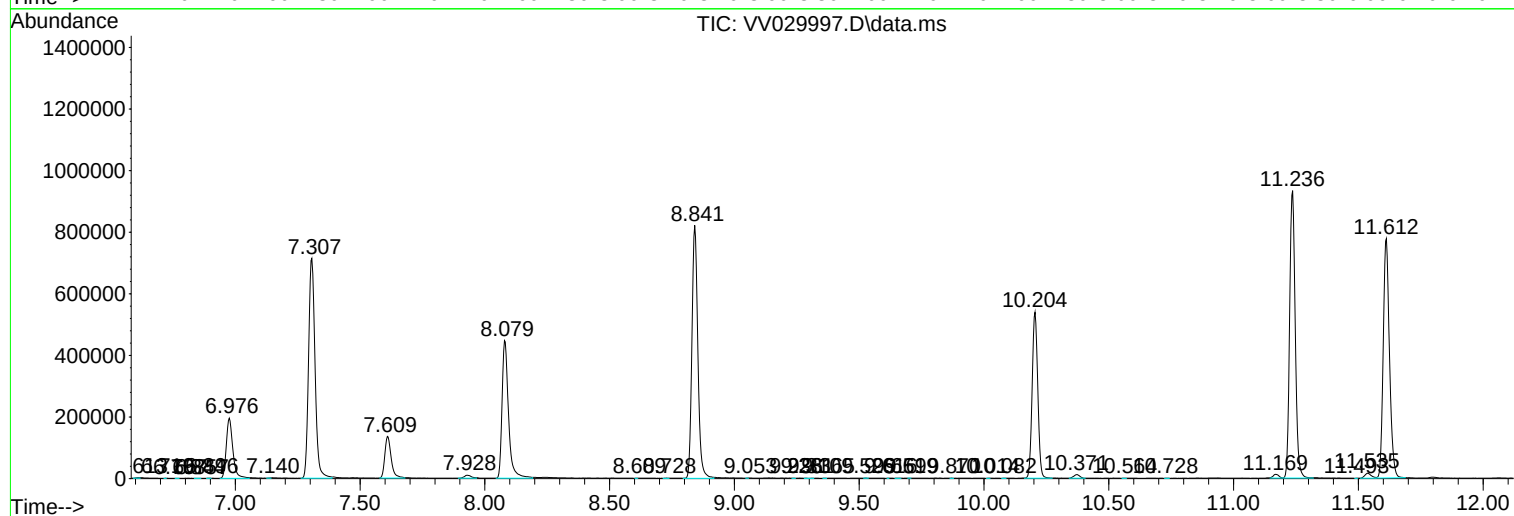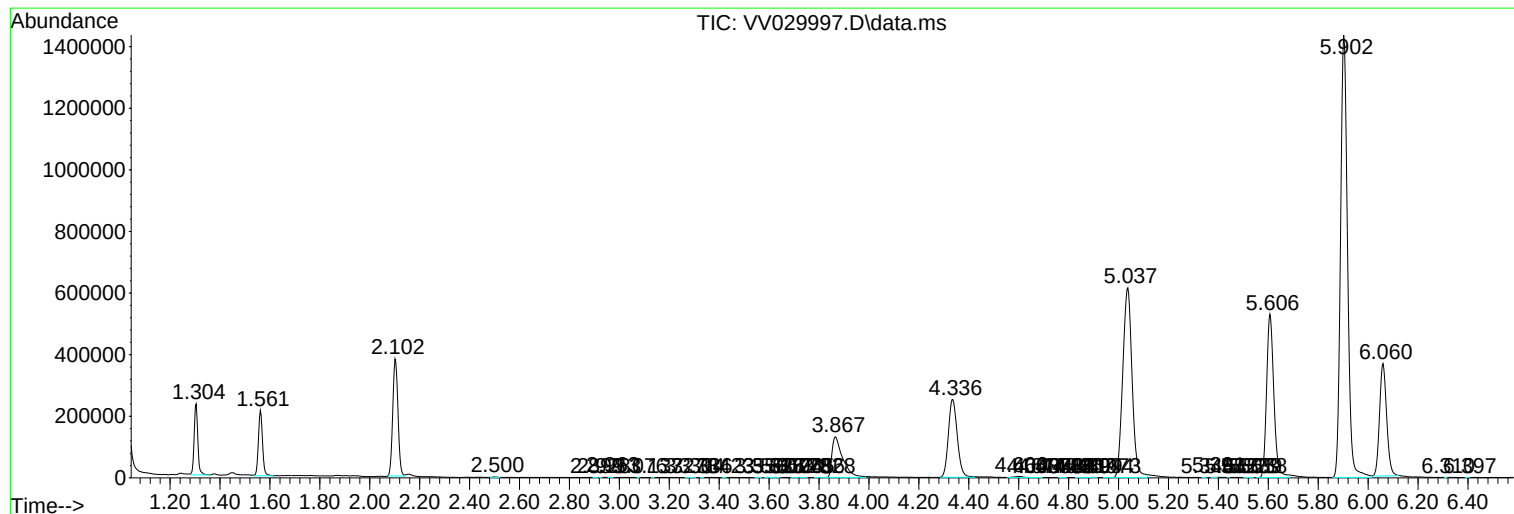

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029997.D
Acq On : 30 Jan 2023 17:23
Operator : SY/MD
Sample : 01314-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029997.D
Acq On : 30 Jan 2023 17:23
Operator : SY/MD
Sample : 01314-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc