

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029998.D
 Acq On : 30 Jan 2023 17:47
 Operator : SY/MD
 Sample : 01314-11DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	226875	234938	7.95%	1.497%
2	1.561	154	162	178	rVB	204718	235732	7.97%	1.502%
3	2.101	320	330	343	rBV	380461	540743	18.29%	3.445%
4	2.500	445	454	466	rVB4	3208	5068	0.17%	0.032%
5	2.757	530	534	536	rBV3	412	381	0.01%	0.002%
6	2.844	558	561	564	rBV3	315	267	0.01%	0.002%
7	2.960	594	597	601	rBV3	297	261	0.01%	0.002%
8	3.281	689	697	701	rVB3	301	404	0.01%	0.003%
9	3.339	711	715	719	rVV2	307	295	0.01%	0.002%
10	3.365	719	723	728	rVB2	481	384	0.01%	0.002%
11	3.658	812	814	819	rVB2	268	260	0.01%	0.002%
12	3.693	819	825	826	rBV2	372	275	0.01%	0.002%
13	3.731	835	837	842	rVB3	343	256	0.01%	0.002%
14	3.760	842	846	848	rBV2	465	335	0.01%	0.002%
15	3.867	867	879	914	rBV	143627	466633	15.78%	2.973%
16	4.272	1000	1005	1007	rBV3	532	450	0.02%	0.003%
17	4.336	1007	1025	1048	rBV	256904	629908	21.30%	4.013%
18	4.706	1135	1140	1142	rBV4	315	301	0.01%	0.002%
19	4.764	1155	1158	1164	rBV3	370	386	0.01%	0.002%
20	4.786	1164	1165	1171	rVB2	372	272	0.01%	0.002%
21	5.037	1223	1243	1271	rBV2	620353	1611181	54.49%	10.265%
22	5.204	1293	1295	1297	rBV3	521	263	0.01%	0.002%
23	5.342	1334	1338	1341	rBV3	418	265	0.01%	0.002%
24	5.397	1353	1355	1360	rVB3	835	773	0.03%	0.005%
25	5.448	1367	1371	1374	rBV4	466	403	0.01%	0.003%
26	5.474	1376	1379	1384	rVB2	497	322	0.01%	0.002%
27	5.526	1392	1395	1399	rBV2	374	262	0.01%	0.002%
28	5.548	1399	1402	1405	rVB2	456	251	0.01%	0.002%
29	5.606	1405	1420	1445	rBV	535115	1077794	36.45%	6.867%
30	5.905	1499	1513	1546	rBV	278500	552010	18.67%	3.517%
31	6.059	1547	1561	1594	rVV	369752	749019	25.33%	4.772%
32	6.493	1692	1696	1700	rBV3	300	267	0.01%	0.002%
33	6.609	1723	1732	1735	rBV6	1899	2484	0.08%	0.016%
34	6.677	1751	1753	1757	rVB3	446	320	0.01%	0.002%
35	6.792	1782	1789	1791	rBV2	369	246	0.01%	0.002%
36	6.837	1801	1803	1809	rVB3	332	316	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029998.D
 Acq On : 30 Jan 2023 17:47
 Operator : SY/MD
 Sample : 01314-11DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	6.976	1832	1846	1872	rBV	192475	353973	11.97%	2.255%
38	7.146	1893	1899	1903	rBV6	1090	1259	0.04%	0.008%
39	7.307	1934	1949	1983	rBV	721472	1266894	42.85%	8.071%
40	7.542	2020	2022	2030	rVB5	718	683	0.02%	0.004%
41	7.609	2032	2043	2065	rBV	136074	237527	8.03%	1.513%
42	7.744	2082	2085	2087	rBV4	501	266	0.01%	0.002%
43	7.934	2137	2144	2151	rVB2	2360	3745	0.13%	0.024%
44	7.963	2151	2153	2155	rBV3	728	355	0.01%	0.002%
45	8.079	2178	2189	2221	rBV	465604	801884	27.12%	5.109%
46	8.587	2343	2347	2353	rVB4	375	345	0.01%	0.002%
47	8.641	2360	2364	2367	rBV3	475	465	0.02%	0.003%
48	8.841	2412	2426	2456	rBV	818913	1370097	46.34%	8.729%
49	8.969	2464	2466	2470	rBV3	498	390	0.01%	0.002%
50	9.127	2512	2515	2518	rVB4	665	393	0.01%	0.003%
51	9.175	2527	2530	2534	rBV2	611	494	0.02%	0.003%
52	9.230	2544	2547	2551	rVB3	499	427	0.01%	0.003%
53	9.529	2632	2640	2643	rBV5	500	791	0.03%	0.005%
54	9.545	2643	2645	2649	rVB3	547	412	0.01%	0.003%
55	9.567	2649	2652	2657	rBV4	850	708	0.02%	0.005%
56	9.612	2663	2666	2669	rBV3	452	272	0.01%	0.002%
57	9.754	2704	2710	2713	rBV4	308	306	0.01%	0.002%
58	9.799	2722	2724	2727	rBV	591	378	0.01%	0.002%
59	9.831	2731	2734	2737	rBV2	445	302	0.01%	0.002%
60	9.924	2759	2763	2767	rVV3	372	400	0.01%	0.003%
61	10.008	2786	2789	2793	rVB	405	271	0.01%	0.002%
62	10.091	2811	2815	2818	rBV4	324	353	0.01%	0.002%
63	10.159	2831	2836	2837	rBV2	755	548	0.02%	0.003%
64	10.204	2838	2850	2871	rVB	538404	850332	28.76%	5.418%
65	10.323	2883	2887	2893	rBV3	584	545	0.02%	0.003%
66	10.365	2895	2900	2910	rVB5	1757	2926	0.10%	0.019%
67	10.516	2942	2947	2952	rVB4	599	504	0.02%	0.003%
68	10.564	2960	2962	2964	rBV2	395	250	0.01%	0.002%
69	10.715	3005	3009	3012	rBV2	361	323	0.01%	0.002%
70	10.776	3024	3028	3033	rVB3	328	297	0.01%	0.002%
71	10.824	3038	3043	3044	rBV2	342	325	0.01%	0.002%
72	10.844	3044	3049	3053	rBV7	790	935	0.03%	0.006%
73	10.911	3066	3070	3073	rBV3	679	615	0.02%	0.004%
74	11.033	3102	3108	3118	rVB5	809	1288	0.04%	0.008%
75	11.101	3125	3129	3131	rBV2	289	247	0.01%	0.002%
76	11.172	3136	3151	3159	rBV2	10642	17248	0.58%	0.110%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029998.D
 Acq On : 30 Jan 2023 17:47
 Operator : SY/MD
 Sample : 01314-11DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44L7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	11.236	3159	3171	3193	rBV2	937586	1619217	54.76%	10.316%
78	11.413	3224	3226	3229	rVB2	848	446	0.02%	0.003%
79	11.474	3242	3245	3250	rVB5	397	371	0.01%	0.002%
80	11.538	3260	3265	3266	rBV2	1236	896	0.03%	0.006%
81	11.625	3275	3292	3328	rBV2	1333902	2956804	100.00%	18.838%
82	11.802	3340	3347	3351	rBV4	2448	3444	0.12%	0.022%
83	12.030	3415	3418	3421	rBV3	457	265	0.01%	0.002%
84	12.059	3421	3427	3430	rBV3	1130	1153	0.04%	0.007%
85	12.233	3472	3481	3485	rBV5	2285	3254	0.11%	0.021%
86	12.326	3507	3510	3511	rBV	649	346	0.01%	0.002%
87	12.390	3525	3530	3533	rBV3	663	499	0.02%	0.003%
88	12.631	3598	3605	3614	rBV9	2086	3617	0.12%	0.023%
89	12.834	3663	3668	3676	rVB8	3164	4287	0.14%	0.027%
90	12.914	3690	3693	3696	rBV2	612	412	0.01%	0.003%
91	12.947	3699	3703	3706	rVB4	815	719	0.02%	0.005%
92	13.249	3787	3797	3806	rBV3	6941	10966	0.37%	0.070%
93	13.625	3912	3914	3919	rBV3	433	318	0.01%	0.002%
94	13.728	3941	3946	3954	rBV6	1963	2619	0.09%	0.017%
95	13.937	4009	4011	4014	rBV4	516	248	0.01%	0.002%
96	14.024	4030	4038	4050	rBV3	2889	5532	0.19%	0.035%
97	14.377	4145	4148	4150	rBV3	611	371	0.01%	0.002%
98	15.368	4450	4456	4467	rVB3	5552	8397	0.28%	0.053%
99	15.757	4573	4577	4587	rVB5	10869	14706	0.50%	0.094%
100	15.940	4627	4634	4647	rBV5	11391	23522	0.80%	0.150%




Sum of corrected areas: 15695907

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029998.D
Acq On : 30 Jan 2023 17:47
Operator : SY/MD
Sample : 01314-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

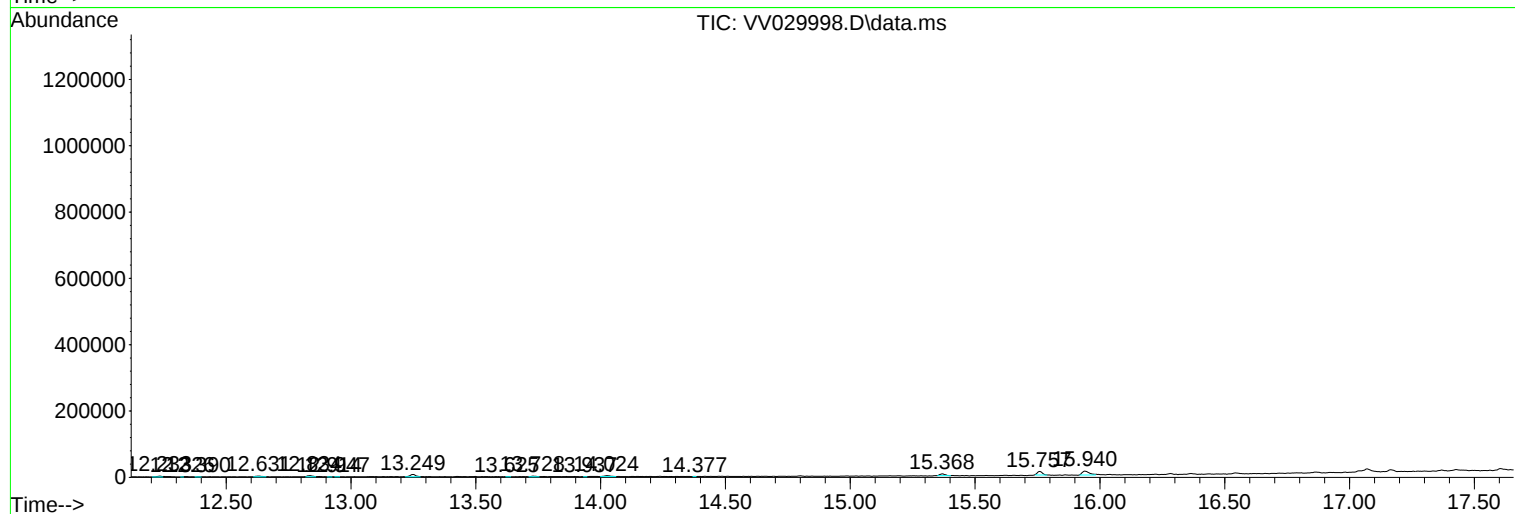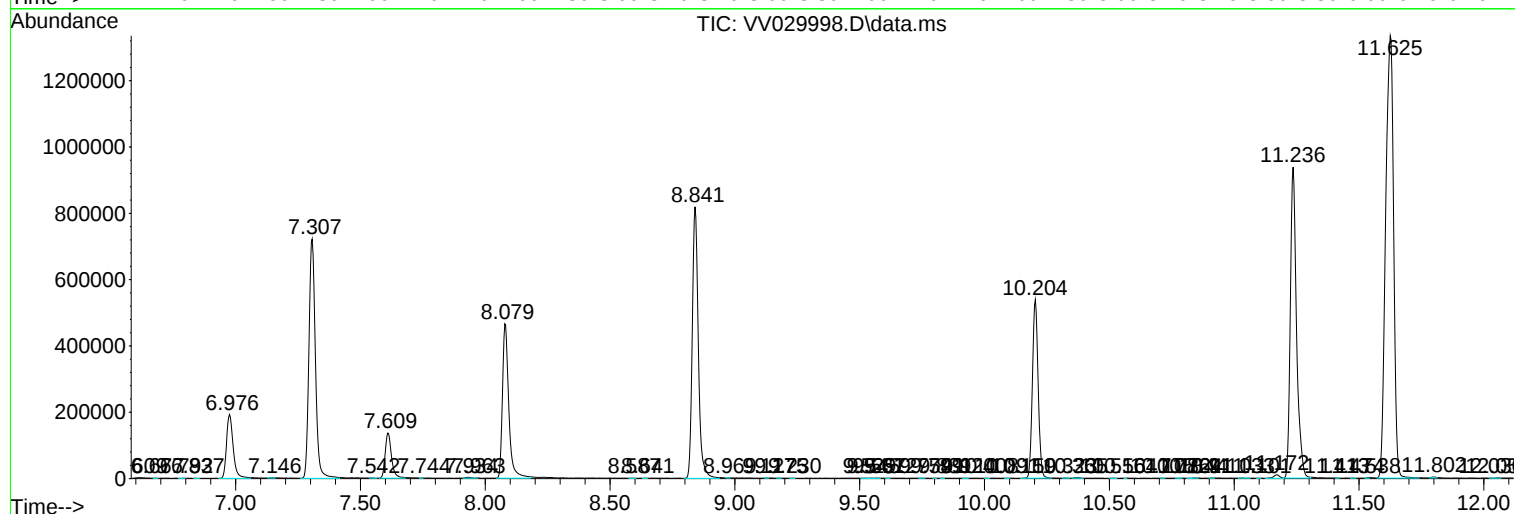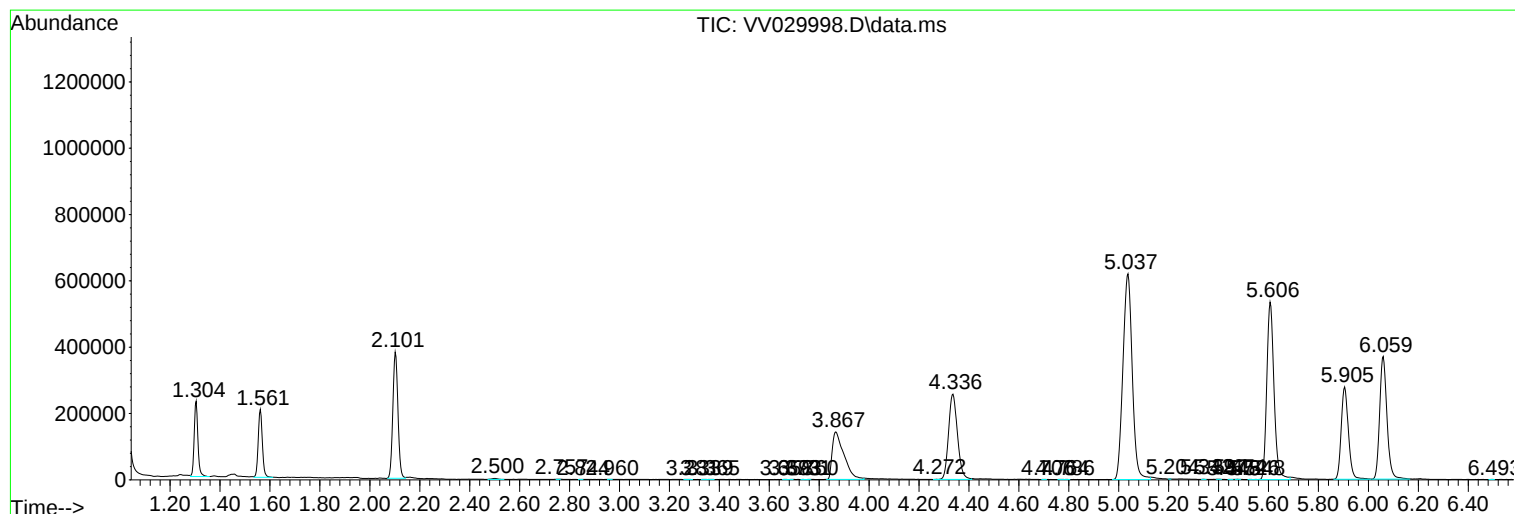

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029998.D
Acq On : 30 Jan 2023 17:47
Operator : SY/MD
Sample : 01314-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029998.D
Acq On : 30 Jan 2023 17:47
Operator : SY/MD
Sample : 01314-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44L7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc