

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029999.D
 Acq On : 30 Jan 2023 18:10
 Operator : SY/MD
 Sample : 01295-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

Signal : TIC: VV029999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	224693	225261	14.58%	1.796%
2	1.561	155	162	180	rVB	201410	229793	14.88%	1.832%
3	2.101	321	330	343	rBV	363475	514113	33.28%	4.098%
4	2.912	577	582	584	rBV3	300	237	0.02%	0.002%
5	2.941	585	591	594	rBV3	546	626	0.04%	0.005%
6	3.031	616	619	621	rVB2	300	169	0.01%	0.001%
7	3.175	661	664	665	rBV	220	120	0.01%	0.001%
8	3.339	712	715	718	rBV2	301	243	0.02%	0.002%
9	3.397	730	733	738	rVB3	384	282	0.02%	0.002%
10	3.426	739	742	745	rBV2	248	210	0.01%	0.002%
11	3.523	769	772	775	rBV3	385	280	0.02%	0.002%
12	3.542	776	778	781	rVV	407	211	0.01%	0.002%
13	3.561	781	784	789	rVB2	386	303	0.02%	0.002%
14	3.590	789	793	799	rVB2	330	364	0.02%	0.003%
15	3.638	805	808	810	rBV	174	109	0.01%	0.001%
16	3.651	810	812	814	rBV	193	87	0.01%	0.001%
17	3.741	835	840	844	rBV3	382	423	0.03%	0.003%
18	3.818	862	864	867	rBV2	348	246	0.02%	0.002%
19	3.867	868	879	915	rBV	128757	343468	22.23%	2.738%
20	4.336	1007	1025	1049	rBV	246788	603939	39.09%	4.815%
21	4.677	1129	1131	1133	rBV	221	117	0.01%	0.001%
22	4.731	1146	1148	1151	rBV	130	56	0.00%	0.000%
23	4.748	1151	1153	1158	rVB2	316	171	0.01%	0.001%
24	4.770	1158	1160	1162	rBV	169	88	0.01%	0.001%
25	4.789	1162	1166	1167	rBV2	200	140	0.01%	0.001%
26	4.844	1181	1183	1184	rBV	160	70	0.00%	0.001%
27	4.892	1197	1198	1202	rVB2	270	173	0.01%	0.001%
28	4.921	1202	1207	1212	rBV2	307	310	0.02%	0.002%
29	5.037	1224	1243	1266	rBV2	596712	1544802	100.00%	12.315%
30	5.375	1342	1348	1352	rBV7	709	736	0.05%	0.006%
31	5.397	1352	1355	1358	rBV3	476	319	0.02%	0.003%
32	5.461	1371	1375	1379	rBV2	617	718	0.05%	0.006%
33	5.522	1391	1394	1399	rBV3	439	411	0.03%	0.003%
34	5.606	1404	1420	1456	rBV	528006	1070914	69.32%	8.537%
35	5.960	1527	1530	1534	rBV2	358	300	0.02%	0.002%
36	6.059	1547	1561	1596	rBV	356418	726801	47.05%	5.794%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029999.D
 Acq On : 30 Jan 2023 18:10
 Operator : SY/MD
 Sample : 01295-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

37	6.275	1626	1628	1630	rBV	208	113	0.01%	0.001%
38	6.371	1656	1658	1663	rBV3	257	187	0.01%	0.001%
39	6.436	1675	1678	1682	rBV	236	160	0.01%	0.001%
40	6.471	1687	1689	1692	rBV	292	196	0.01%	0.002%
41	6.510	1698	1701	1707	rVB2	306	250	0.02%	0.002%
42	6.535	1707	1709	1711	rVV2	225	112	0.01%	0.001%
43	6.551	1711	1714	1716	rVB2	378	181	0.01%	0.001%
44	6.609	1725	1732	1740	rBV5	1953	3894	0.25%	0.031%
45	6.738	1769	1772	1775	rVB2	253	187	0.01%	0.001%
46	6.770	1775	1782	1785	rBV3	322	337	0.02%	0.003%
47	6.789	1785	1788	1792	rVV3	528	415	0.03%	0.003%
48	6.815	1792	1796	1800	rVB3	371	286	0.02%	0.002%
49	6.850	1805	1807	1810	rBV2	526	313	0.02%	0.002%
50	6.899	1820	1822	1828	rVB	207	142	0.01%	0.001%
51	6.924	1828	1830	1832	rBV	156	70	0.00%	0.001%
52	6.976	1833	1846	1878	rBV	184298	341329	22.10%	2.721%
53	7.249	1926	1931	1936	rBV2	579	475	0.03%	0.004%
54	7.307	1936	1949	1972	rBV	690912	1206406	78.09%	9.617%
55	7.497	2005	2008	2010	rBV3	592	400	0.03%	0.003%
56	7.609	2033	2043	2065	rBV	127706	225720	14.61%	1.799%
57	7.741	2081	2084	2087	rBV2	580	315	0.02%	0.003%
58	7.854	2117	2119	2122	rVB3	268	170	0.01%	0.001%
59	7.873	2122	2125	2126	rBV	387	212	0.01%	0.002%
60	7.985	2159	2160	2162	rBV	282	99	0.01%	0.001%
61	8.018	2168	2170	2173	rBV2	281	150	0.01%	0.001%
62	8.079	2178	2189	2224	rBV	445564	781114	50.56%	6.227%
63	8.493	2316	2318	2320	rBV	295	135	0.01%	0.001%
64	8.600	2348	2351	2352	rBV	388	221	0.01%	0.002%
65	8.622	2356	2358	2361	rVV	509	307	0.02%	0.002%
66	8.657	2365	2369	2372	rBV4	500	346	0.02%	0.003%
67	8.699	2379	2382	2384	rBV	283	178	0.01%	0.001%
68	8.841	2414	2426	2455	rBV	814245	1307769	84.66%	10.425%
69	9.101	2504	2507	2509	rBV	315	210	0.01%	0.002%
70	9.188	2531	2534	2536	rVB3	527	248	0.02%	0.002%
71	9.297	2566	2568	2572	rBV3	297	176	0.01%	0.001%
72	9.336	2577	2580	2581	rBV	311	165	0.01%	0.001%
73	9.384	2592	2595	2598	rVB2	333	235	0.02%	0.002%
74	9.403	2598	2601	2602	rBV2	196	117	0.01%	0.001%
75	9.413	2602	2604	2606	rVB	378	199	0.01%	0.002%
76	9.452	2613	2616	2621	rVB3	359	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
 Data File : VV029999.D
 Acq On : 30 Jan 2023 18:10
 Operator : SY/MD
 Sample : 01295-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
 Title : VOC Analysis

77	9.487	2624	2627	2630	rVV3	387	267	0.02%	0.002%
78	9.538	2641	2643	2646	rVB2	504	272	0.02%	0.002%
79	9.554	2646	2648	2650	rBV2	328	130	0.01%	0.001%
80	9.609	2663	2665	2668	rBV3	432	272	0.02%	0.002%
81	9.664	2681	2682	2685	rBV2	158	109	0.01%	0.001%
82	9.722	2697	2700	2703	rBV2	288	233	0.02%	0.002%
83	9.956	2769	2773	2776	rBV3	333	209	0.01%	0.002%
84	10.043	2797	2800	2802	rBV3	353	189	0.01%	0.002%
85	10.085	2811	2813	2815	rBV	209	71	0.00%	0.001%
86	10.127	2824	2826	2827	rBV	290	123	0.01%	0.001%
87	10.204	2838	2850	2872	rVB	524223	817238	52.90%	6.515%
88	10.423	2914	2918	2920	rBV	405	287	0.02%	0.002%
89	10.435	2920	2922	2925	rBV	375	259	0.02%	0.002%
90	10.596	2970	2972	2975	rBV2	524	374	0.02%	0.003%
91	10.728	3008	3013	3020	rBV4	465	629	0.04%	0.005%
92	10.847	3045	3050	3054	rBV3	965	1216	0.08%	0.010%
93	11.236	3159	3171	3196	rBV	925549	1402730	90.80%	11.182%
94	11.612	3275	3288	3316	rBV	744486	1170836	75.79%	9.334%
95	11.799	3338	3346	3360	rBV6	2768	5606	0.36%	0.045%
96	12.329	3509	3511	3512	rBV2	842	359	0.02%	0.003%
97	12.500	3561	3564	3567	rBV2	644	596	0.04%	0.005%
98	13.072	3738	3742	3744	rBV2	958	740	0.05%	0.006%
99	13.140	3760	3763	3766	rBV3	586	568	0.04%	0.005%
100	13.291	3807	3810	3811	rBV2	578	330	0.02%	0.003%




Sum of corrected areas: 12544018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029999.D
Acq On : 30 Jan 2023 18:10
Operator : SY/MD
Sample : 01295-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

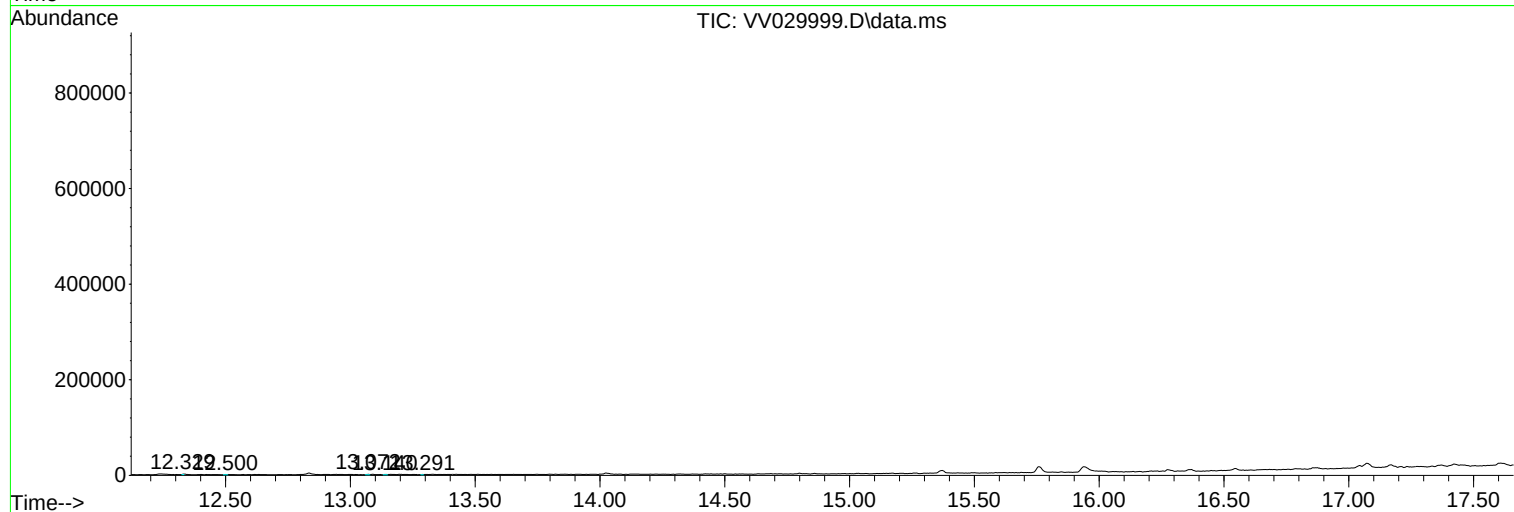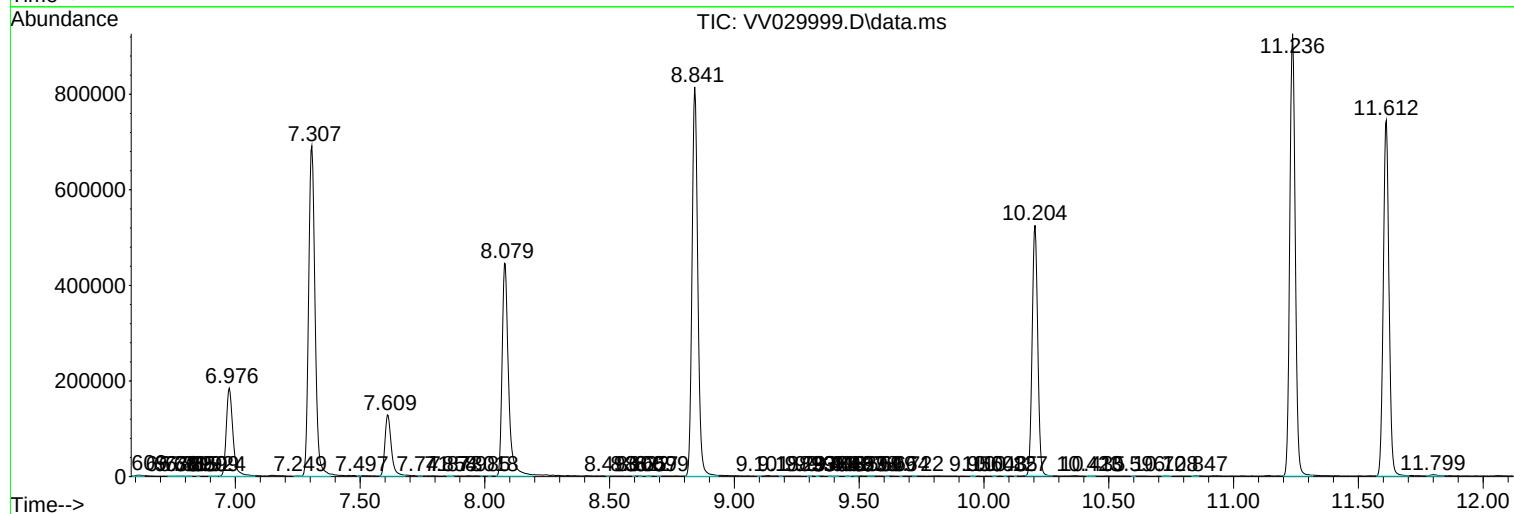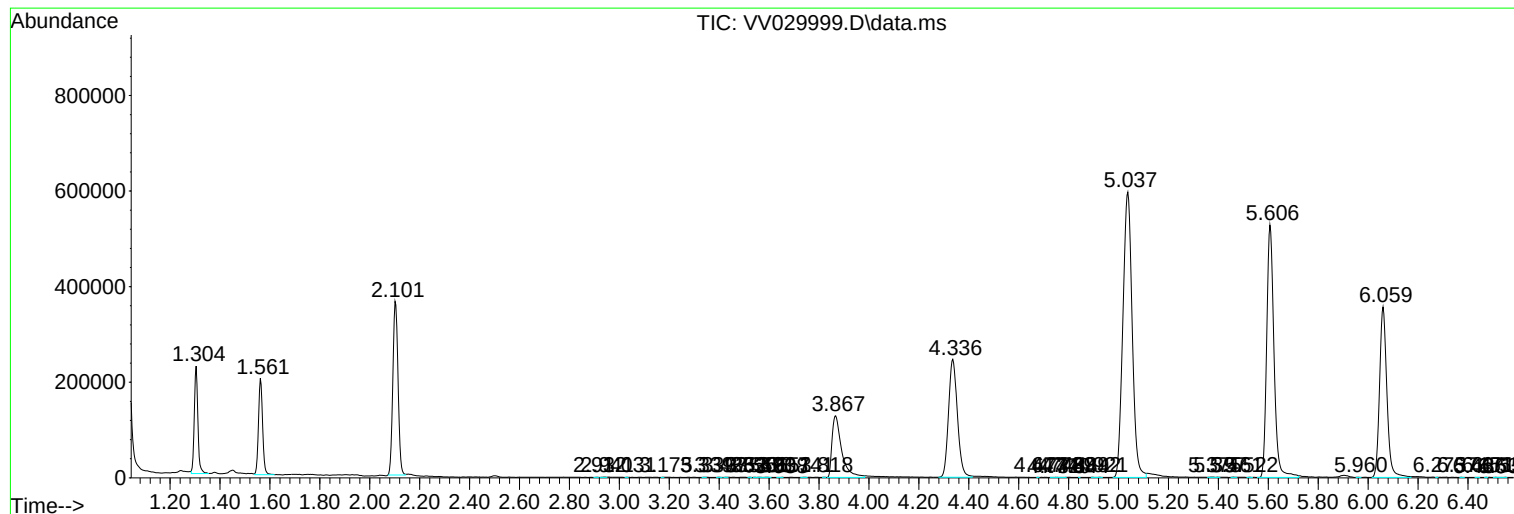

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029999.D
Acq On : 30 Jan 2023 18:10
Operator : SY/MD
Sample : 01295-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029999.D
Acq On : 30 Jan 2023 18:10
Operator : SY/MD
Sample : 01295-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc