


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013023\
Data File : VV029980.D
Acq On : 30 Jan 2023 09:36
Operator : SY/MD
Sample : BFB362
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB362

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Title : VOC Analysis
Last Update : Tue Jan 31 02:16:13 2023

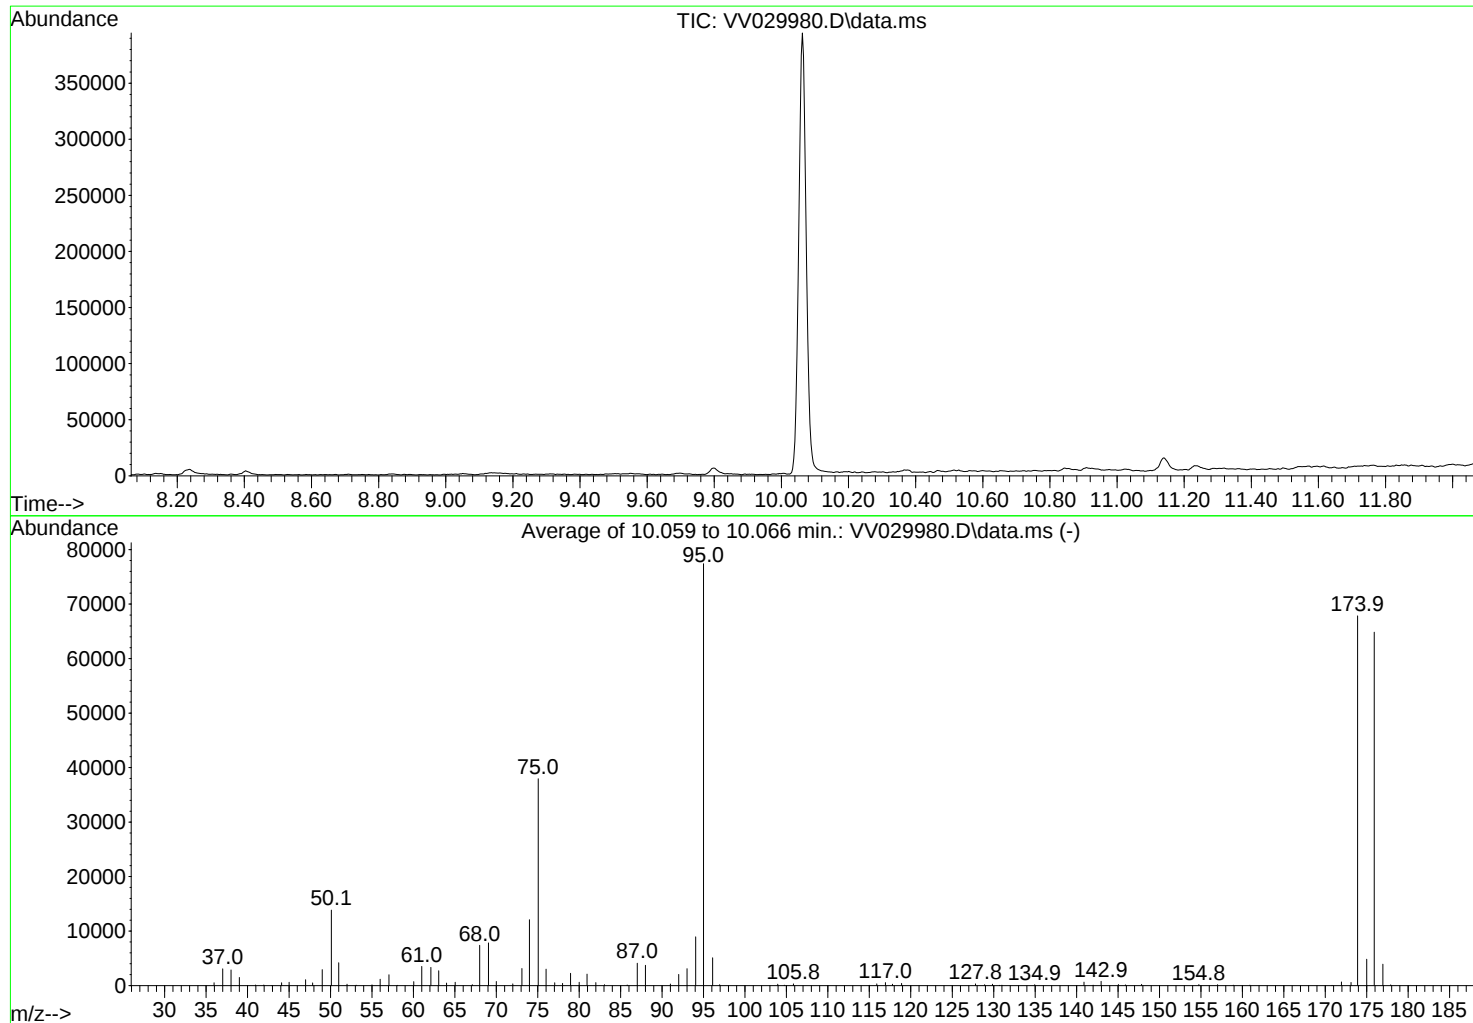

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	13855	PASS
75	95	30	80	49.0	37936	PASS
95	95	100	100	100.0	77405	PASS
96	95	5	9	6.6	5101	PASS
173	174	0.00	2	0.8	574	PASS
174	95	50	120	87.6	67835	PASS
175	174	5	9	7.1	4829	PASS
176	174	95	105	95.6	64856	PASS
177	176	5	10	6.1	3925	PASS

m/z	Abundance
35.00	137.0
40.00	394.0
40.90	139.0
43.00	168.0
43.90	431.0
55.00	173.0
81.00	101.0
91.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
36.00	642.0
37.00	3198.0
38.00	2855.0
39.00	1475.0
40.00	384.0
41.00	207.0
42.00	108.0
42.90	234.0
43.90	692.0
45.00	603.0
47.00	1075.0
47.90	430.0
49.00	2916.0
50.10	13948.0
51.00	4309.0
52.00	269.0
53.10	127.0
55.00	295.0
56.00	1105.0
57.00	1965.0
60.10	773.0
61.00	3455.0
62.10	3503.0
63.10	2676.0
64.00	442.0
65.10	543.0
67.10	253.0
68.00	7071.0
69.10	7998.0
70.00	824.0
72.00	336.0
73.10	3124.0
74.00	12010.0
75.00	37592.0
76.00	3020.0
77.00	458.0
78.00	414.0
79.00	2112.0
80.00	680.0
81.00	2126.0
82.00	513.0
83.00	165.0
85.80	100.0
87.00	4232.0
88.00	3680.0
91.00	416.0
92.00	2022.0
93.00	3001.0
94.00	9029.0
95.00	76496.0
96.10	5194.0
97.00	191.0
104.00	271.0
105.80	287.0
115.90	304.0
116.90	545.0
117.80	232.0
118.90	433.0
127.80	322.0
128.90	156.0
129.90	264.0
130.70	127.0
131.00	124.0
134.90	163.0
140.90	661.0
142.00	103.0
142.90	788.0
145.10	207.0
145.90	129.0
147.80	201.0
154.70	173.0
157.00	139.0
160.90	111.0
172.00	647.0
173.10	839.0
173.90	65232.0
175.00	4711.0
175.90	62480.0
177.00	3812.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
36.00	679.0
37.00	3176.0
38.00	2944.0
39.00	1590.0
40.00	385.0
41.00	253.0
41.90	117.0
42.90	184.0
44.10	736.0
45.00	644.0
47.00	1095.0
47.80	468.0
49.00	3018.0
50.10	14371.0
51.00	4335.0
52.00	272.0
53.10	109.0
55.00	313.0
56.00	1191.0
57.00	2038.0
60.00	744.0
61.00	3628.0
62.10	3419.0
63.00	2846.0
64.00	489.0
65.00	610.0
67.10	241.0
68.00	7641.0
69.10	8071.0
70.00	799.0
72.00	311.0
73.10	3272.0
74.00	12533.0
75.00	39304.0
76.00	3098.0
77.10	535.0
78.00	413.0
78.90	2350.0
80.00	594.0
80.90	2223.0
82.00	555.0
83.00	163.0
85.80	109.0
87.00	4233.0
88.00	3848.0
91.00	397.0
92.00	2092.0
93.00	3199.0
94.00	9200.0
95.00	80008.0
96.10	5286.0
96.90	179.0
103.90	268.0
104.80	110.0
105.90	308.0
115.00	102.0
115.90	323.0
116.90	533.0
117.80	253.0
118.90	417.0
127.80	323.0
128.90	181.0
129.80	264.0
131.00	131.0
135.00	178.0
140.90	677.0
142.00	109.0
142.90	809.0
145.00	190.0
145.90	127.0
147.90	230.0
154.80	176.0
157.00	154.0
158.90	105.0
160.90	105.0
171.90	706.0
173.10	884.0
173.90	70504.0
175.00	4979.0
175.90	67144.0
177.00	4041.0
177.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
36.00	670.0
37.00	2860.0
38.00	2802.0
39.00	1422.0
40.00	405.0
41.00	266.0
41.90	120.0
43.00	169.0
44.10	818.0
45.00	596.0
47.00	1027.0
47.80	517.0
49.00	2809.0
50.10	13247.0
51.00	3951.0
52.00	261.0
55.00	310.0
56.00	1153.0
57.10	1977.0
58.10	117.0
60.00	641.0
61.00	3487.0
62.10	3066.0
63.10	2670.0
64.00	437.0
65.00	653.0
68.00	7438.0
69.00	7388.0
70.00	656.0
72.00	279.0
73.10	3028.0
74.00	11744.0
75.10	36912.0
76.00	2939.0
77.10	549.0
78.00	377.0
78.90	2318.0
80.00	528.0
80.90	2223.0
82.00	539.0
83.10	128.0
85.80	131.0
87.00	3851.0
88.00	3656.0
91.00	381.0
92.00	1991.0
93.00	3127.0
94.10	8648.0
95.00	75712.0
96.10	4824.0
97.00	152.0
103.90	247.0
104.70	133.0
105.90	309.0
115.90	326.0
117.00	522.0
117.80	235.0
118.90	377.0
127.80	313.0
128.90	171.0
129.90	258.0
135.00	162.0
140.90	594.0
143.00	718.0
145.00	178.0
145.90	119.0
147.90	221.0
154.80	199.0
157.00	156.0
158.90	112.0
170.80	107.0
171.90	679.0
173.90	67768.0
175.00	4798.0
175.90	64944.0
176.90	3922.0
177.90	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362