
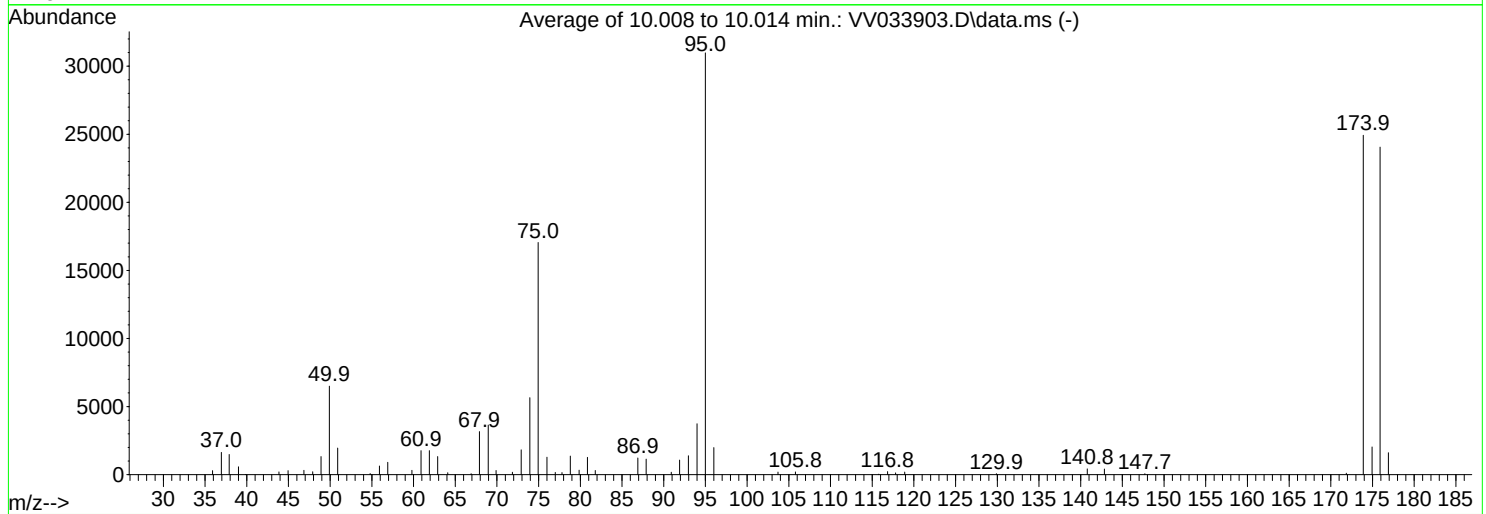


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013024\
Data File : VV033903.D
Acq On : 30 Jan 2024 08:44
Operator : SY/MD
Sample : BFB244
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB244

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 30 03:43:29 2024

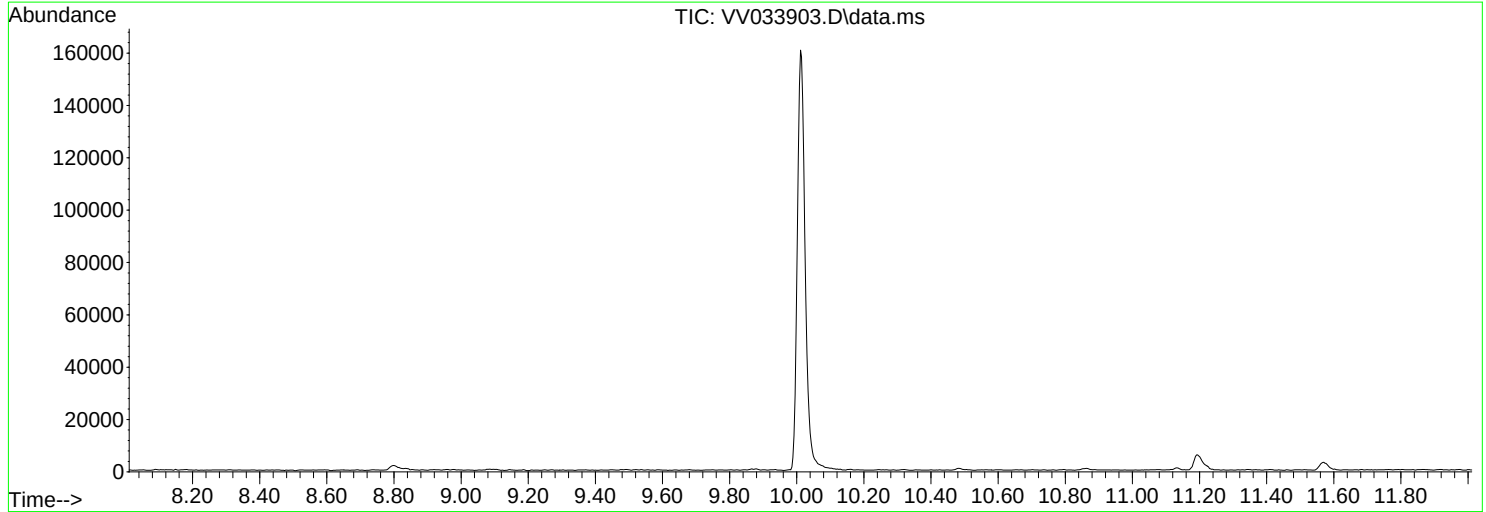

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	6501	PASS
75	95	30	80	55.0	17048	PASS
95	95	100	100	100.0	30981	PASS
96	95	5	9	6.4	1992	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.4	24923	PASS
175	174	5	9	8.2	2032	PASS
176	174	95	105	96.5	24056	PASS
177	176	5	10	6.7	1609	PASS

m/z	Abundance
39.80	572.0
43.80	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
35.90	306.0
37.00	1605.0
37.90	1515.0
39.00	624.0
39.90	563.0
43.90	424.0
44.90	274.0
46.90	299.0
47.90	240.0
48.90	1231.0
49.90	6332.0
50.90	1841.0
54.90	132.0
55.90	651.0
56.90	930.0
59.80	342.0
60.90	1794.0
61.90	1637.0
62.90	1220.0
64.10	140.0
67.90	2949.0
68.90	3437.0
69.90	301.0
71.90	195.0
72.90	1783.0
73.90	5434.0
74.90	16249.0
76.00	1374.0
77.00	166.0
77.90	151.0
78.80	1261.0
79.90	337.0
80.80	1191.0
81.80	273.0
86.90	1180.0
87.90	1133.0
90.90	175.0
91.90	1008.0
92.90	1331.0
94.00	3570.0
95.00	29568.0
96.00	1887.0
103.70	148.0
105.80	164.0
116.80	213.0
117.70	130.0
118.90	162.0
129.90	115.0
140.80	445.0
142.80	421.0
171.90	117.0
173.90	22760.0
175.00	1876.0
175.90	22352.0
176.90	1532.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
35.90	301.0
37.00	1690.0
37.90	1528.0
39.00	594.0
39.90	592.0
43.90	445.0
44.90	311.0
46.80	322.0
47.90	217.0
48.90	1383.0
49.90	6749.0
50.90	2012.0
54.70	106.0
55.90	675.0
56.90	917.0
59.80	334.0
60.90	1814.0
61.90	1846.0
62.90	1375.0
64.10	147.0
66.90	104.0
67.90	3285.0
68.90	3792.0
69.90	324.0
71.90	172.0
72.90	1922.0
74.00	5829.0
75.00	17544.0
76.00	1287.0
77.00	175.0
77.80	152.0
78.80	1425.0
79.90	348.0
80.80	1295.0
81.80	319.0
86.90	1288.0
87.90	1149.0
90.90	180.0
91.90	1135.0
92.90	1429.0
94.00	3885.0
95.00	32088.0
96.00	2065.0
103.70	199.0
105.80	210.0
116.80	229.0
117.80	133.0
118.90	205.0
129.90	106.0
140.80	450.0
142.80	414.0
147.70	101.0
171.90	116.0
173.90	25760.0
175.00	2110.0
175.90	24864.0
176.90	1672.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
35.90	280.0
36.90	1618.0
37.90	1415.0
39.00	520.0
39.90	611.0
43.90	378.0
45.00	315.0
46.80	327.0
47.90	170.0
48.90	1363.0
49.90	6421.0
50.90	2007.0
55.90	578.0
56.90	859.0
59.80	289.0
60.90	1699.0
61.90	1824.0
62.90	1388.0
64.10	133.0
66.90	102.0
67.90	3242.0
69.00	3714.0
69.90	305.0
71.80	152.0
72.90	1755.0
74.00	5697.0
75.00	17352.0
76.00	1191.0
77.00	163.0
77.70	145.0
78.80	1417.0
79.80	317.0
80.90	1322.0
81.80	340.0
86.90	1217.0
87.90	1151.0
90.90	161.0
91.90	1082.0
93.00	1408.0
94.00	3761.0
95.00	31288.0
96.00	2023.0
103.70	210.0
105.80	226.0
115.80	114.0
116.90	229.0
117.90	140.0
118.90	211.0
140.80	378.0
142.90	391.0
147.70	100.0
171.70	102.0
173.90	26248.0
174.90	2109.0
175.90	24952.0
176.90	1623.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244