

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV013025\
 Data File : VV038572.D
 Acq On : 29 Jan 2025 16:48
 Operator : SY/MD
 Sample : VIBLK217
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK217

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV038572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	87	rBV	63469	69737	11.45%	1.455%
2	1.529	144	152	163	rBV	66407	80869	13.28%	1.687%
3	2.053	304	315	327	rBV	121263	174881	28.71%	3.648%
4	3.812	851	862	901	rBV2	62493	260495	42.77%	5.435%
5	4.243	977	996	1027	rBV2	103038	276036	45.32%	5.759%
6	4.950	1203	1216	1249	rBV3	208410	558460	91.69%	11.651%
7	5.529	1385	1396	1422	rBV	171348	385120	63.23%	8.034%
8	5.982	1524	1537	1573	rBV	132498	300181	49.29%	6.262%
9	6.915	1816	1827	1859	rBV	46984	112331	18.44%	2.343%
10	7.239	1918	1928	1952	rBV	176468	343771	56.44%	7.172%
11	7.561	2019	2028	2050	rBV3	25615	59421	9.76%	1.240%
12	8.024	2161	2172	2213	rBV	224734	609065	100.00%	12.706%
13	8.780	2397	2407	2434	rBV	298142	539620	88.60%	11.258%
14	10.149	2822	2833	2845	rBV	116656	196104	32.20%	4.091%
15	11.181	3144	3154	3178	rVV	247043	428763	70.40%	8.945%
16	11.554	3256	3270	3292	rBV	199799	356080	58.46%	7.429%
17	12.593	3585	3593	3606	rBV10	4544	8054	1.32%	0.168%
18	13.207	3774	3784	3793	rBV8	5400	9536	1.57%	0.199%
19	13.451	3852	3860	3870	rBV	8691	18491	3.04%	0.386%
20	13.680	3922	3931	3932	rBV3	6517	6325	1.04%	0.132%




Sum of corrected areas: 4793340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV013025\
Data File : VV038572.D
Acq On : 29 Jan 2025 16:48
Operator : SY/MD
Sample : VIBLK217
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

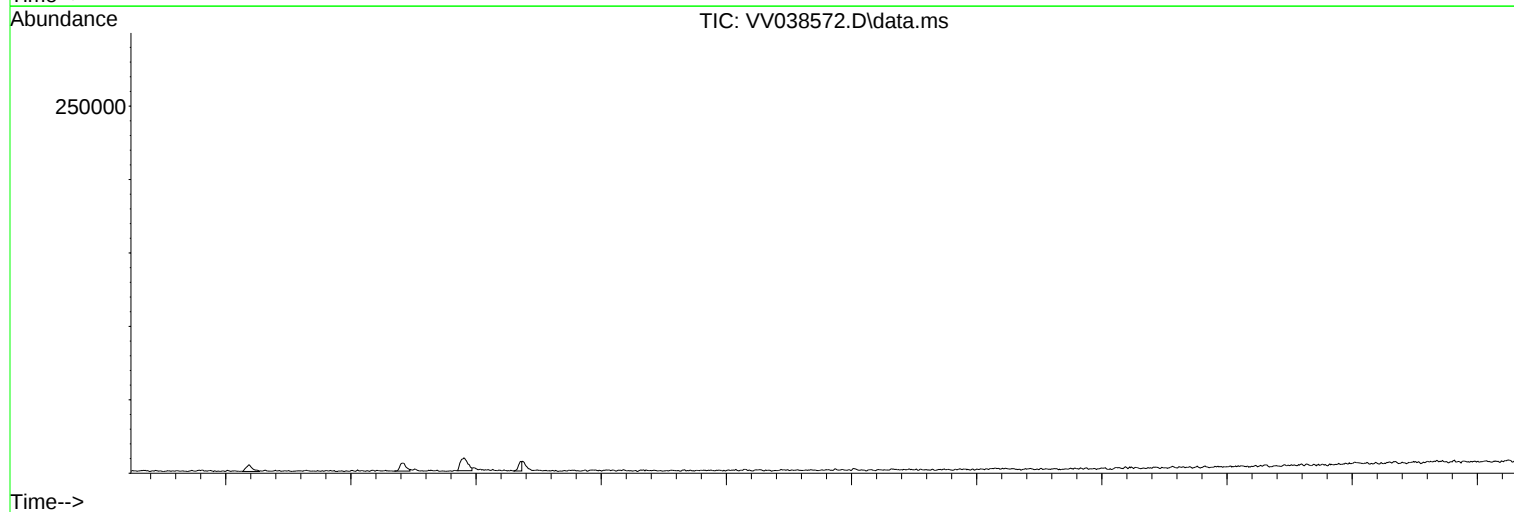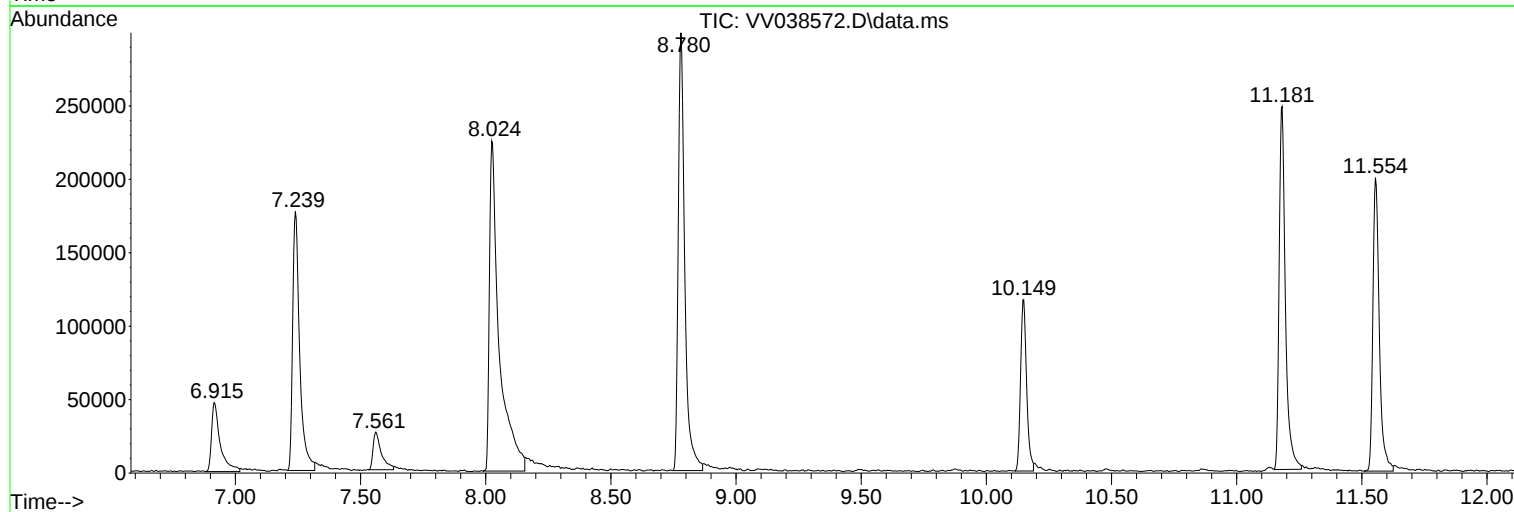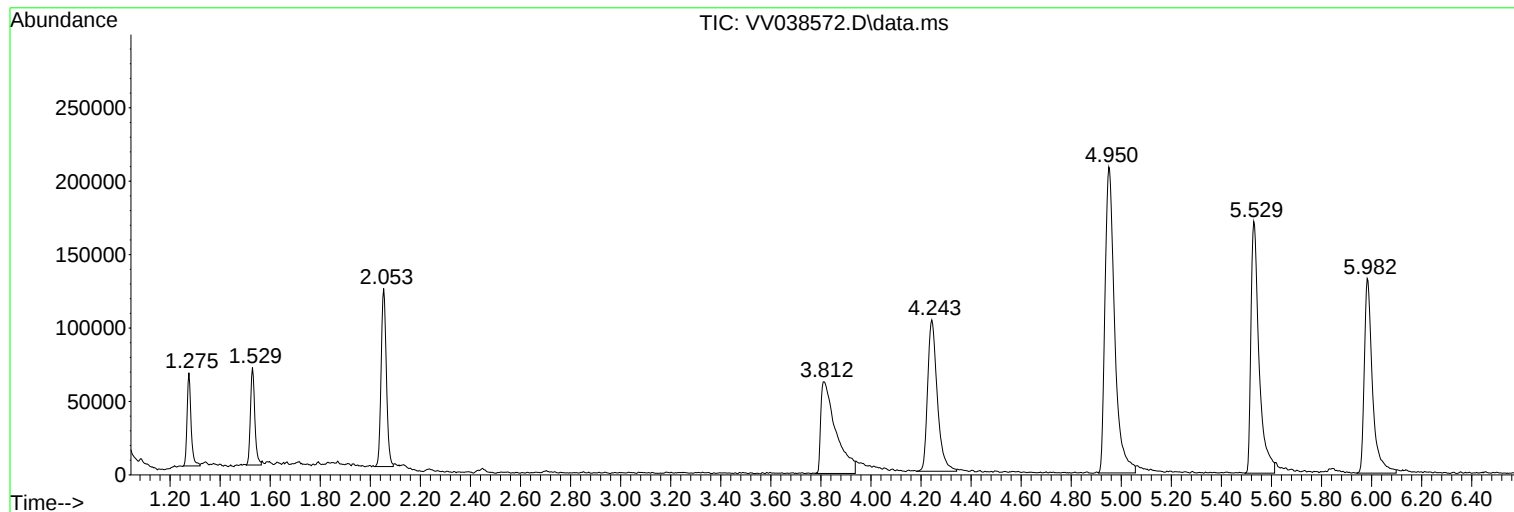

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV013025\
Data File : VV038572.D
Acq On : 29 Jan 2025 16:48
Operator : SY/MD
Sample : VIBLK217
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV013025\
Data File : VV038572.D
Acq On : 29 Jan 2025 16:48
Operator : SY/MD
Sample : VIBLK217
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc