
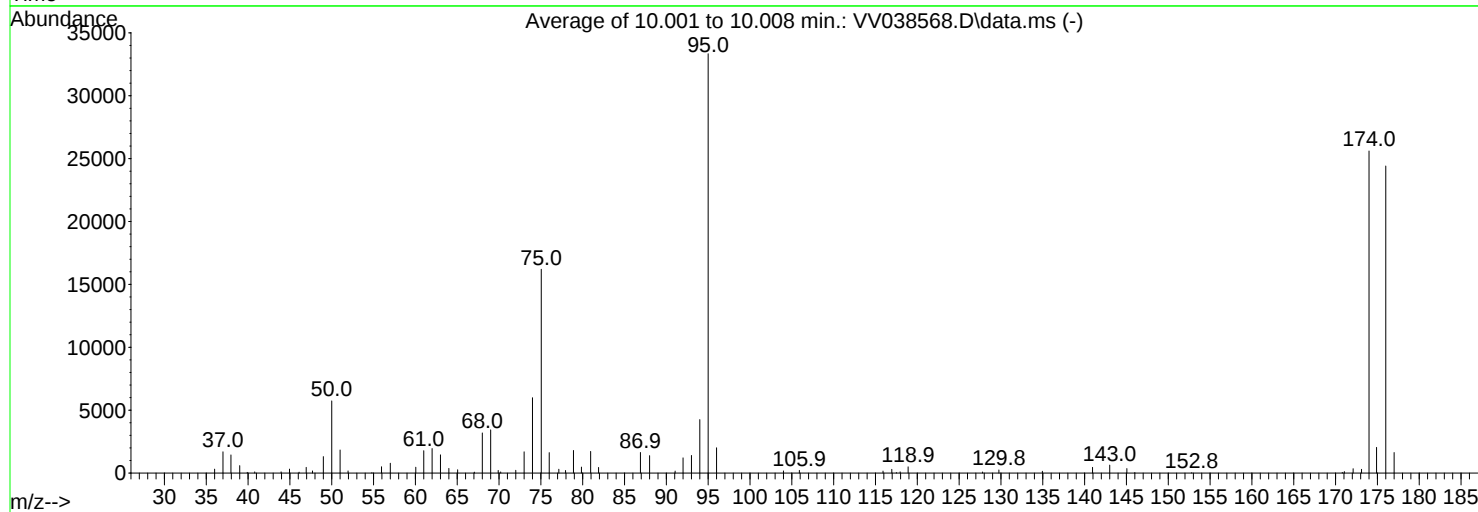


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV013025\
Data File : VV038568.D
Acq On : 29 Jan 2025 13:39
Operator : SY/MD
Sample : BFB200
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB200

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 30 08:15:13 2025

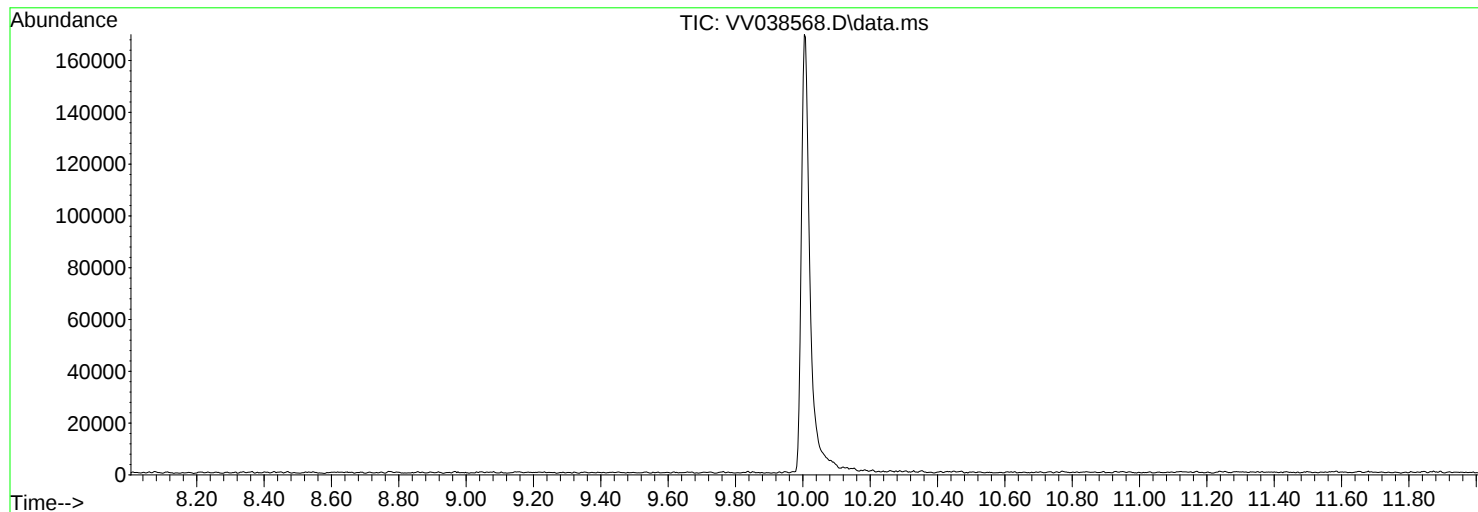

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	5736	PASS
75	95	30	80	48.6	16205	PASS
95	95	100	100	100.0	33339	PASS
96	95	5	9	6.0	2010	PASS
173	174	0.00	2	1.2	299	PASS
174	95	50	120	76.8	25608	PASS
175	174	5	9	8.0	2041	PASS
176	174	95	105	95.3	24413	PASS
177	176	5	10	6.7	1634	PASS

m/z	Abundance
37.90	100.0
39.90	451.0
44.00	505.0
50.20	103.0
77.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

m/z	Abundance
36.00	344.0
37.00	1682.0
38.00	1700.0
39.00	591.0
40.00	541.0
44.00	570.0
45.00	278.0
46.90	497.0
47.60	157.0
49.00	1127.0
50.00	5407.0
51.00	1700.0
52.00	174.0
55.90	491.0
57.00	756.0
60.00	440.0
61.00	1698.0
62.00	1751.0
63.00	1344.0
64.00	324.0
65.10	209.0
68.00	3088.0
69.00	3115.0
70.20	278.0
72.00	179.0
73.00	1627.0
74.00	5551.0
75.10	15087.0
76.00	1610.0
76.90	228.0
77.30	241.0
77.90	198.0
78.90	1667.0
79.80	463.0
80.90	1608.0
81.90	483.0
86.90	1661.0
88.00	1303.0
91.10	143.0
92.00	1168.0
93.00	1324.0
94.00	3933.0
95.00	31352.0
96.00	1979.0
104.10	167.0
105.90	197.0
115.90	114.0
116.90	271.0
117.50	120.0
118.00	169.0
118.90	450.0
129.70	265.0
135.00	127.0
140.90	377.0
143.00	605.0
145.00	308.0
170.80	165.0
172.20	338.0
173.10	291.0
174.00	23600.0
174.90	1960.0
176.00	22656.0
177.00	1579.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

m/z	Abundance
36.00	320.0
37.00	1736.0
38.00	1563.0
39.00	618.0
40.00	526.0
40.80	117.0
44.00	620.0
45.00	318.0
46.10	113.0
46.90	438.0
47.70	166.0
49.00	1374.0
50.00	6015.0
51.00	1909.0
51.90	181.0
56.00	507.0
57.00	796.0
60.10	497.0
61.00	1850.0
62.00	2087.0
63.00	1488.0
64.00	397.0
65.10	271.0
67.10	116.0
68.00	3304.0
69.00	3601.0
69.90	289.0
72.00	212.0
73.00	1751.0
74.00	6253.0
75.00	16672.0
76.00	1665.0
77.10	303.0
77.90	220.0
78.90	1861.0
79.80	474.0
81.00	1777.0
81.90	468.0
86.90	1677.0
88.00	1422.0
91.00	165.0
92.00	1279.0
93.00	1476.0
94.00	4334.0
95.00	34608.0
96.00	2046.0
104.00	189.0
105.90	226.0
115.90	165.0
116.90	284.0
117.90	125.0
118.90	543.0
127.80	110.0
129.80	273.0
135.00	147.0
141.00	468.0
143.00	679.0
145.10	390.0
146.00	115.0
152.80	100.0
171.00	169.0
172.10	358.0
173.10	301.0
174.00	26536.0
174.90	2130.0
176.00	25120.0
177.00	1712.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

m/z	Abundance
36.00	273.0
37.00	1655.0
38.00	1370.0
39.00	564.0
39.90	459.0
40.80	168.0
43.90	621.0
44.90	352.0
46.10	102.0
47.00	426.0
47.80	190.0
49.00	1433.0
50.00	6094.0
51.00	1902.0
51.90	155.0
54.80	109.0
56.00	509.0
57.00	800.0
60.00	461.0
61.00	1796.0
62.00	2019.0
63.00	1524.0
64.00	388.0
65.00	309.0
67.00	112.0
68.00	3177.0
69.00	3594.0
69.90	340.0
72.00	276.0
73.00	1700.0
74.00	6166.0
75.00	16856.0
76.00	1599.0
77.10	377.0
78.00	207.0
78.90	1859.0
79.90	494.0
81.00	1782.0
81.90	394.0
86.90	1578.0
88.00	1429.0
91.00	174.0
92.00	1187.0
93.00	1405.0
94.00	4488.0
95.00	34056.0
96.00	2005.0
103.90	159.0
105.90	215.0
115.90	202.0
117.00	336.0
118.90	498.0
127.80	154.0
129.80	214.0
134.90	165.0
141.00	518.0
143.00	622.0
145.00	384.0
171.10	186.0
172.00	346.0
173.10	304.0
174.00	26688.0
174.90	2032.0
176.00	25464.0
177.00	1611.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200