


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV013120\
 Data File : VV014444.D
 Acq On : 31 Jan 2020 09:20
 Operator : SY/MD
 Sample : BFB37
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR012920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Feb 04 12:46:25 2020

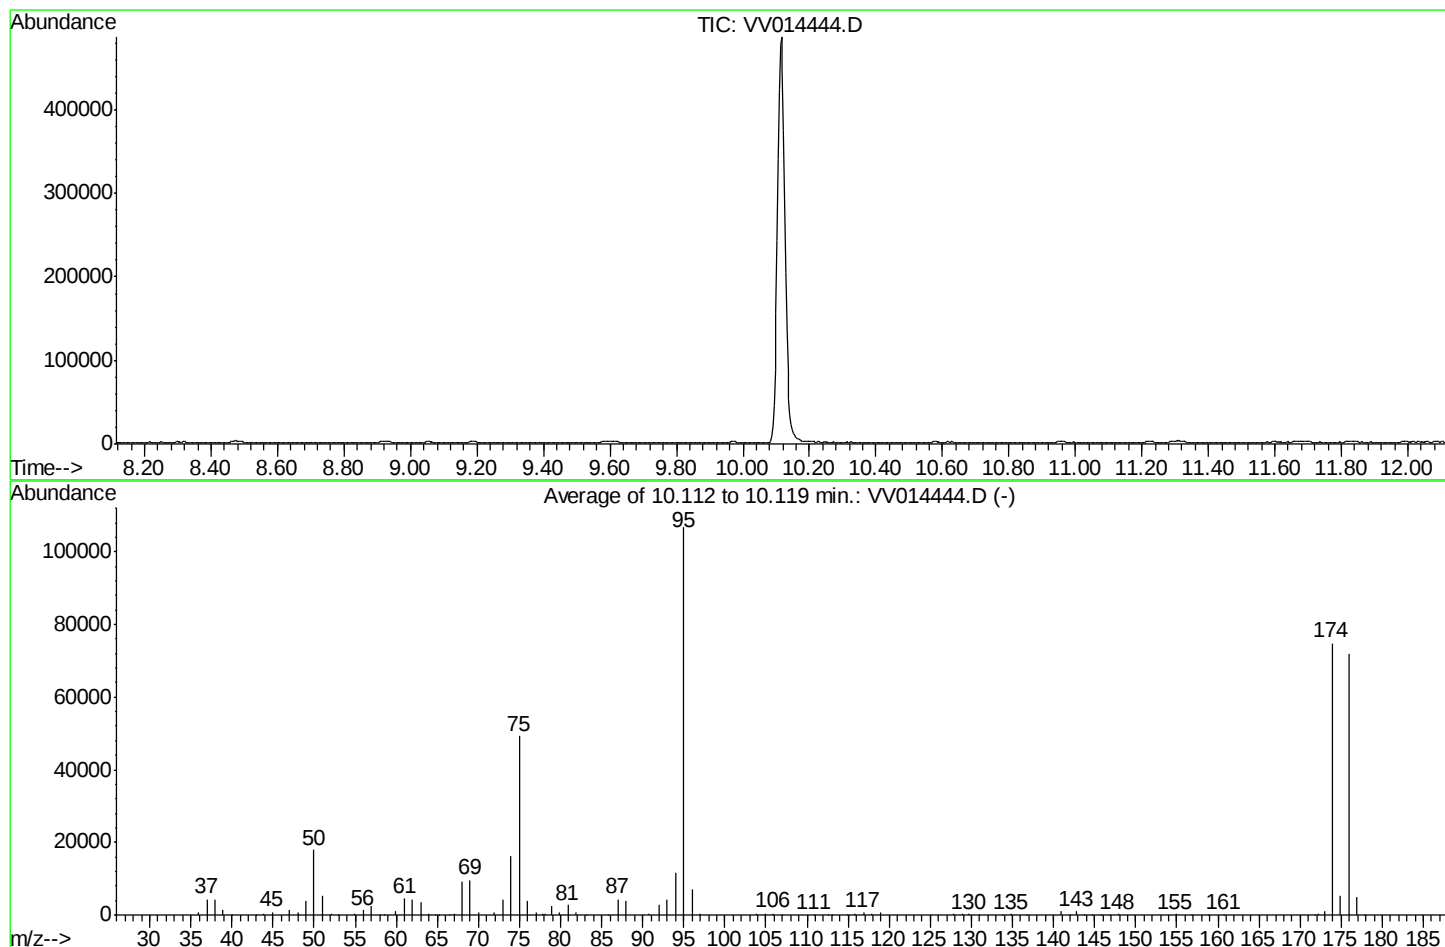

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	17880	PASS
75	95	30	80	46.1	49197	PASS
95	95	100	100	100.0	106736	PASS
96	95	5	9	6.8	7220	PASS
173	174	0.00	2	1.3	947	PASS
174	95	50	120	70.1	74845	PASS
175	174	5	9	7.2	5368	PASS
176	174	95	101	95.9	71800	PASS
177	176	5	9	7.0	4996	PASS

m/z	Abundance
36.00	929.0
37.00	4392.0
38.00	4359.0
39.00	1490.0
39.90	400.0
43.00	185.0
44.00	1004.0
45.00	863.0
46.90	1399.0
48.00	668.0
49.00	3751.0
50.00	18336.0
51.00	5494.0
52.10	275.0
52.90	127.0
54.90	388.0
56.00	1292.0
57.00	2653.0
58.50	113.0
59.90	934.0
61.00	4761.0
62.00	4368.0
63.00	3532.0
64.00	345.0
65.20	164.0
66.40	153.0
67.00	257.0
68.00	9478.0
69.00	9873.0
70.00	882.0
71.90	604.0
73.00	4564.0
74.00	16616.0
75.00	51064.0
76.00	4118.0
77.00	643.0
77.90	316.0
78.90	2531.0
79.90	766.0
80.90	2909.0
81.80	682.0
83.10	104.0
85.80	164.0
87.00	4508.0
87.90	4145.0
90.80	353.0
92.00	3110.0
93.00	4627.0
94.00	11844.0
95.00	109000.0
96.00	7599.0
97.00	225.0
103.80	398.0
104.90	202.0
105.90	430.0
106.90	115.0
110.90	140.0
112.60	104.0
113.00	113.0
114.90	148.0
115.90	466.0
116.90	654.0
117.80	423.0
118.90	529.0
127.70	274.0
128.90	212.0
129.80	297.0
130.90	122.0
134.90	202.0
136.80	181.0
140.90	959.0
141.90	156.0
142.80	1022.0
145.70	158.0
147.90	261.0
154.80	291.0
156.80	201.0
158.80	150.0
160.80	126.0
171.80	241.0
173.00	824.0
173.90	74296.0
174.90	5226.0
175.90	70976.0
176.90	5111.0
177.80	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.00	841.0
37.00	4425.0
38.00	4237.0
38.90	1481.0
39.90	404.0
43.00	193.0
43.90	1036.0
45.00	776.0
46.90	1489.0
48.00	663.0
49.00	3961.0
50.00	18488.0
51.00	5489.0
52.10	315.0
52.90	126.0
54.90	361.0
56.00	1321.0
57.00	2626.0
58.00	116.0
58.60	104.0
59.90	990.0
61.00	4740.0
62.00	4517.0
63.00	3474.0
64.00	389.0
65.20	171.0
66.40	135.0
67.00	282.0
68.00	9573.0
69.00	9914.0
70.00	823.0
71.90	635.0
73.00	4575.0
74.00	16616.0
75.00	50672.0
76.00	4129.0
77.00	694.0
77.70	302.0
78.10	294.0
78.90	2591.0
79.90	854.0
80.90	2879.0
81.80	717.0
85.70	153.0
87.00	4330.0
87.90	4143.0
90.80	339.0
92.00	3068.0
93.00	4397.0
94.00	12012.0
95.00	110304.0
96.00	7424.0
97.00	214.0
103.80	382.0
104.80	205.0
105.90	455.0
106.90	121.0
110.90	157.0
113.10	125.0
114.90	161.0
115.90	422.0
116.90	676.0
117.80	420.0
118.90	550.0
127.70	278.0
128.80	193.0
129.80	307.0
130.90	139.0
133.70	116.0
134.90	259.0
136.70	160.0
140.90	1045.0
142.00	145.0
142.80	1052.0
143.70	122.0
145.70	159.0
147.90	201.0
154.90	219.0
156.80	176.0
158.80	113.0
160.70	145.0
172.10	261.0
173.00	992.0
173.90	77640.0
174.90	5502.0
175.90	74168.0
176.90	5173.0
177.80	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
35.90	709.0
37.00	3952.0
38.00	3665.0
38.90	1351.0
39.90	443.0
43.00	176.0
43.90	1049.0
44.90	647.0
46.90	1297.0
48.00	603.0
49.00	3594.0
50.00	16816.0
51.00	5068.0
52.00	360.0
54.90	278.0
56.00	1174.0
57.00	2354.0
58.00	130.0
59.90	882.0
61.00	4242.0
62.00	4284.0
63.00	3079.0
64.00	390.0
64.80	115.0
65.20	131.0
67.00	264.0
68.00	8926.0
69.00	9151.0
70.10	703.0
72.00	534.0
73.00	4120.0
74.00	15239.0
75.00	45856.0
76.00	3811.0
77.00	666.0
77.70	296.0
78.10	291.0
78.90	2330.0
79.90	788.0
80.90	2614.0
81.80	650.0
85.80	115.0
86.90	3976.0
87.90	3673.0
90.80	290.0
92.00	2711.0
93.00	3866.0
94.00	11066.0
95.00	100904.0
96.00	6638.0
97.00	191.0
103.80	376.0
104.80	209.0
105.90	430.0
106.90	120.0
110.90	171.0
113.10	117.0
114.90	155.0
115.90	359.0
116.90	683.0
117.80	372.0
118.90	548.0
127.80	254.0
128.80	166.0
129.70	290.0
131.00	167.0
134.90	265.0
136.80	154.0
140.90	994.0
141.90	124.0
142.80	995.0
143.70	160.0
144.70	104.0
145.70	159.0
146.80	110.0
147.70	174.0
154.90	156.0
156.80	145.0
158.90	102.0
160.80	118.0
172.20	348.0
173.00	1026.0
173.90	72600.0
174.90	5377.0
175.90	70256.0
176.90	4704.0
177.80	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

Scan 2793 (10.071 min): VV014444.D
BFB37

m/z	Abundance
40.00	407.0
40.70	114.0
41.60	102.0
43.00	109.0
43.90	623.0
62.50	101.0
67.30	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37