

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013121\
 Data File : VW020222.D
 Acq On : 29 Jan 2021 14:19
 Operator : SY/MD
 Sample : VSTD0.0535
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05206

Quant Time: Jan 30 03:38:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 30 03:37:50 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	13409	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.863	117	12609	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6624	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.310	65	926	0.08 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	480	0.04 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	527	0.04 ug/L	0.00
8) Toluene-d8	7.332	98	1527	0.05 ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.216	84	308	0.04 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	782	0.04 ug/L	Qvalue # 76
6) Trichloroethene	5.925	95	484	0.04 ug/L	93
9) 1,2-Dibromoethane	8.368	107	273	0.04 ug/L	Qvalue # 90
12) 1,2,3-Trichloropropane	10.267	75	267	0.04 ug/L	94
13) 1,2-Dibromo-3-chloropr...	12.426	75	60	0.06 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
Data File : VV020222.D
Acq On : 29 Jan 2021 14:19
Operator : SY/MD
Sample : VSTD0.0535
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05206

Quant Time: Jan 30 03:38:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 30 03:37:50 2021
Response via : Initial Calibration




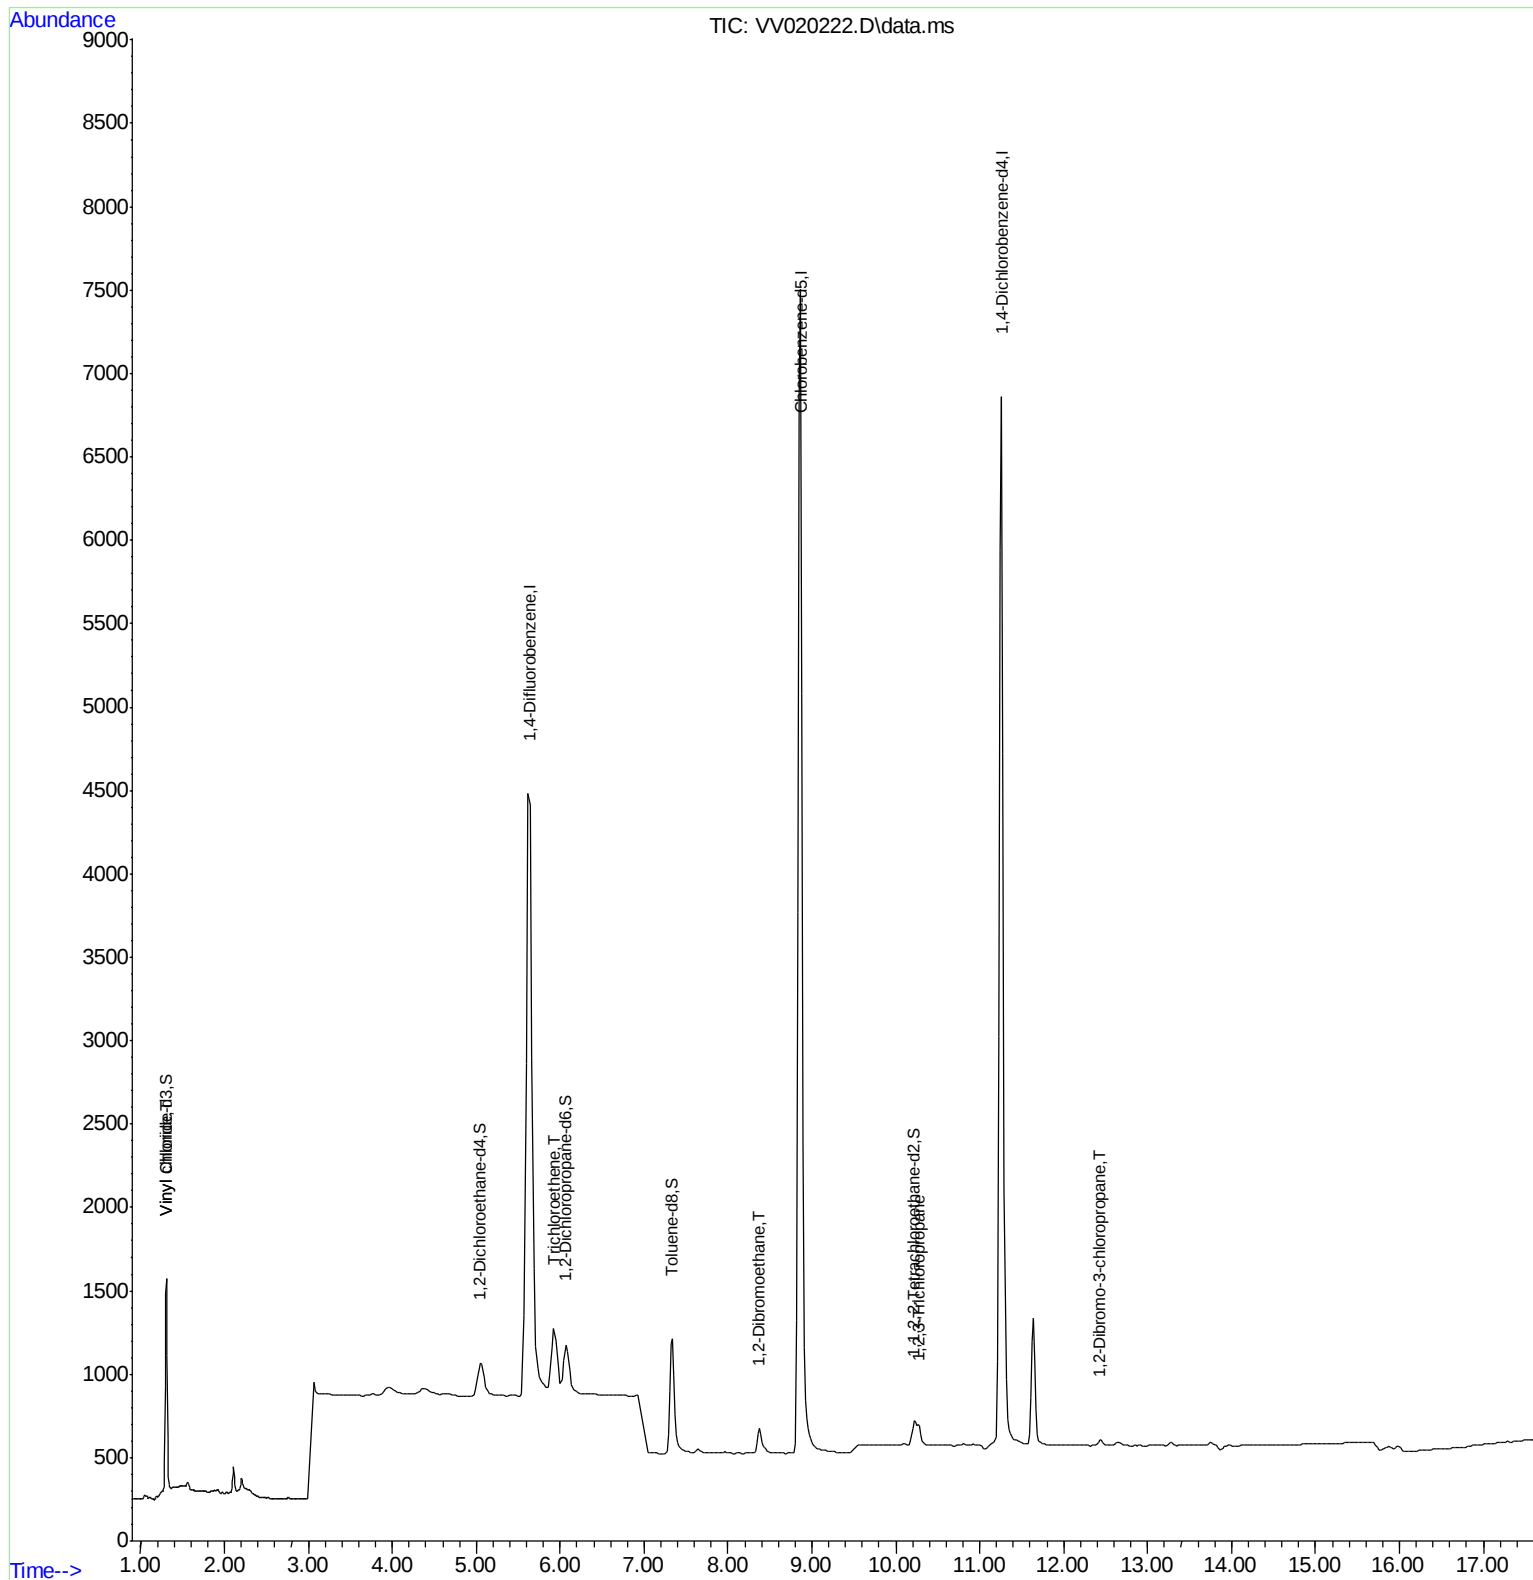


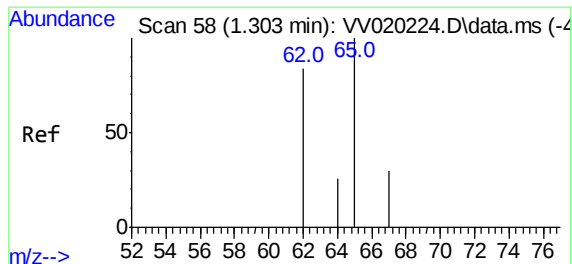

#3
Vinyl chloride
Concen: 0.04 ug/L
RT: 1.310 min Scan# 59
Delta R.T. 0.007 min
Lab File: VV020222.D
Acq: 29 Jan 2021 14:19




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05206


Tgt Ion: 62 Resp: 782
Ion Ratio Lower Upper
62 100
64 45.1 22.3 41.3#

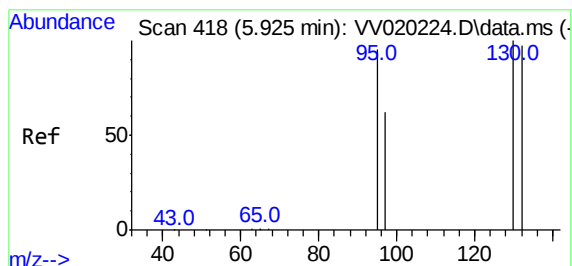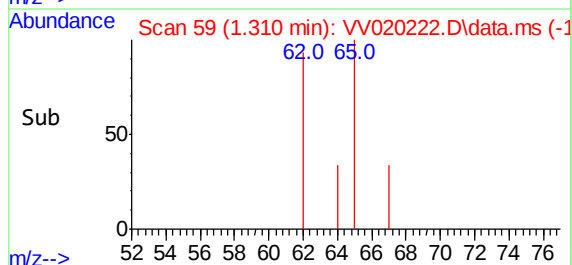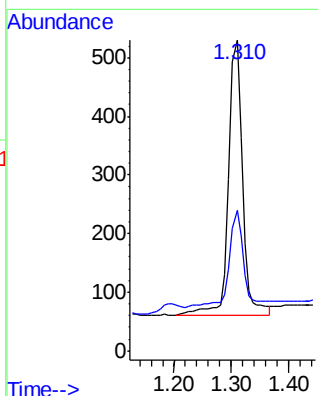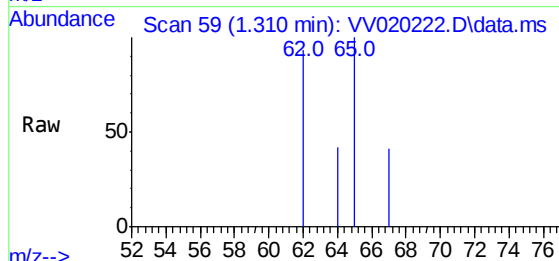

#6
Trichloroethene
Concen: 0.04 ug/L
RT: 5.925 min Scan# 418
Delta R.T. -0.000 min
Lab File: VV020222.D
Acq: 29 Jan 2021 14:19

Tgt Ion: 95 Resp: 484
Ion Ratio Lower Upper
95 100
97 77.0 46.8 86.8
132 96.9 71.3 132.5
130 98.8 73.4 136.2


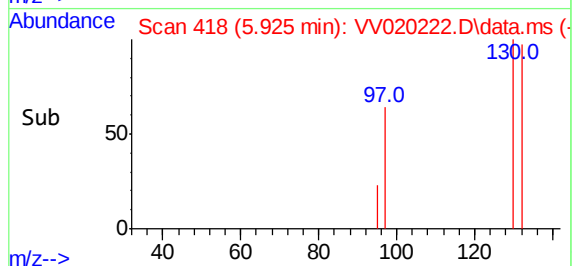
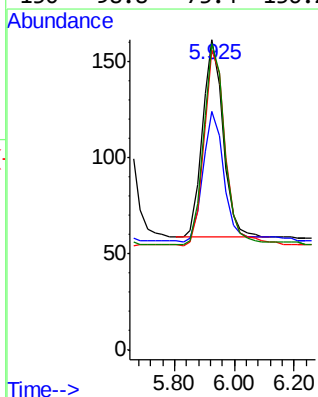
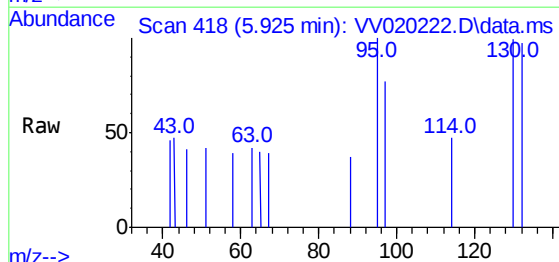


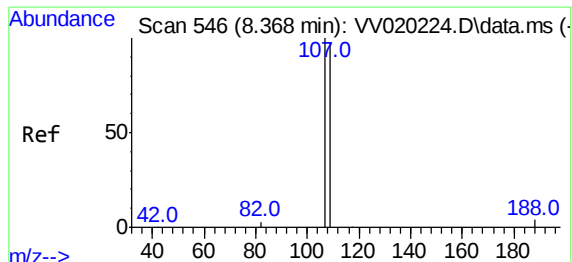

#9
1,2-Dibromoethane
Concen: 0.04 ug/L
RT: 8.368 min Scan# 546
Delta R.T. -0.000 min
Lab File: VV020222.D
Acq: 29 Jan 2021 14:19




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05206


Tgt Ion:107 Resp: 273
Ion Ratio Lower Upper
107 100
109 95.3 67.8 126.0
188 43.4 7.8 11.8#

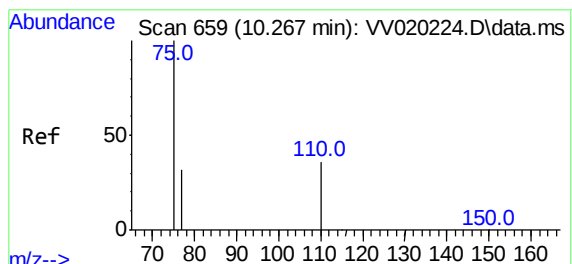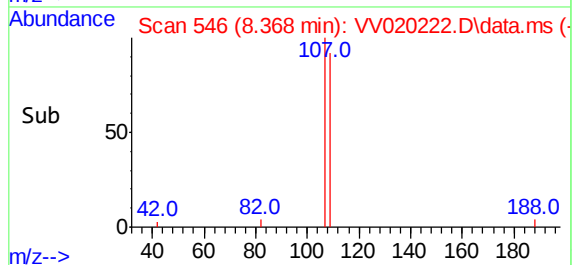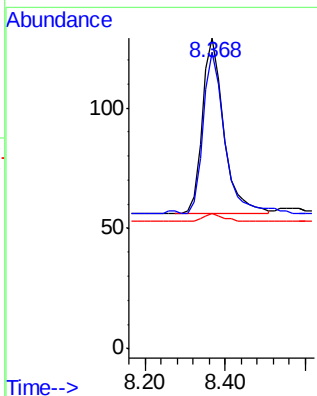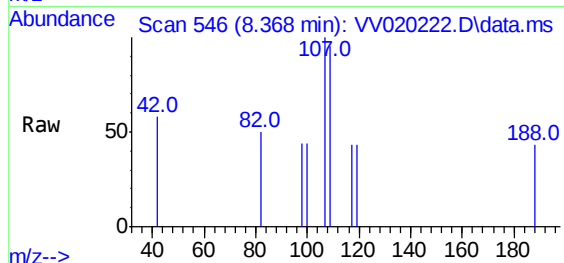

#12
1,2,3-Trichloropropane
Concen: 0.04 ug/L
RT: 10.267 min Scan# 659
Delta R.T. -0.000 min
Lab File: VV020222.D
Acq: 29 Jan 2021 14:19


Tgt Ion: 75 Resp: 267
Ion Ratio Lower Upper
75 100
110 37.5 32.4 48.6
77 37.1 26.6 40.0

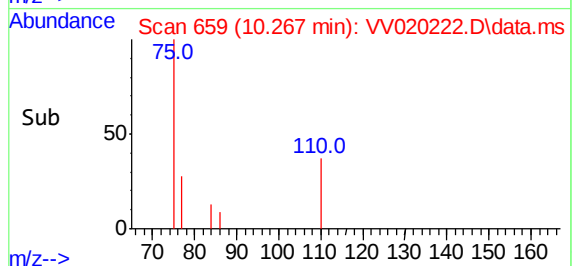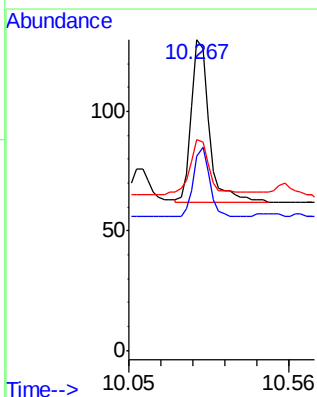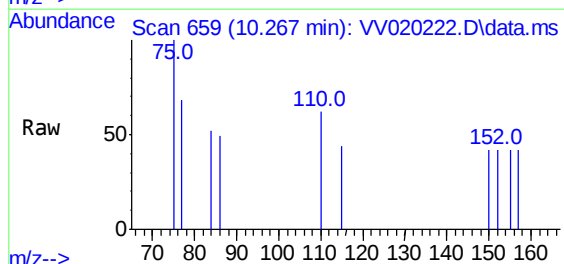

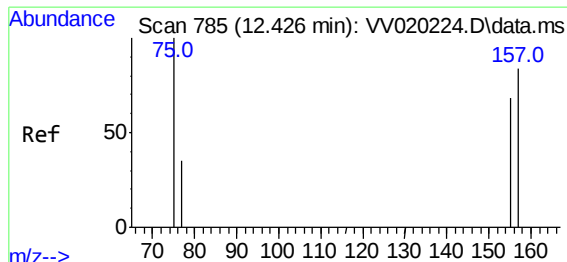

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.06 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. -0.000 min
 Lab File: VV020222.D
 Acq: 29 Jan 2021 14:19

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05206

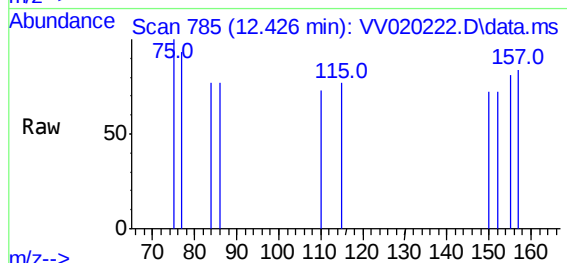

Tgt Ion: 75 Resp: 60

Ion	Ratio	Lower	Upper
75	100		
157	84.0	67.9	101.9
155	81.3	59.1	88.7

