

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013121\
 Data File : VW020223.D
 Acq On : 29 Jan 2021 14:40
 Operator : SY/MD
 Sample : VSTD0.136
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1207

Quant Time: Jan 30 03:38:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 30 03:37:50 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	12785	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.863	117	12372	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6454	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.310	65	1562	0.13 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.066	65	1047	0.10 ug/L	0.02
7) 1,2-Dichloropropane-d6	6.092	67	1188	0.10 ug/L	0.02
8) Toluene-d8	7.332	98	3287	0.11 ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.216	84	731	0.10 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	1353	0.08 ug/L	Qvalue 88
6) Trichloroethene	5.925	95	1032	0.09 ug/L	92
9) 1,2-Dibromoethane	8.368	107	604	0.09 ug/L #	93
12) 1,2,3-Trichloropropane	10.267	75	565	0.09 ug/L #	90
13) 1,2-Dibromo-3-chloropr...	12.426	75	96	0.10 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
Data File : VV020223.D
Acq On : 29 Jan 2021 14:40
Operator : SY/MD
Sample : VSTD0.136
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1207

Quant Time: Jan 30 03:38:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 30 03:37:50 2021
Response via : Initial Calibration




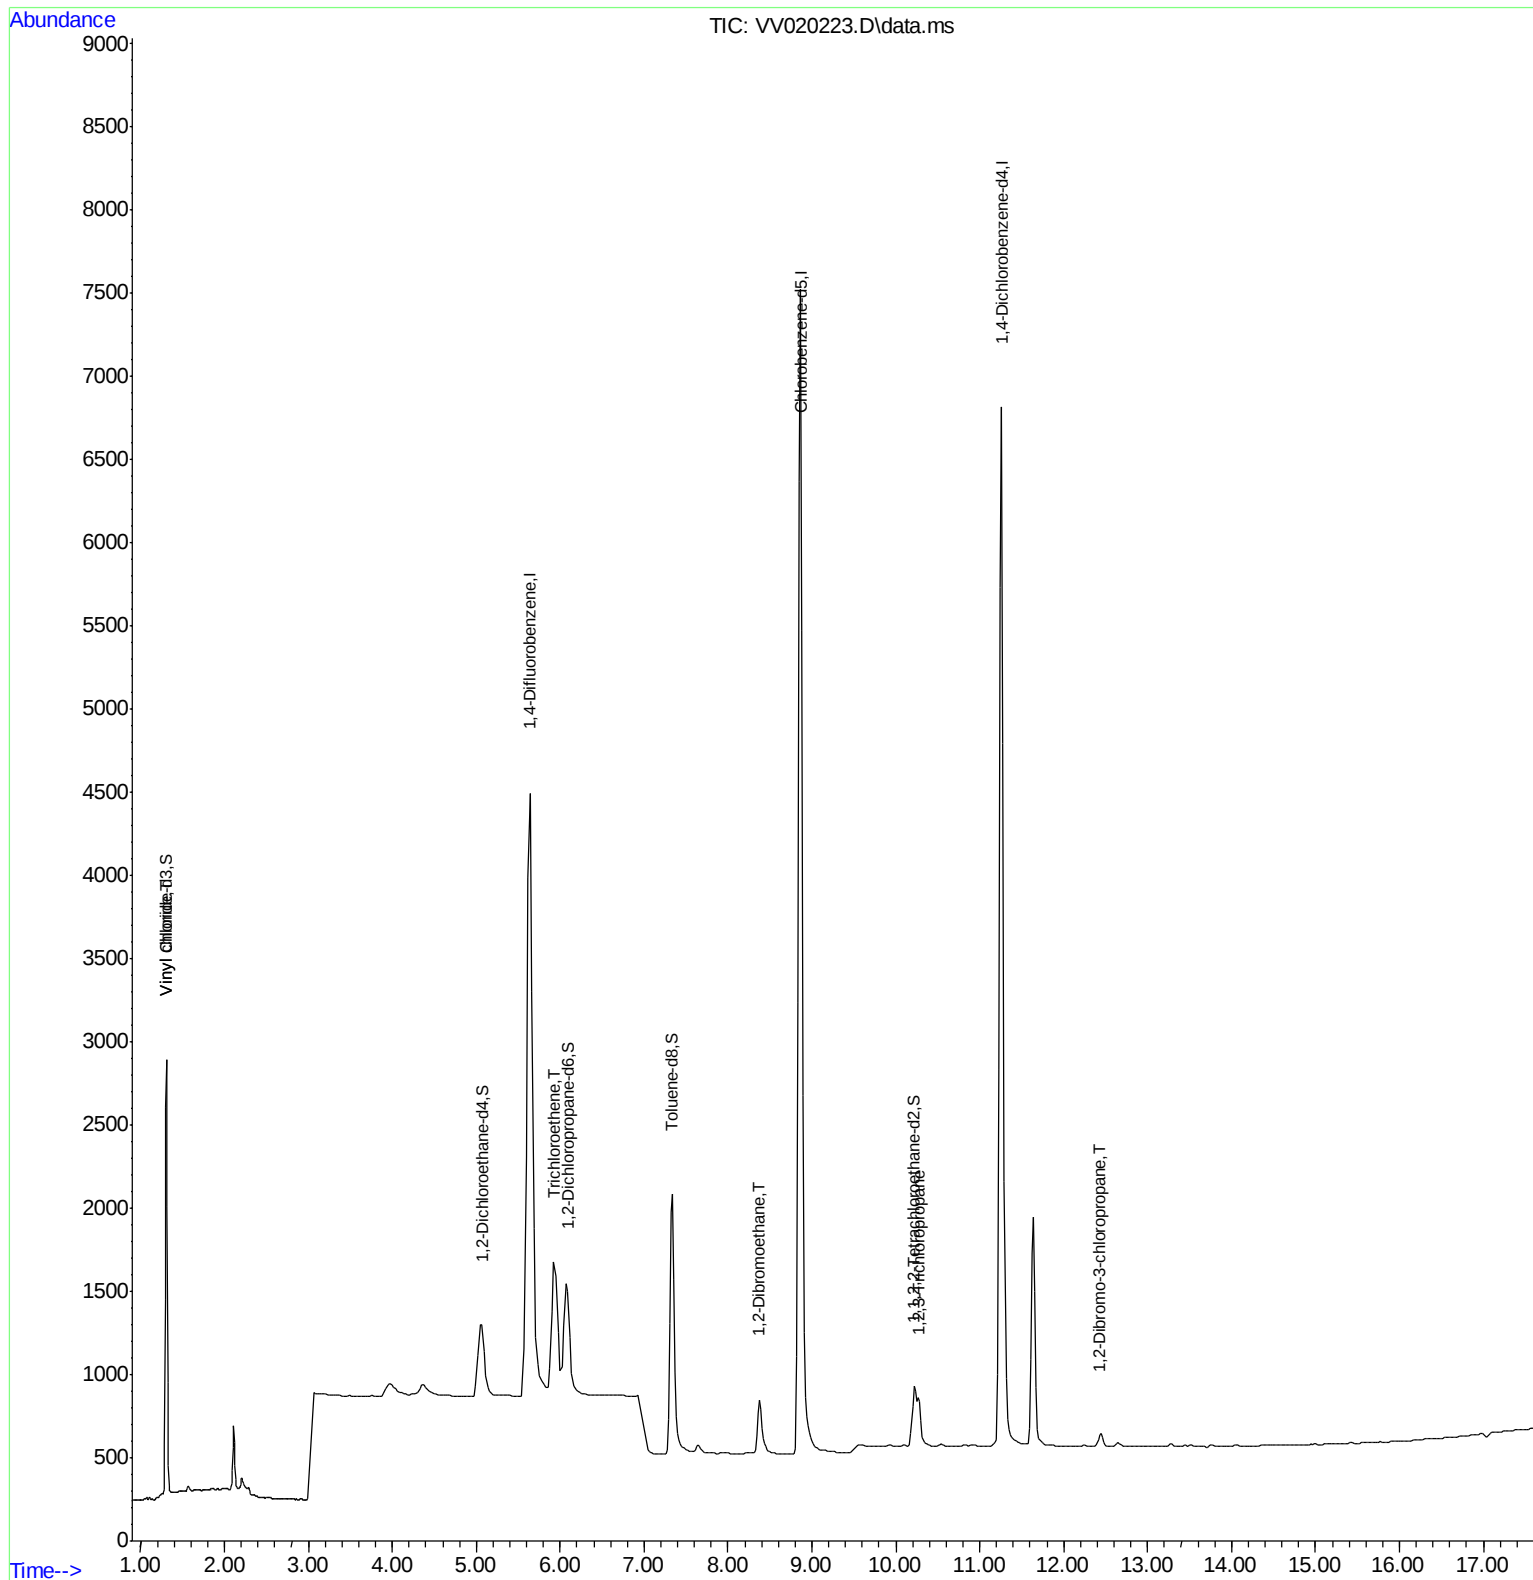


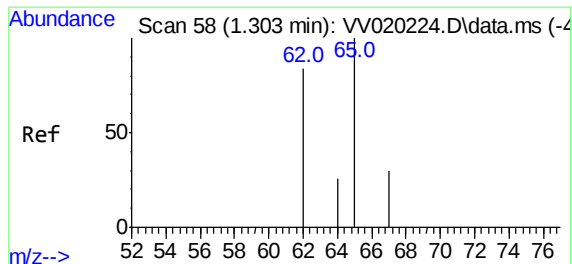

#3
Vinyl chloride
Concen: 0.08 ug/L
RT: 1.310 min Scan# 59
Delta R.T. 0.007 min
Lab File: VV020223.D
Acq: 29 Jan 2021 14:40




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1207


Tgt Ion: 62 Resp: 1353
Ion Ratio Lower Upper
62 100
64 38.6 22.3 41.3

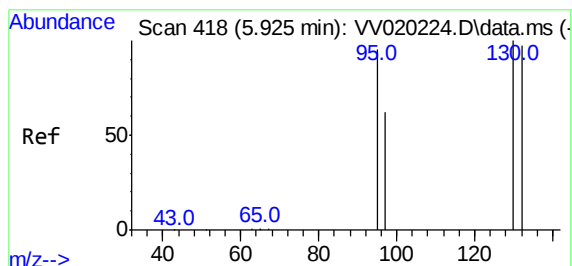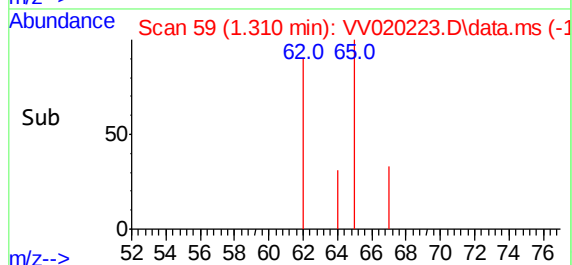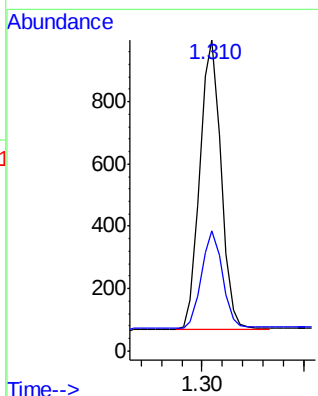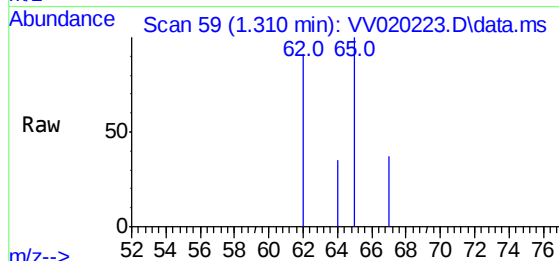

#6
Trichloroethene
Concen: 0.09 ug/L
RT: 5.925 min Scan# 418
Delta R.T. 0.000 min
Lab File: VV020223.D
Acq: 29 Jan 2021 14:40

Tgt Ion: 95 Resp: 1032
Ion Ratio Lower Upper
95 100
97 71.5 46.8 86.8
132 92.8 71.3 132.5
130 97.1 73.4 136.2


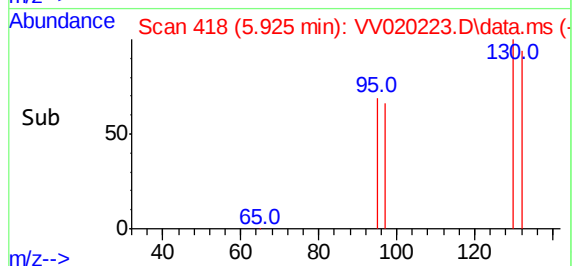
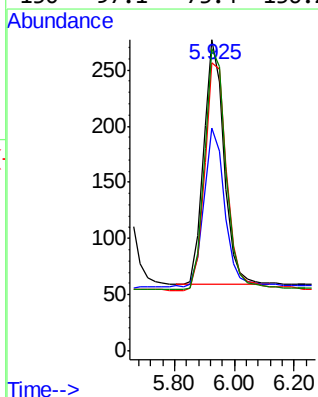
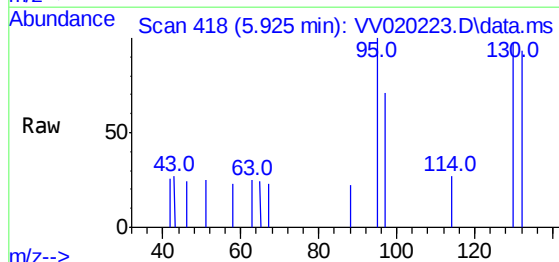


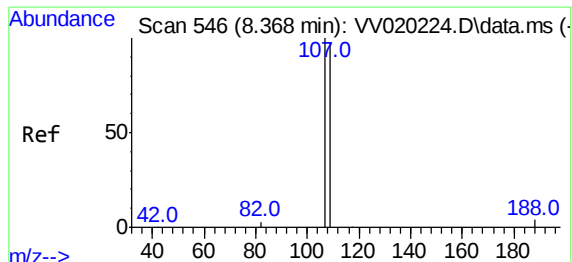

#9
1,2-Dibromoethane
Concen: 0.09 ug/L
RT: 8.368 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV020223.D
Acq: 29 Jan 2021 14:40




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1207


Tgt Ion:107 Resp: 604
Ion Ratio Lower Upper
107 100
109 94.5 67.8 126.0
188 27.1 7.8 11.8#

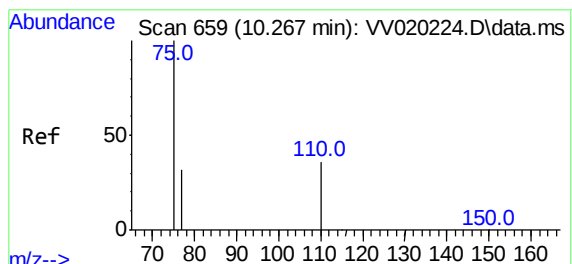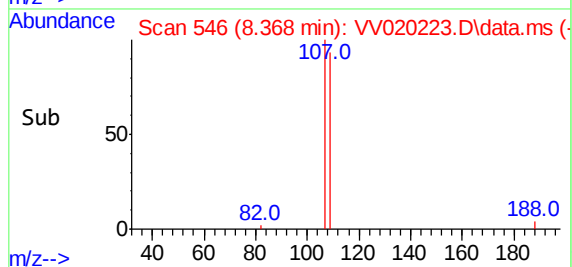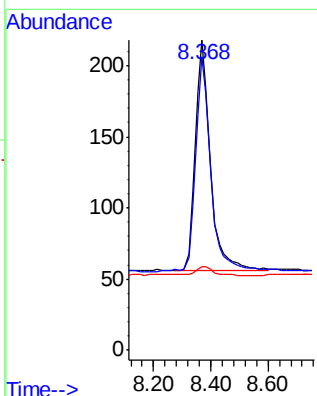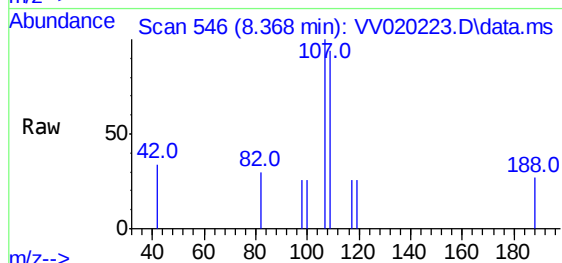

#12
1,2,3-Trichloropropane
Concen: 0.09 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020223.D
Acq: 29 Jan 2021 14:40

Tgt Ion: 75 Resp: 565
Ion Ratio Lower Upper
75 100
110 39.1 32.4 48.6
77 44.6 26.6 40.0#

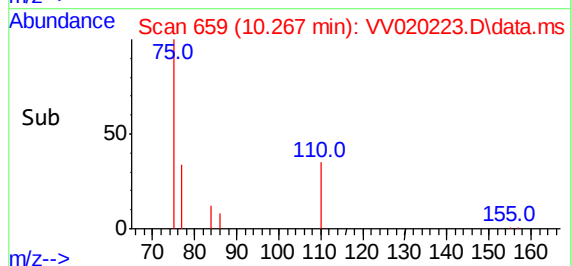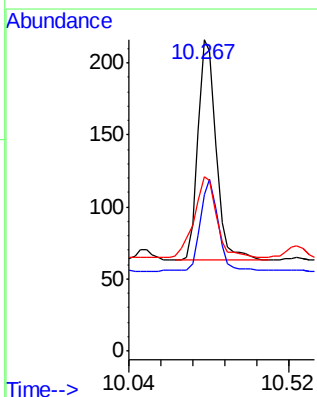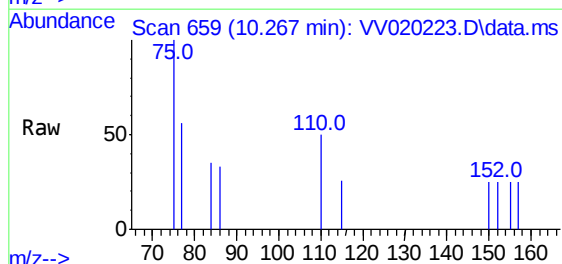

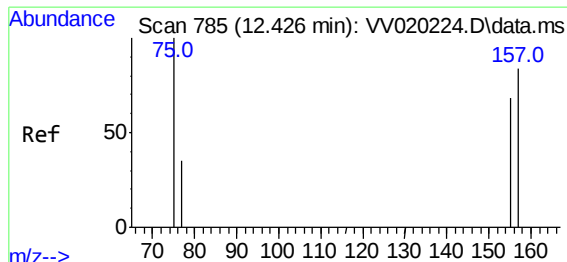

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.10 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020223.D
 Acq: 29 Jan 2021 14:40

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1207

Tgt Ion: 75 Resp: 96
 Ion Ratio Lower Upper
 75 100
 157 83.9 67.9 101.9
 155 80.5 59.1 88.7

