

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013121\
 Data File : VW020224.D
 Acq On : 29 Jan 2021 15:18
 Operator : SY/MD
 Sample : VSTD0.531
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5208

Quant Time: Jan 30 03:38:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 30 03:37:50 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	15208	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.863	117	14133	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	7410	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.303	65	9148	0.66 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	5578	0.45 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	6513	0.46 ug/L	0.00
8) Toluene-d8	7.317	98	17990	0.53 ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	3713	0.45 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.303	62	8083	0.38 ug/L	Qvalue 100
6) Trichloroethene	5.925	95	5509	0.40 ug/L	100
9) 1,2-Dibromoethane	8.368	107	3148	0.42 ug/L	100
12) 1,2,3-Trichloropropane	10.267	75	2945	0.39 ug/L	100
13) 1,2-Dibromo-3-chloropr...	12.426	75	451	0.41 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
Data File : VV020224.D
Acq On : 29 Jan 2021 15:18
Operator : SY/MD
Sample : VSTD0.531
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5208

Quant Time: Jan 30 03:38:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 30 03:37:50 2021
Response via : Initial Calibration




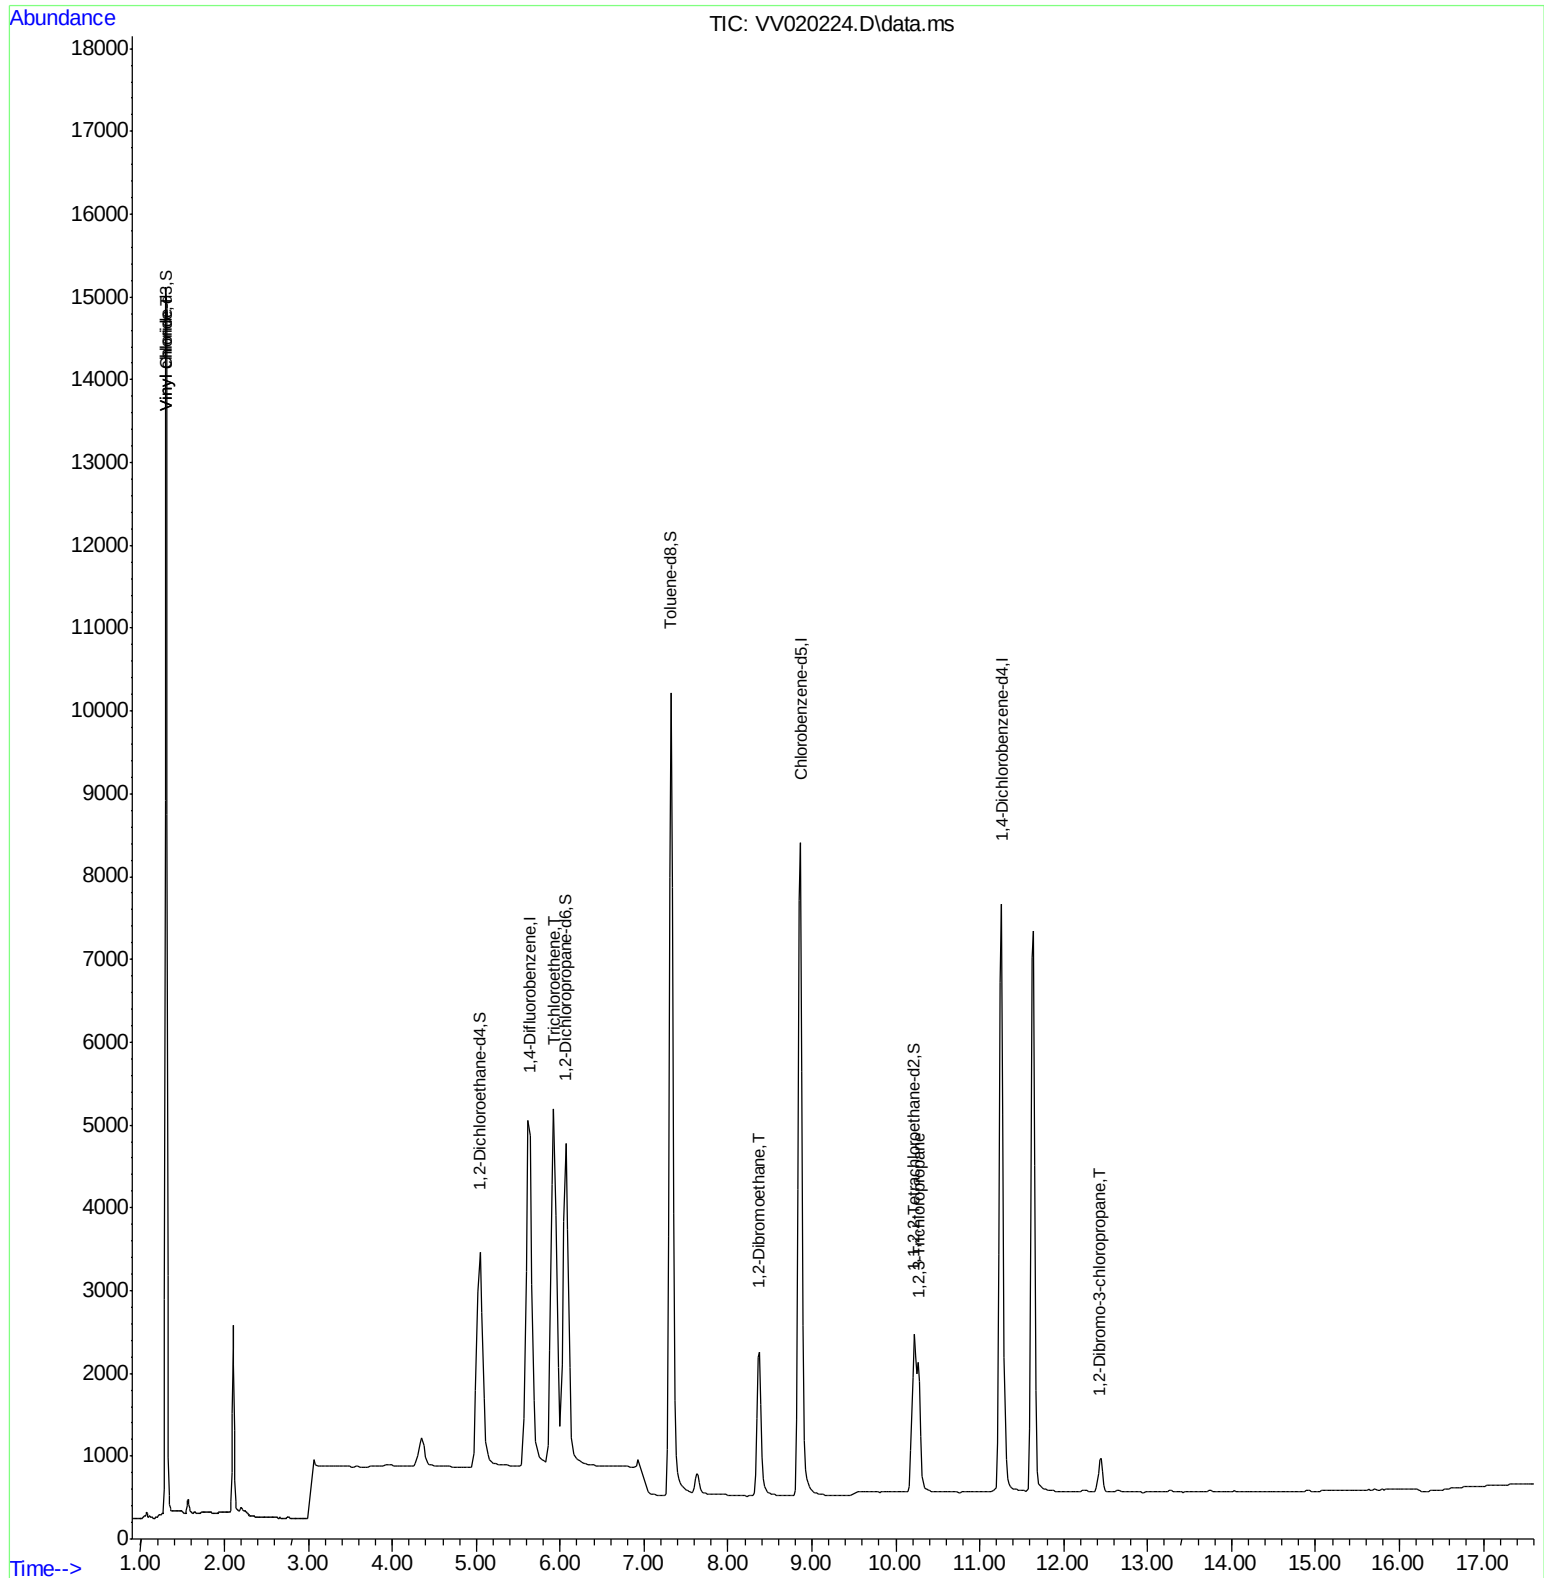


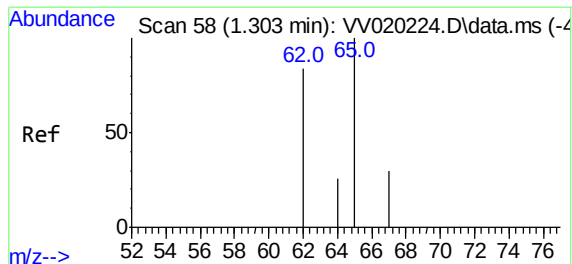

#3
 Vinyl chloride
 Concen: 0.38 ug/L
 RT: 1.303 min Scan# 58
 Delta R.T. 0.000 min
 Lab File: VV020224.D
 Acq: 29 Jan 2021 15:18




Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5208


Tgt Ion: 62 Resp: 8083
 Ion Ratio Lower Upper
 62 100
 64 31.8 22.3 41.3

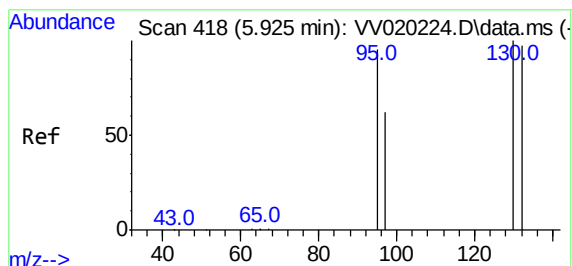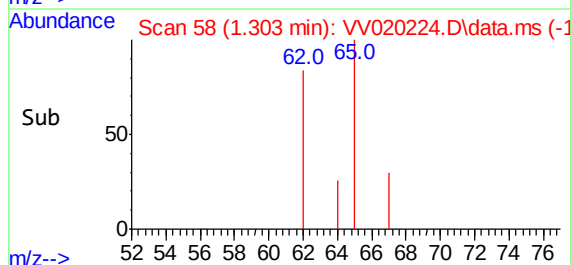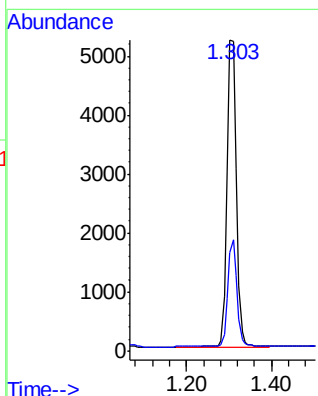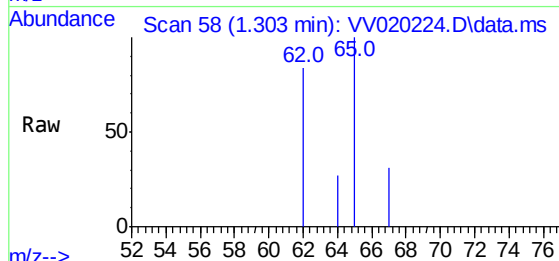

#6
 Trichloroethene
 Concen: 0.40 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. 0.000 min
 Lab File: VV020224.D
 Acq: 29 Jan 2021 15:18

Tgt Ion: 95 Resp: 5509
 Ion Ratio Lower Upper
 95 100
 97 66.8 46.8 86.8
 132 101.9 71.3 132.5
 130 104.8 73.4 136.2


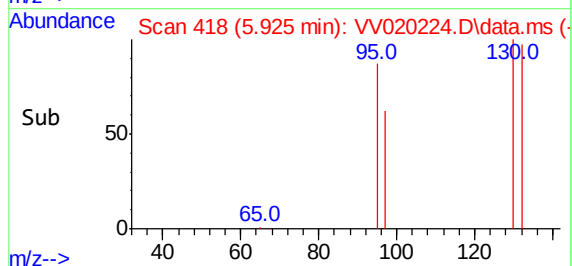
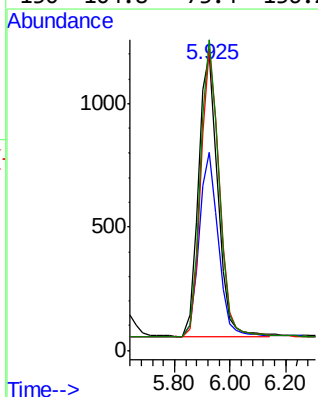
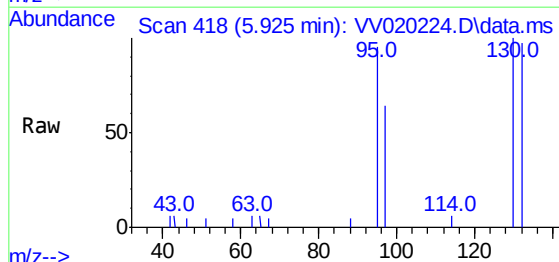


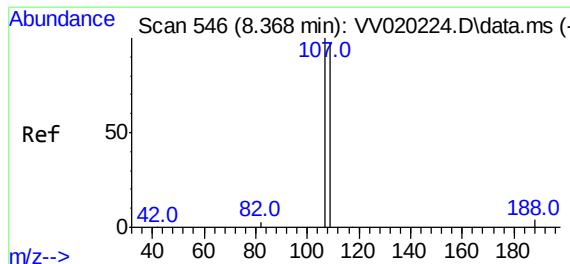

#9
1,2-Dibromoethane
Concen: 0.42 ug/L
RT: 8.368 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV020224.D
Acq: 29 Jan 2021 15:18




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5208


Tgt Ion:107 Resp: 3148
Ion Ratio Lower Upper
107 100
109 96.9 67.8 126.0
188 9.8 7.8 11.8

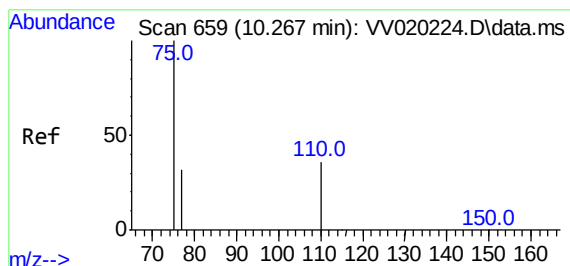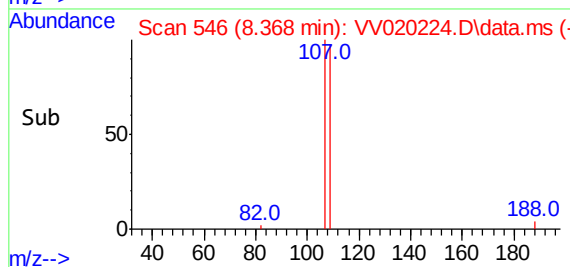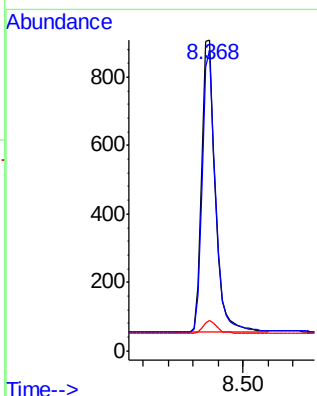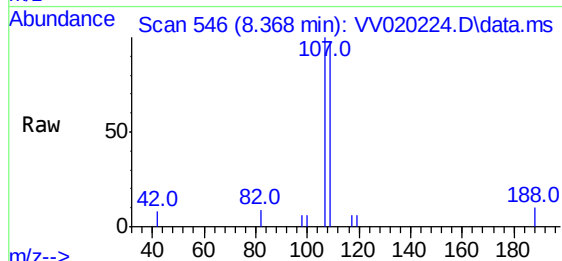

#12
1,2,3-Trichloropropane
Concen: 0.39 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020224.D
Acq: 29 Jan 2021 15:18


Tgt Ion: 75 Resp: 2945
Ion Ratio Lower Upper
75 100
110 40.5 32.4 48.6
77 33.3 26.6 40.0

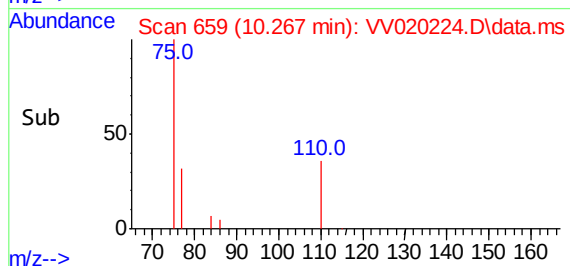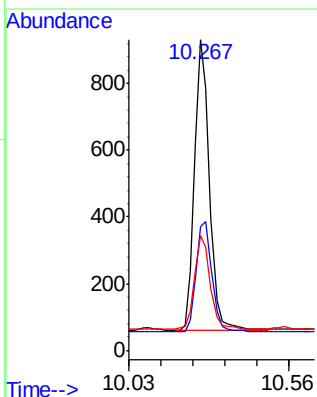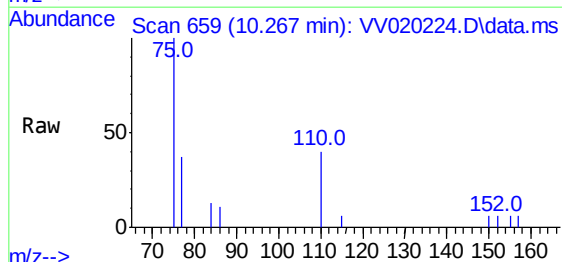

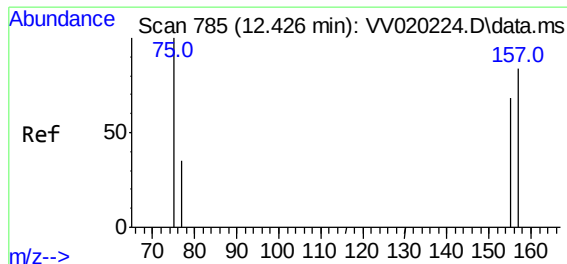

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.41 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020224.D
 Acq: 29 Jan 2021 15:18

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5208

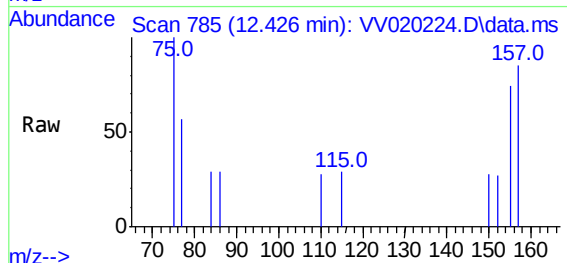

Tgt Ion: 75 Resp: 451

Ion	Ratio	Lower	Upper
75	100		
157	84.9	67.9	101.9
155	73.9	59.1	88.7

