

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013121\
 Data File : VW020225.D
 Acq On : 29 Jan 2021 15:41
 Operator : SY/MD
 Sample : VSTD00132
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001209

Quant Time: Jan 30 03:38:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 30 03:37:50 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	14849	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.864	117	14335	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	7366	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.303	65	18632	1.37 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	11483	0.96 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.069	67	13600	0.95 ug/L	0.00
8) Toluene-d8	7.317	98	37498	1.10 ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	8124	0.97 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	17286	0.83 ug/L	Qvalue 95
6) Trichloroethene	5.925	95	11783	0.84 ug/L	100
9) 1,2-Dibromoethane	8.353	107	6835	0.91 ug/L	# 94
12) 1,2,3-Trichloropropane	10.267	75	6477	0.85 ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.427	75	1018	0.93 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
Data File : VV020225.D
Acq On : 29 Jan 2021 15:41
Operator : SY/MD
Sample : VSTD00132
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001209

Quant Time: Jan 30 03:38:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 30 03:37:50 2021
Response via : Initial Calibration




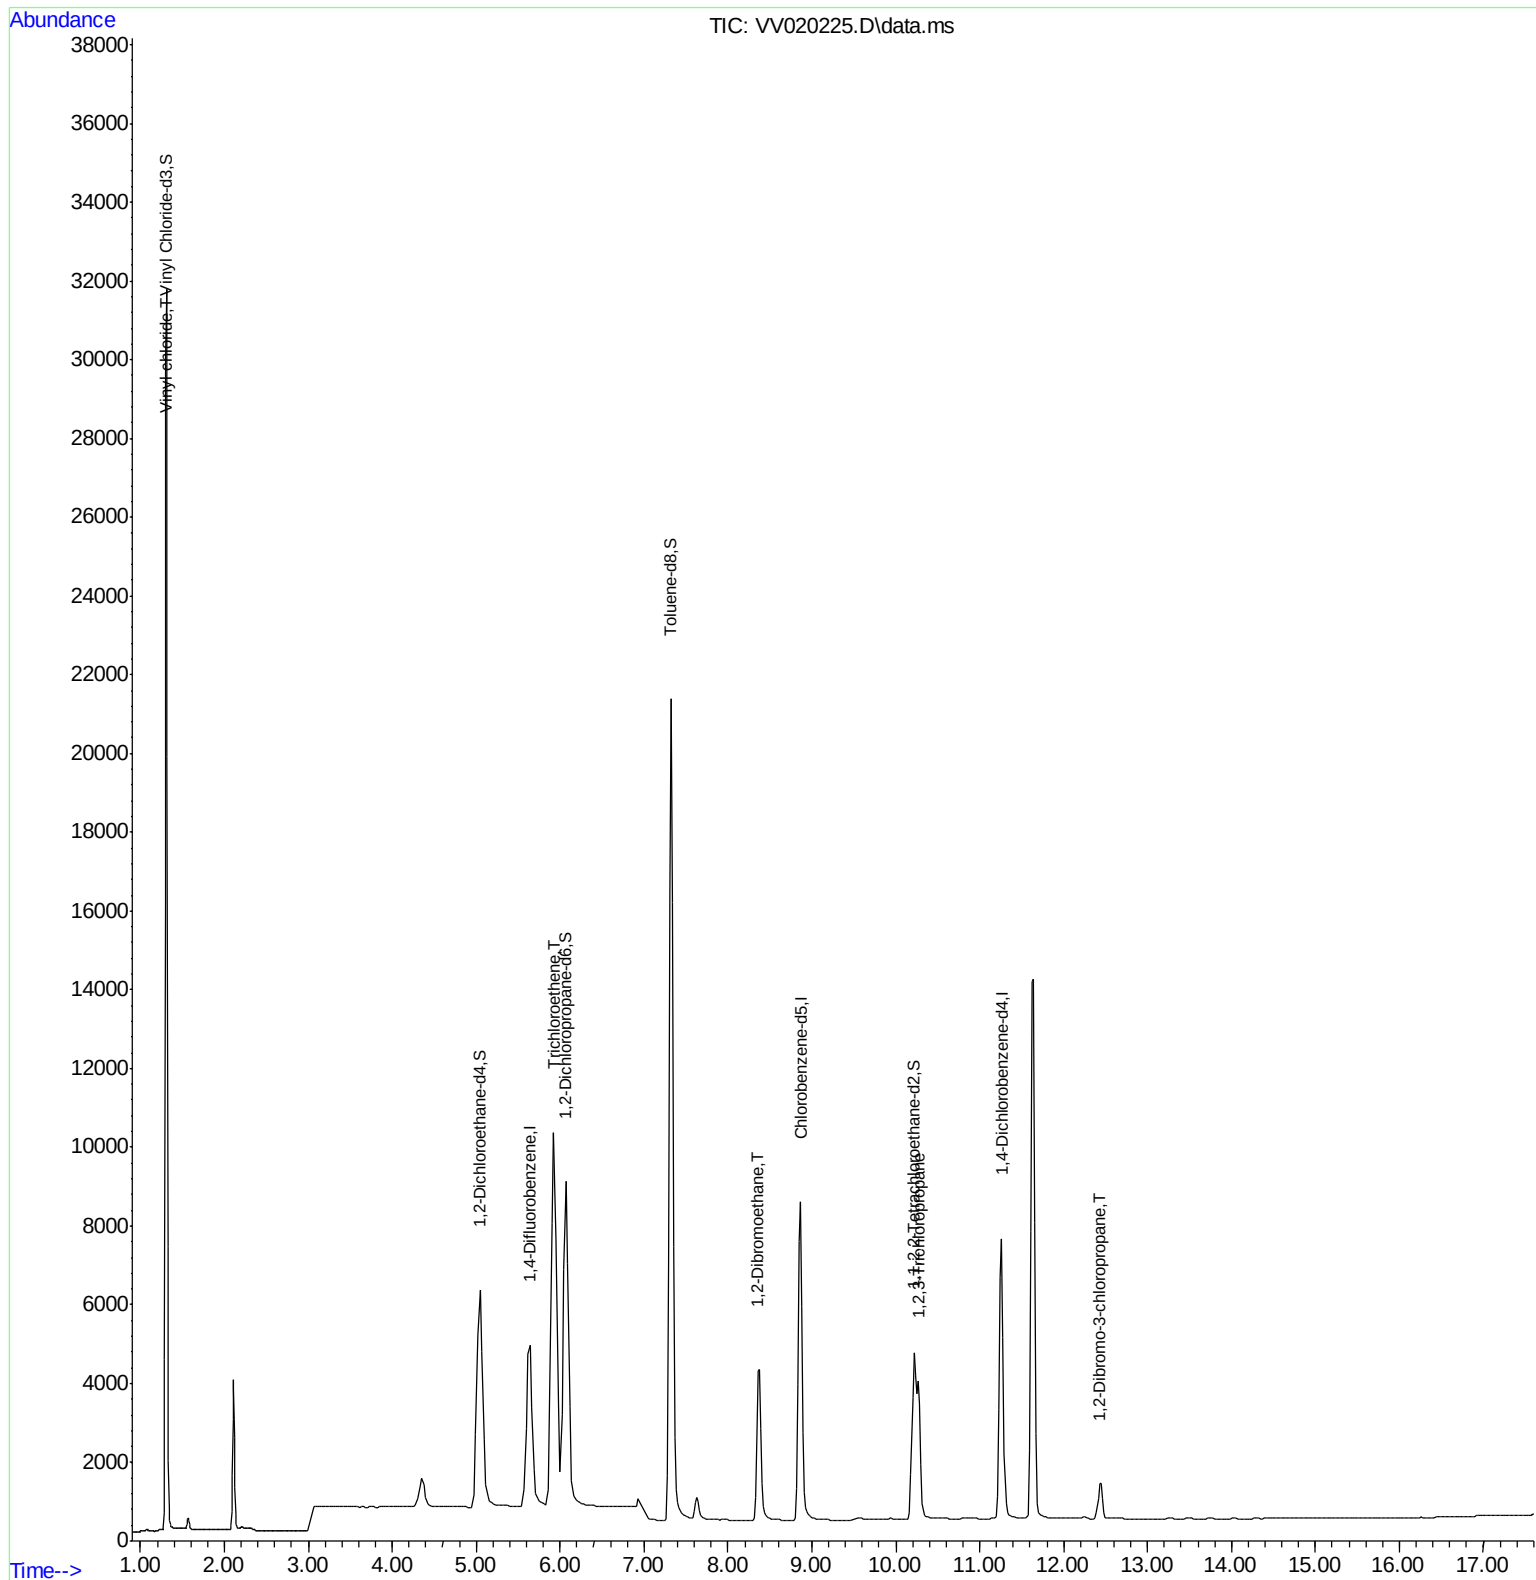


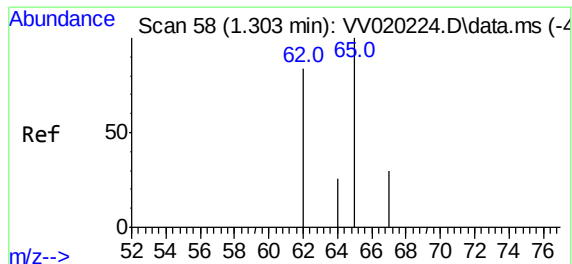

#3
Vinyl chloride
Concen: 0.83 ug/L
RT: 1.310 min Scan# 59
Delta R.T. 0.007 min
Lab File: VV020225.D
Acq: 29 Jan 2021 15:41




Instrument :
MSVOA_V
ClientSampleId :
VSTD001209


Tgt Ion: 62 Resp: 17286
Ion Ratio Lower Upper
62 100
64 34.5 22.3 41.3

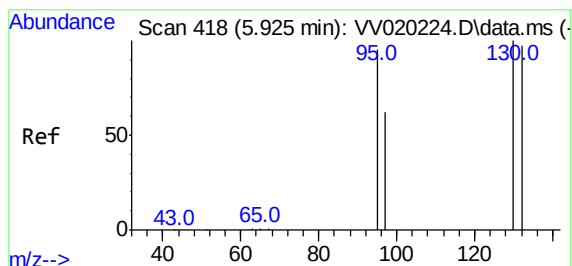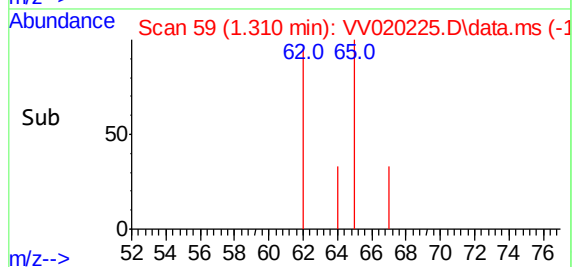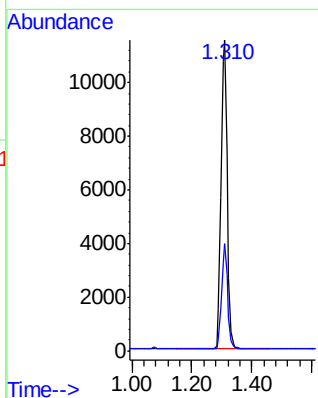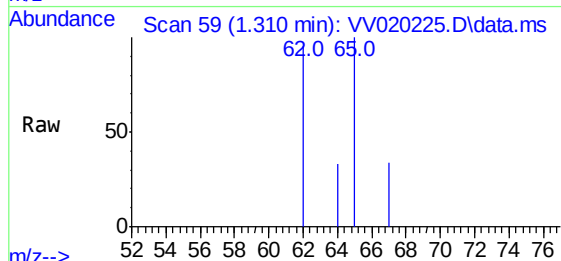

#6
Trichloroethene
Concen: 0.84 ug/L
RT: 5.925 min Scan# 418
Delta R.T. 0.000 min
Lab File: VV020225.D
Acq: 29 Jan 2021 15:41

Tgt Ion: 95 Resp: 11783
Ion Ratio Lower Upper
95 100
97 66.3 46.8 86.8
132 102.0 71.3 132.5
130 105.4 73.4 136.2


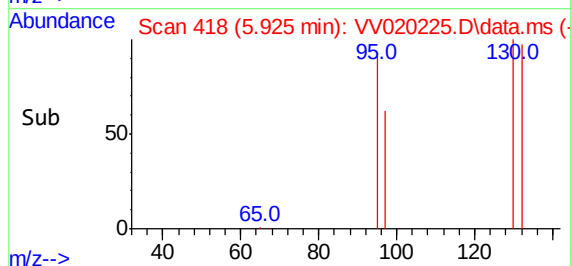
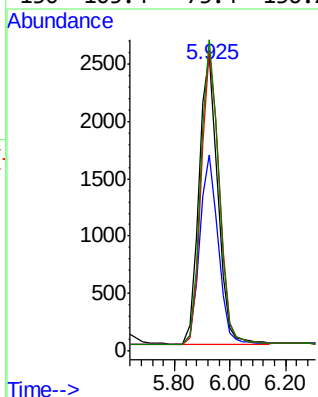
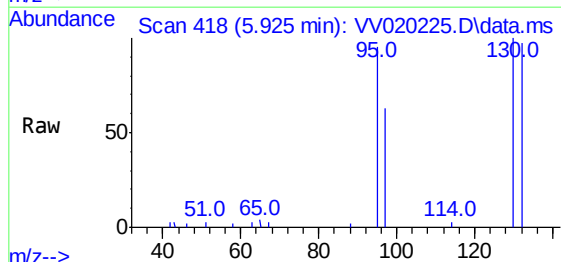


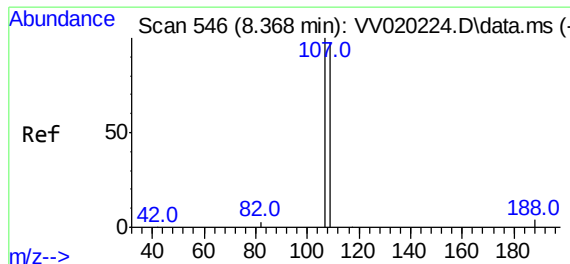

#9
1,2-Dibromoethane
Concen: 0.91 ug/L
RT: 8.353 min Scan# 545
Delta R.T. -0.015 min
Lab File: VV020225.D
Acq: 29 Jan 2021 15:41




Instrument :
MSVOA_V
ClientSampleId :
VSTD001209


Tgt Ion:107 Resp: 6835
Ion Ratio Lower Upper
107 100
109 91.2 67.8 126.0
188 5.9 7.8 11.8#

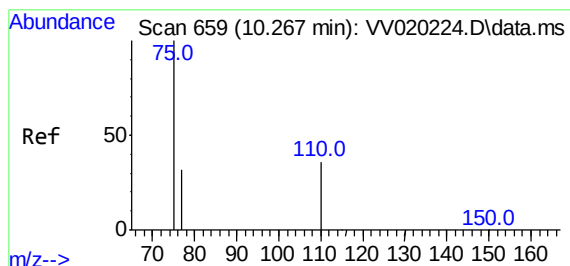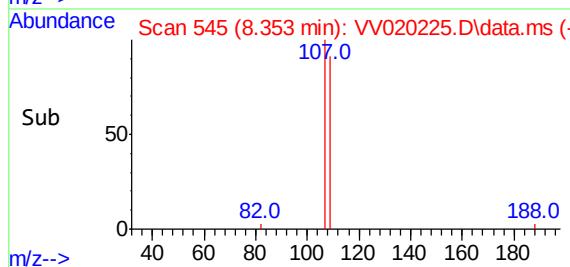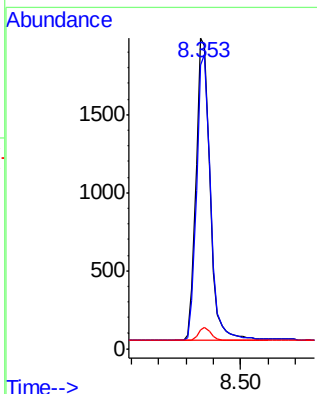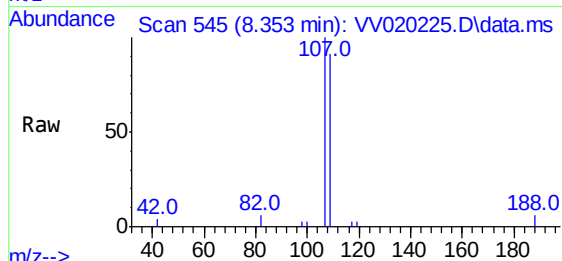

#12
1,2,3-Trichloropropane
Concen: 0.85 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020225.D
Acq: 29 Jan 2021 15:41


Tgt Ion: 75 Resp: 6477
Ion Ratio Lower Upper
75 100
110 40.0 32.4 48.6
77 32.5 26.6 40.0

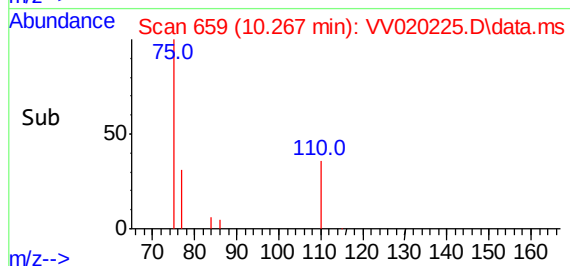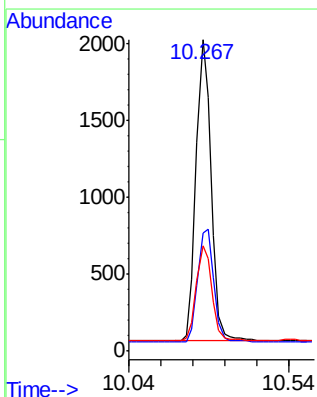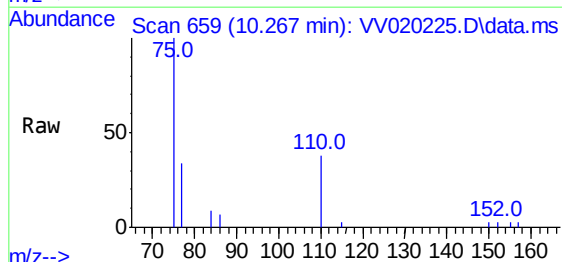

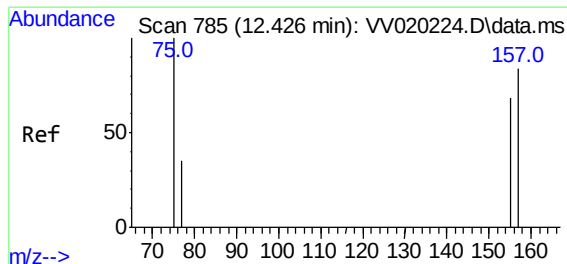

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.93 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020225.D
 Acq: 29 Jan 2021 15:41

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001209

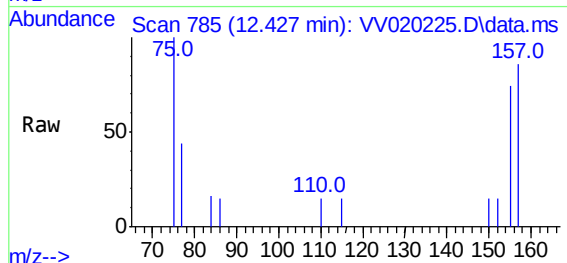

Tgt Ion: 75 Resp: 1018

Ion	Ratio	Lower	Upper
75	100		
157	86.5	67.9	101.9
155	73.5	59.1	88.7

