

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013121\
 Data File : VW020226.D
 Acq On : 29 Jan 2021 16:04
 Operator : SY/MD
 Sample : VSTD00233
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD002210

Quant Time: Jan 30 03:39:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 30 03:37:50 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	13664	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.863	117	13085	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6897	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.303	65	33129	2.65 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	20773	1.88 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	24358	1.87 ug/L	0.00
8) Toluene-d8	7.317	98	68593	2.20 ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	14644	1.91 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	30815	1.61 ug/L	Qvalue 95
6) Trichloroethene	5.925	95	21384	1.67 ug/L	99
9) 1,2-Dibromoethane	8.353	107	12541	1.83 ug/L #	93
12) 1,2,3-Trichloropropane	10.267	75	11686	1.65 ug/L	100
13) 1,2-Dibromo-3-chloropr...	12.426	75	1833	1.80 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
Data File : VV020226.D
Acq On : 29 Jan 2021 16:04
Operator : SY/MD
Sample : VSTD00233
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD002210

Quant Time: Jan 30 03:39:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 30 03:37:50 2021
Response via : Initial Calibration




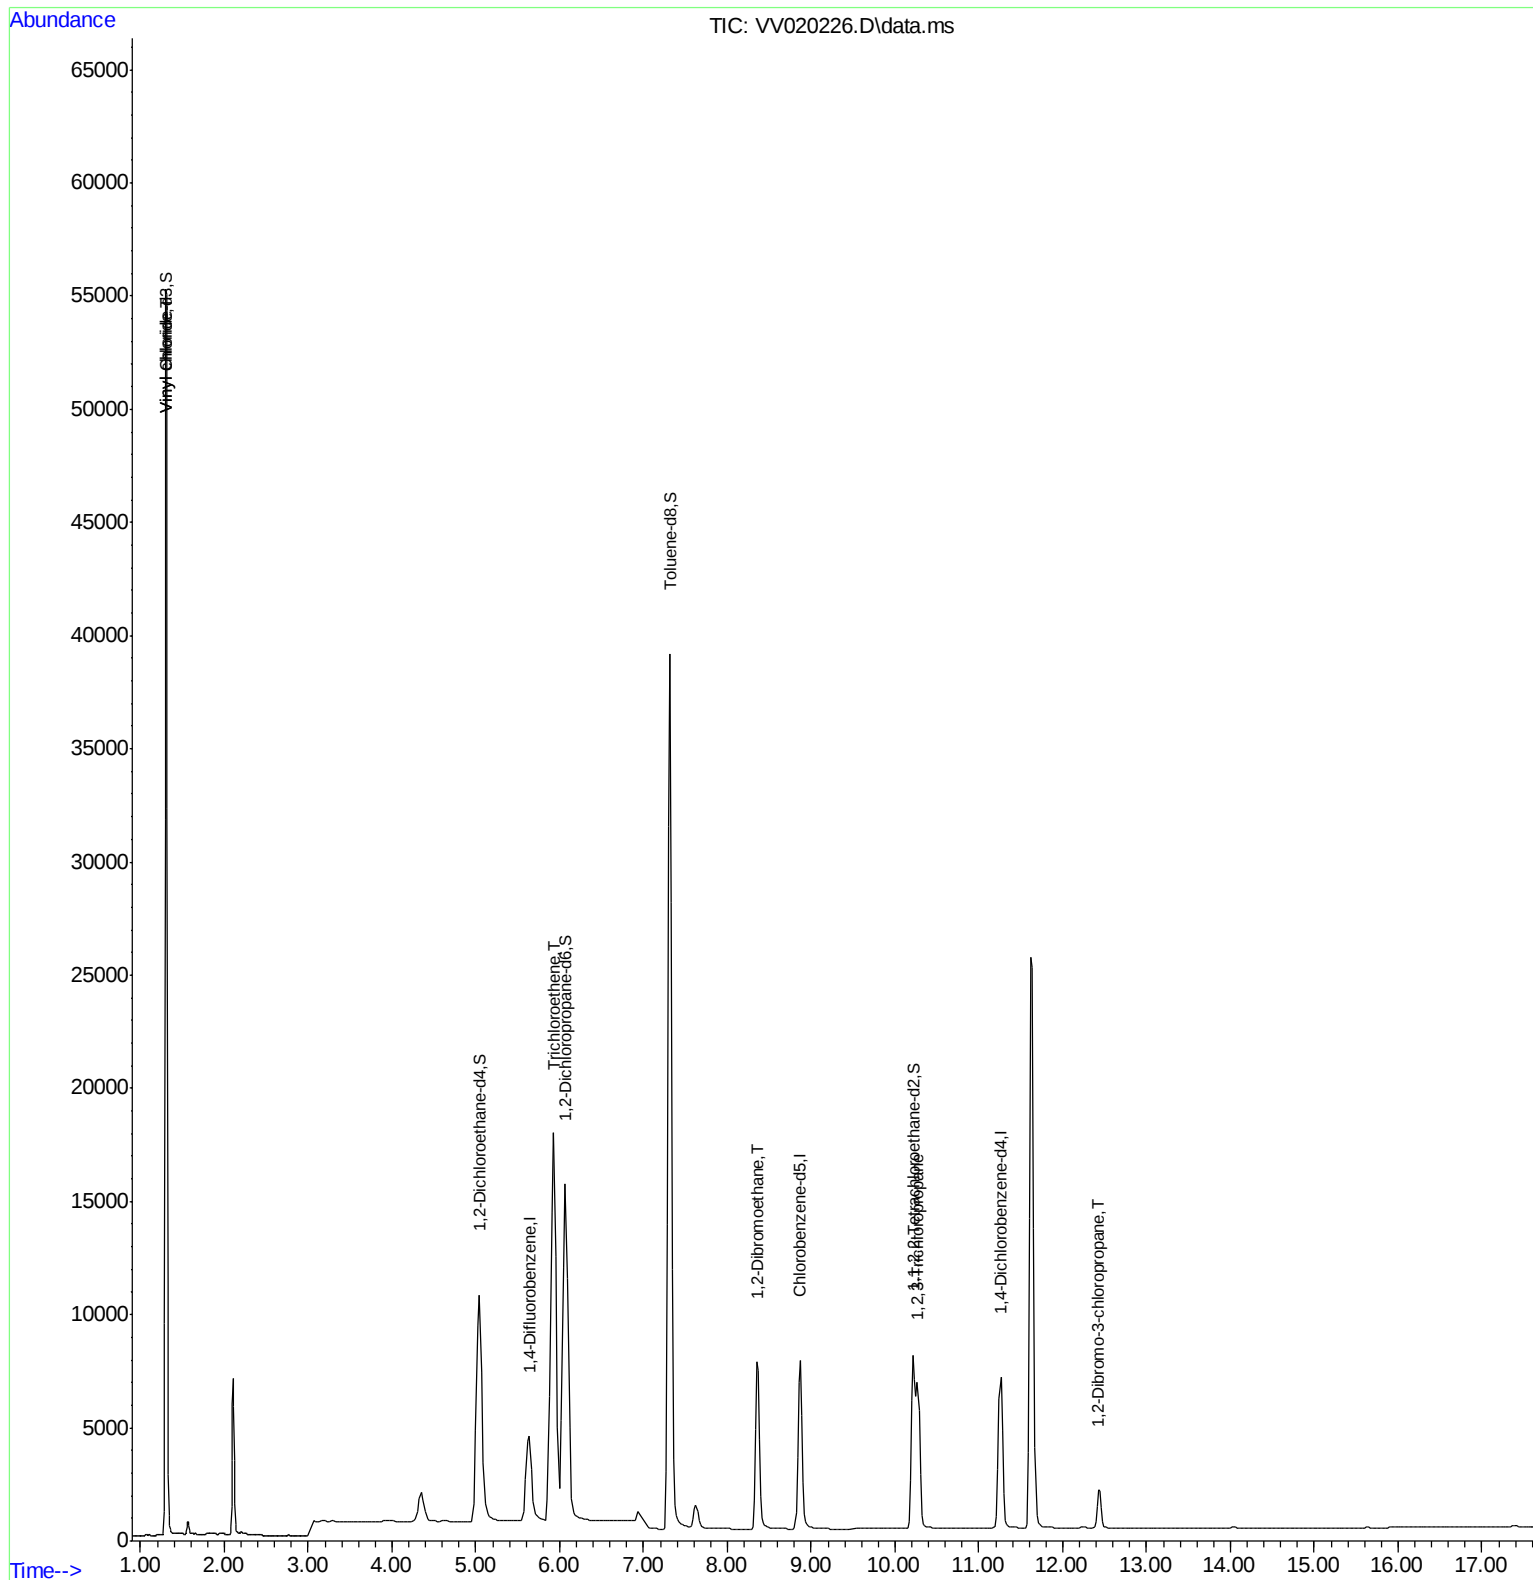


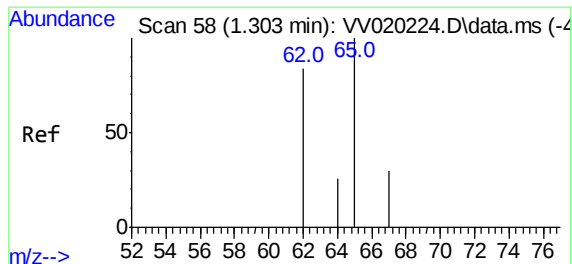

#3
 Vinyl chloride
 Concen: 1.61 ug/L
 RT: 1.310 min Scan# 59
 Delta R.T. 0.007 min
 Lab File: VV020226.D
 Acq: 29 Jan 2021 16:04




Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD002210


Tgt Ion: 62 Resp: 30815
 Ion Ratio Lower Upper
 62 100
 64 34.8 22.3 41.3

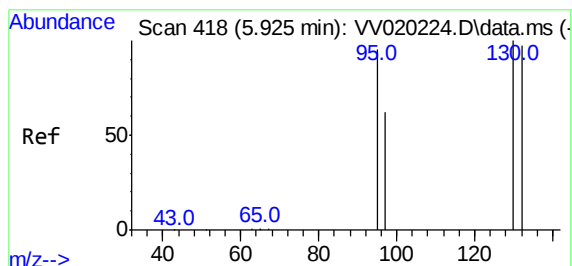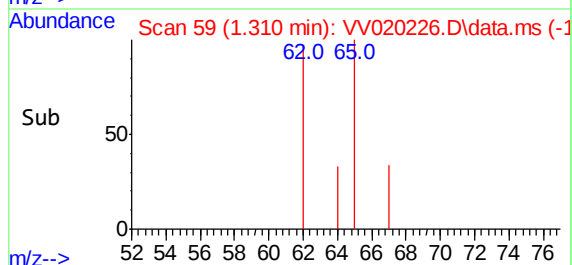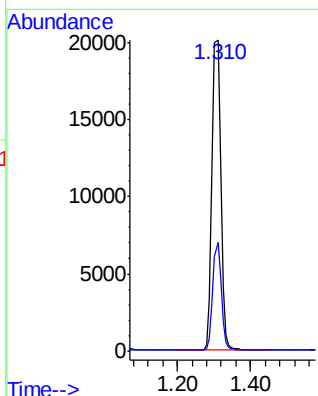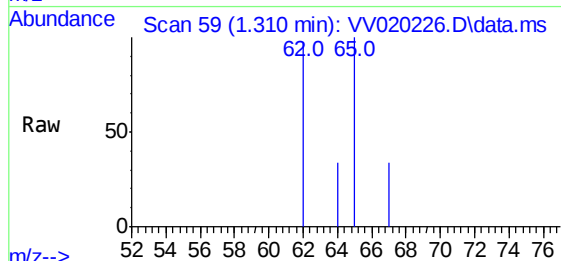

#6
 Trichloroethene
 Concen: 1.67 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. -0.000 min
 Lab File: VV020226.D
 Acq: 29 Jan 2021 16:04

Tgt Ion: 95 Resp: 21384
 Ion Ratio Lower Upper
 95 100
 97 65.6 46.8 86.8
 132 103.2 71.3 132.5
 130 105.8 73.4 136.2


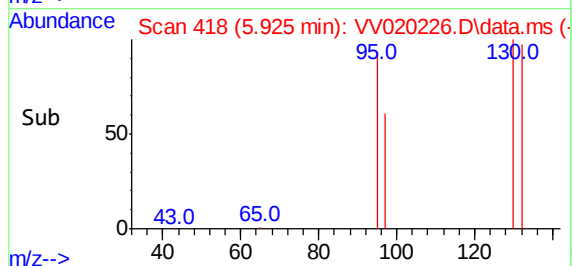
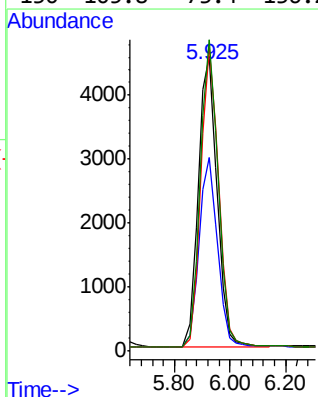
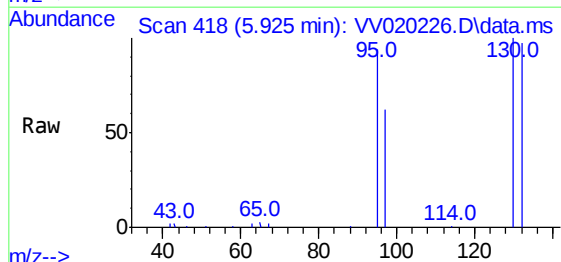


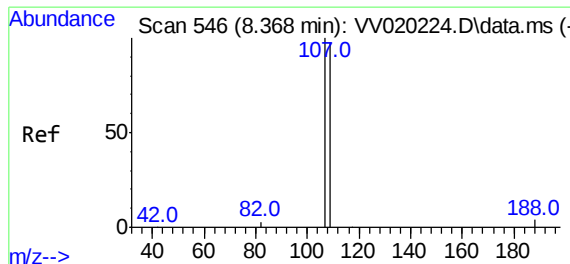

#9
1,2-Dibromoethane
Concen: 1.83 ug/L
RT: 8.353 min Scan# 545
Delta R.T. -0.016 min
Lab File: VV020226.D
Acq: 29 Jan 2021 16:04




Instrument :
MSVOA_V
ClientSampleId :
VSTD002210


Tgt Ion:107 Resp: 12541
Ion Ratio Lower Upper
107 100
109 91.2 67.8 126.0
188 4.8 7.8 11.8#

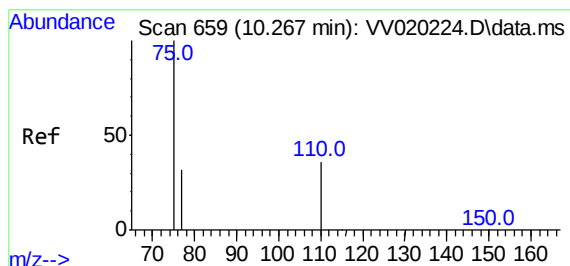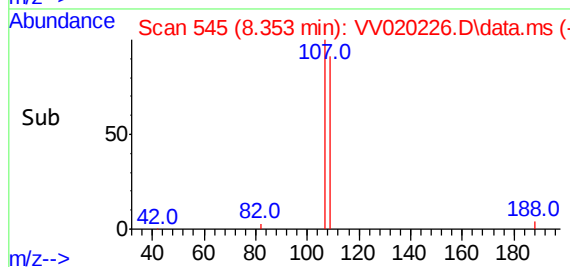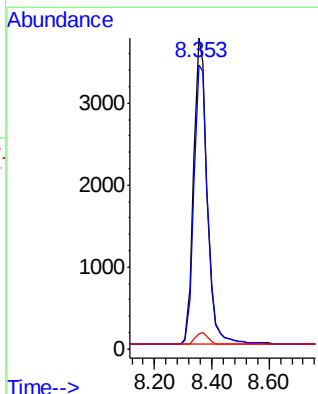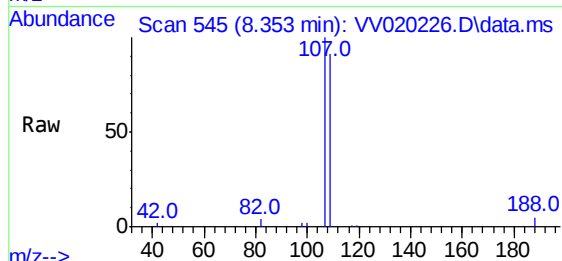

#12
1,2,3-Trichloropropane
Concen: 1.65 ug/L
RT: 10.267 min Scan# 659
Delta R.T. -0.000 min
Lab File: VV020226.D
Acq: 29 Jan 2021 16:04

Tgt Ion: 75 Resp: 11686
Ion Ratio Lower Upper
75 100
110 40.3 32.4 48.6
77 32.9 26.6 40.0

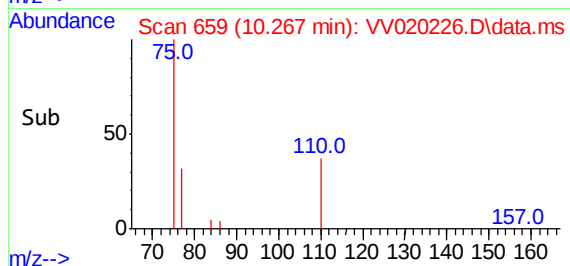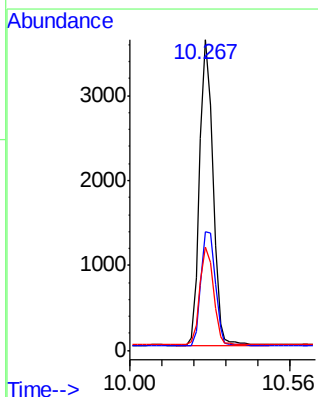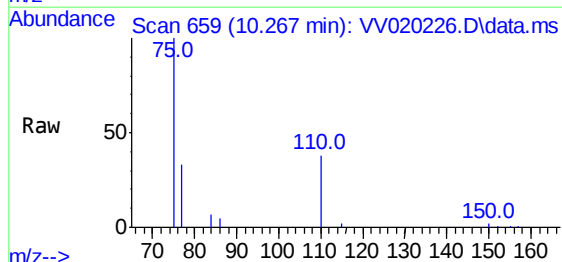

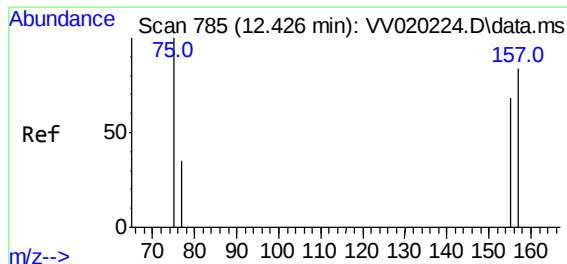

#13
 1,2-Dibromo-3-chloropropane
 Concen: 1.80 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. -0.000 min
 Lab File: VV020226.D
 Acq: 29 Jan 2021 16:04

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD002210

Tgt Ion: 75 Resp: 1833
 Ion Ratio Lower Upper
 75 100
 157 90.2 67.9 101.9
 155 74.4 59.1 88.7

