

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
 Data File : VV020228.D
 Acq On : 29 Jan 2021 17:59
 Operator : SY/MD
 Sample : VV0129WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK205

Quant Time: Jan 30 03:50:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 30 03:45:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	12848	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	12237	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6268	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	7892	0.49	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	98.00%
4) 1,2-Dichloroethane-d4	5.042	65	4859	0.50	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.00%
7) 1,2-Dichloropropane-d6	6.068	67	5798	0.52	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.00%
8) Toluene-d8	7.317	98	15362	0.49	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.00%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	3348	0.50	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	100.00%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.409	75	35	0.04	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
Data File : VV020228.D
Acq On : 29 Jan 2021 17:59
Operator : SY/MD
Sample : VV0129WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK205

Quant Time: Jan 30 03:50:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 30 03:45:01 2021
Response via : Initial Calibration

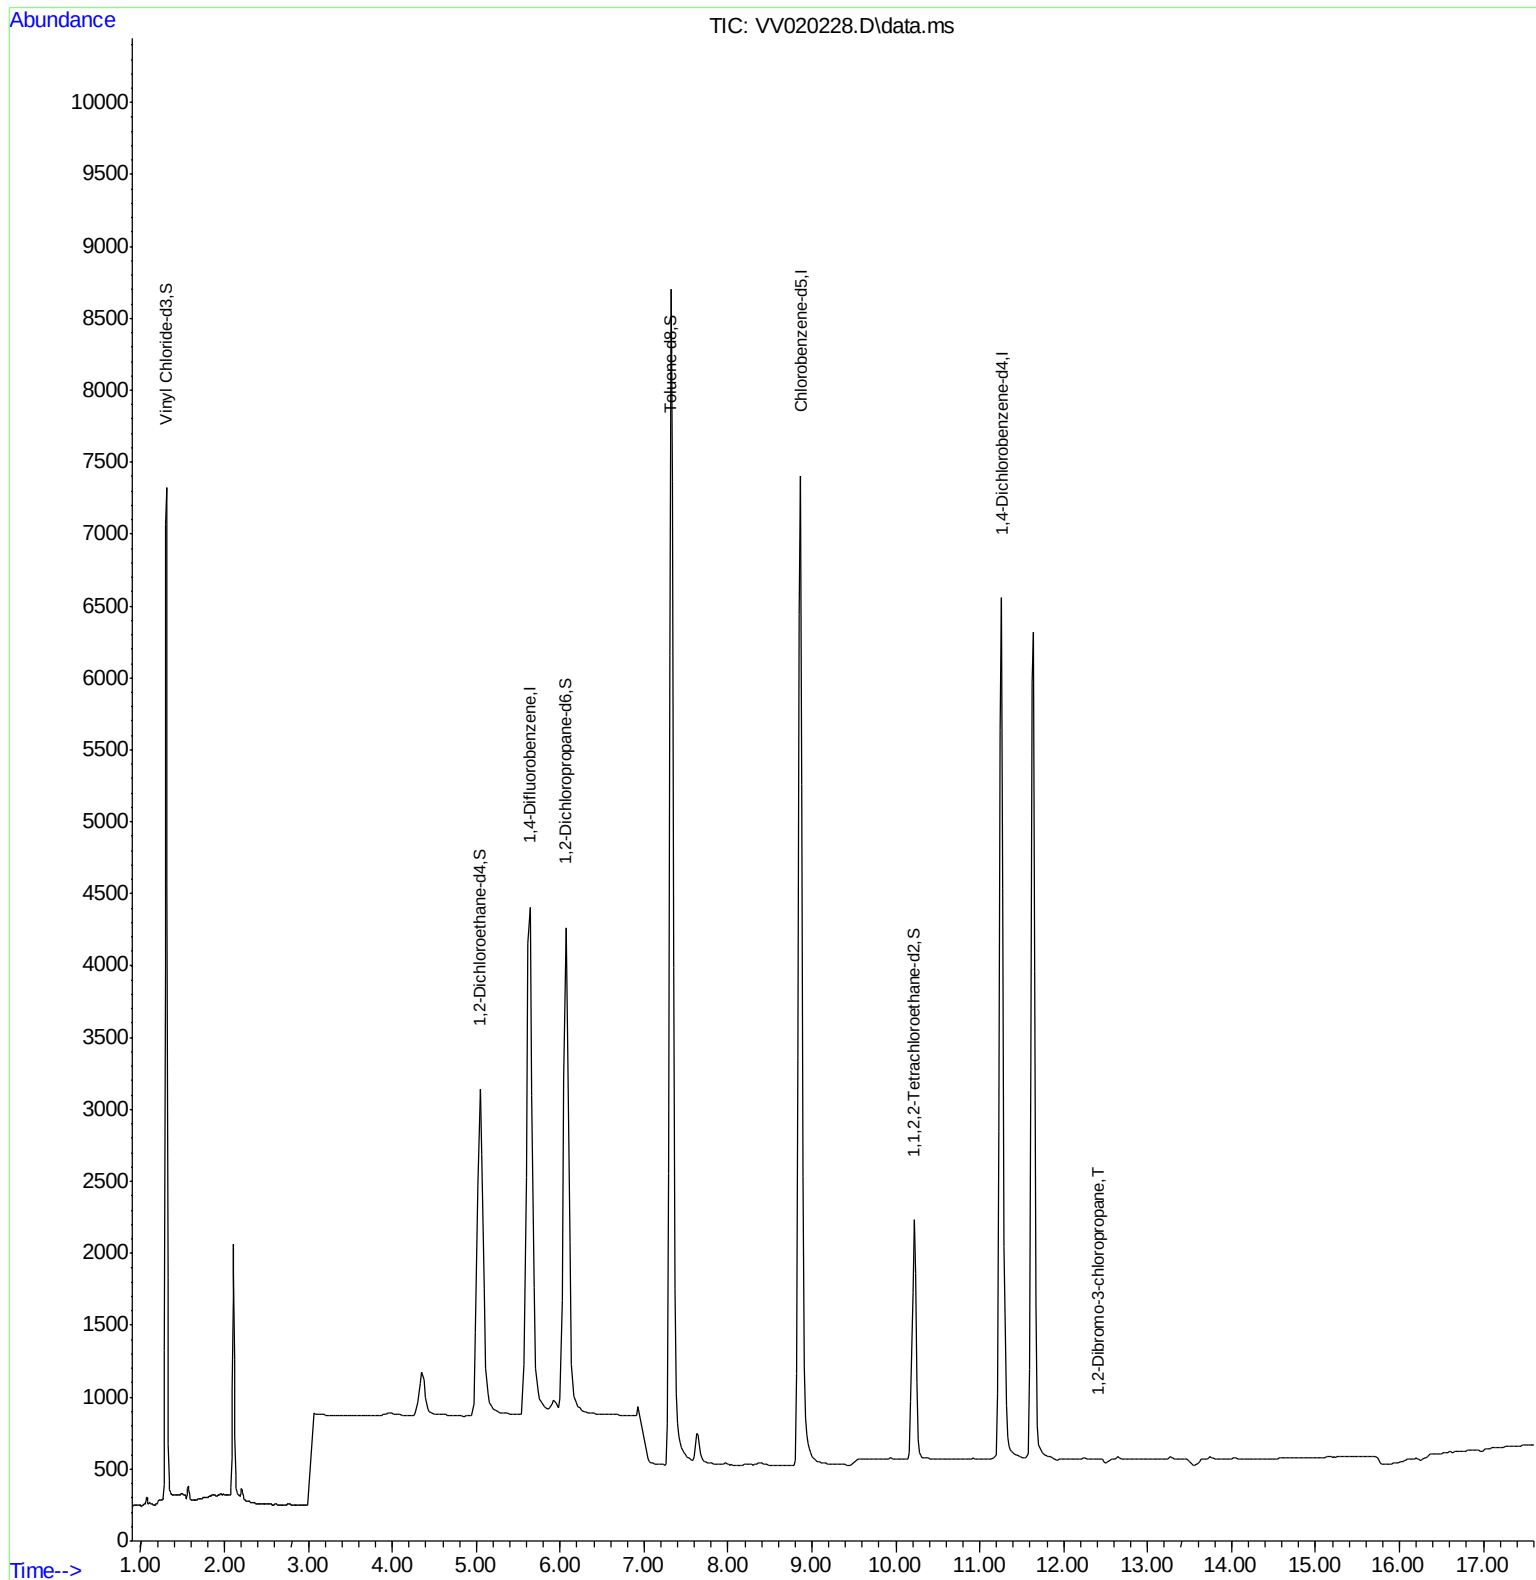

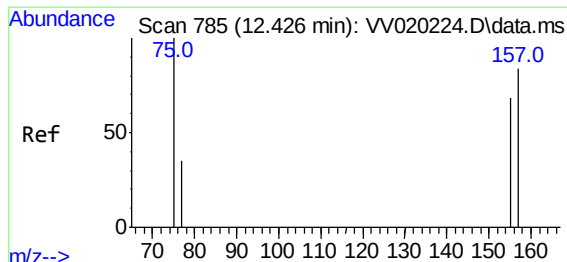

#13

1,2-Dibromo-3-chloropropane

Concen: 0.04 ug/L

RT: 12.409 min Scan# 784

Delta R.T. -0.017 min

Lab File: VV020228.D

Acq: 29 Jan 2021 17:59

Instrument :

MSVOA_V

ClientSampleId :

VBLK205


Tgt Ion: 75 Resp: 35

Ion Ratio Lower Upper

75 100

157 87.1 67.9 101.9

155 87.1 59.1 88.7

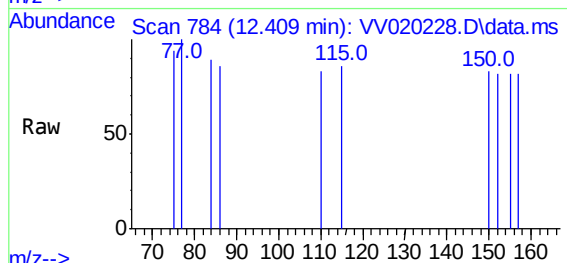

Abundance

