
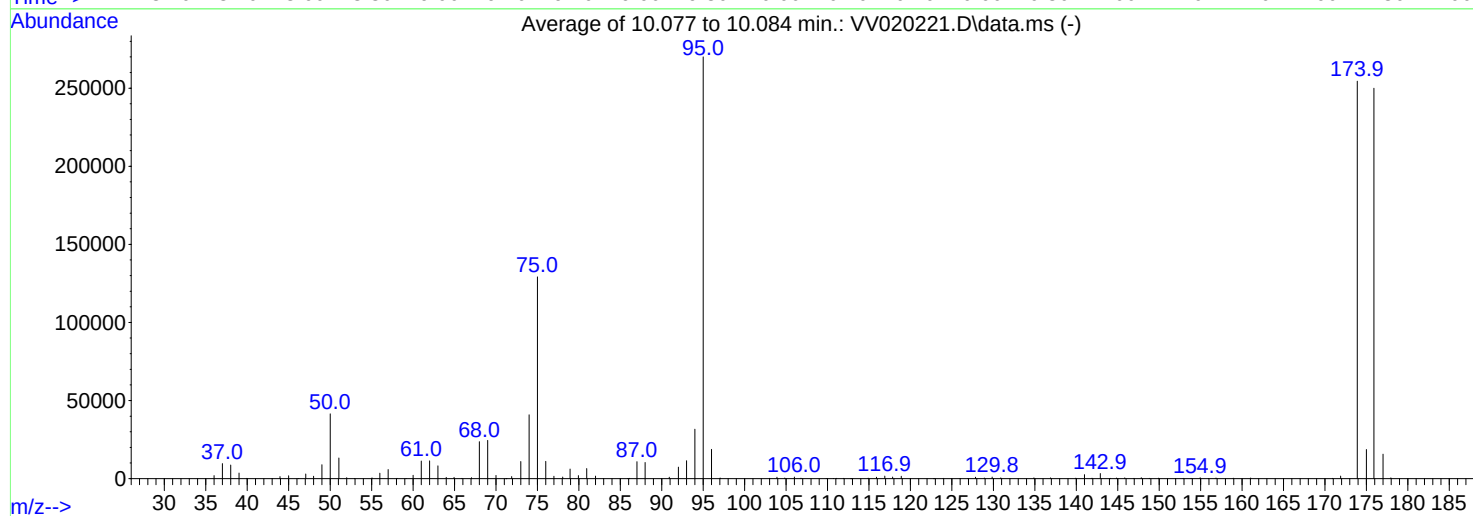


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013121\
 Data File : VV020221.D
 Acq On : 29 Jan 2021 13:10
 Operator : SY/MD
 Sample : BFB33
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB201

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM013121.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 30 03:45:01 2021

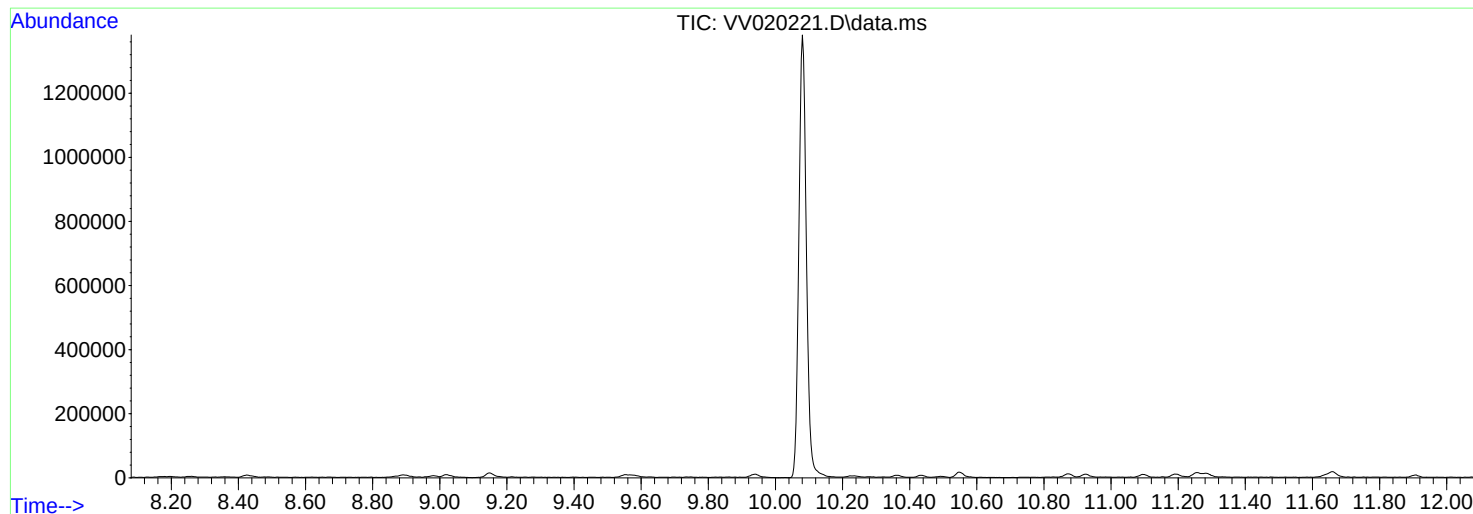

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	41499	PASS
75	95	30	80	47.8	129141	PASS
95	95	100	100	100.0	270059	PASS
96	95	5	9	7.0	18803	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.2	254507	PASS
175	174	5	9	7.3	18683	PASS
176	174	95	101	98.2	250005	PASS
177	176	5	9	6.3	15724	PASS

m/z	Abundance
36.00	1887.0
37.00	9870.0
38.00	8944.0
39.00	3648.0
40.00	390.0
43.00	157.0
44.00	1778.0
45.00	1869.0
46.20	186.0
47.10	3179.0
48.00	1544.0
49.00	8766.0
50.00	42472.0
51.10	13389.0
52.00	595.0
52.90	149.0
55.00	571.0
56.00	3429.0
57.00	5892.0
58.00	218.0
60.00	2085.0
61.00	11293.0
62.00	11311.0
63.00	8270.0
64.00	877.0
65.00	956.0
65.80	180.0
67.00	652.0
68.00	23016.0
69.00	24136.0
70.00	1922.0
71.90	1318.0
73.00	10807.0
74.00	40304.0
75.00	128408.0
76.00	11379.0
77.00	1629.0
78.10	1071.0
78.90	6060.0
79.90	2031.0
80.90	6482.0
82.00	1690.0
82.90	134.0
85.90	365.0
87.00	10689.0
88.00	10303.0
90.90	867.0
92.00	7161.0
93.00	11349.0
94.00	31440.0
95.00	265664.0
96.00	19000.0
97.10	395.0
103.00	175.0
103.90	948.0
104.80	412.0
106.00	1072.0
106.80	345.0
109.90	132.0
110.70	133.0
111.10	149.0
112.00	180.0
112.80	157.0
114.90	260.0
115.90	838.0
116.90	1703.0
117.80	965.0
118.90	1512.0
124.00	172.0
126.10	143.0
127.00	116.0
127.90	888.0
128.90	509.0
129.80	953.0
130.90	493.0
134.90	534.0
136.90	433.0
139.90	190.0
141.00	2610.0
141.90	367.0
142.90	3202.0
144.10	178.0
144.90	531.0
145.90	550.0
147.00	218.0
147.80	516.0
148.80	265.0
150.00	246.0
152.90	214.0
154.00	153.0
155.00	681.0
156.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

156.80	523.0
158.90	330.0
161.00	342.0
170.80	162.0
171.90	1607.0
173.90	244160.0
175.00	18288.0
175.90	238784.0
177.00	15841.0
177.90	440.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	2097.0
37.00	9934.0
38.00	9048.0
39.00	3753.0
40.00	394.0
43.00	116.0
44.00	1875.0
45.00	2073.0
46.20	149.0
47.10	3089.0
48.00	1624.0
49.00	9310.0
50.00	42928.0
51.10	13663.0
52.00	680.0
52.90	145.0
55.00	575.0
56.00	3645.0
57.00	6057.0
58.10	155.0
59.10	103.0
60.00	2144.0
61.00	11670.0
62.00	11768.0
63.00	8419.0
64.00	848.0
65.00	887.0
65.90	203.0
67.10	650.0
68.00	24496.0
69.00	25240.0
70.00	2122.0
71.90	1343.0
73.00	11370.0
74.00	42264.0
75.00	133312.0
76.00	11372.0
77.00	1671.0
78.10	1082.0
78.90	6314.0
80.00	2050.0
80.90	6596.0
82.00	1786.0
83.00	135.0
86.10	310.0
87.00	11274.0
88.00	10705.0
90.90	946.0
92.00	7585.0
93.00	11936.0
94.00	32784.0
95.00	279744.0
96.00	19664.0
97.00	418.0
103.00	179.0
103.90	958.0
104.80	419.0
106.00	1152.0
106.80	384.0
109.80	140.0
110.70	152.0
111.10	178.0
111.90	206.0
113.00	177.0
114.90	293.0
115.90	959.0
116.90	1735.0
117.80	1056.0
118.90	1644.0
122.80	102.0
124.00	177.0
125.90	146.0
127.00	117.0
127.80	953.0
129.00	434.0
129.80	1043.0
130.90	543.0
134.90	614.0
136.90	533.0
140.00	297.0
141.00	2708.0
141.90	318.0
142.90	3463.0
144.10	260.0
144.90	470.0
145.90	548.0
146.90	244.0
147.80	623.0
148.80	264.0
149.90	311.0
152.00	109.0
152.90	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

153.80	170.0
155.00	634.0
156.00	166.0
156.90	483.0
158.90	329.0
161.10	370.0
170.90	148.0
171.90	1755.0
173.90	263680.0
175.00	19384.0
175.90	258944.0
177.00	16232.0
178.00	492.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	1943.0
37.00	9062.0
38.00	8215.0
39.00	3284.0
40.00	365.0
44.00	1780.0
45.00	2011.0
46.10	107.0
47.00	2769.0
48.00	1518.0
49.00	8822.0
50.00	39096.0
51.00	12767.0
52.00	679.0
53.00	145.0
55.10	506.0
56.00	3319.0
57.00	5687.0
58.10	135.0
59.20	110.0
60.00	2118.0
61.00	10758.0
62.00	10935.0
63.00	7928.0
64.00	786.0
64.90	781.0
66.00	203.0
67.10	596.0
68.00	23480.0
69.00	23976.0
70.00	2144.0
71.20	164.0
71.90	1325.0
73.00	10779.0
74.00	40208.0
75.00	125704.0
76.00	10359.0
77.00	1483.0
78.00	970.0
79.00	6143.0
80.00	1961.0
81.00	6394.0
82.00	1602.0
83.00	123.0
86.10	299.0
87.00	10575.0
88.00	10029.0
90.90	908.0
92.00	7336.0
93.00	11316.0
94.00	30784.0
95.00	264768.0
96.00	17744.0
97.00	458.0
103.00	154.0
103.90	979.0
104.90	426.0
106.00	1028.0
106.80	286.0
109.80	139.0
111.00	204.0
111.90	269.0
113.10	209.0
114.90	316.0
115.90	1091.0
116.90	1641.0
117.90	975.0
118.90	1579.0
123.90	180.0
126.00	142.0
126.90	110.0
127.90	906.0
128.80	361.0
129.90	989.0
130.90	480.0
134.90	539.0
136.90	515.0
140.00	363.0
141.00	2536.0
141.90	291.0
142.90	3243.0
144.10	266.0
144.80	371.0
145.80	496.0
146.90	209.0
147.90	676.0
148.80	206.0
149.90	330.0
151.90	111.0
152.90	241.0
153.80	208.0
154.90	580.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

155.90	150.0
156.90	387.0
159.00	391.0
160.90	315.0
161.20	322.0
171.00	193.0
171.90	1690.0
173.90	255680.0
175.00	18376.0
175.90	252288.0
177.00	15099.0
178.00	554.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
39.90	206.0
43.90	470.0
45.10	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201