




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
 Data File : VV030007.D
 Acq On : 31 Jan 2023 11:53
 Operator : SY/MD
 Sample : 01315-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B57

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:14:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 01 00:13:14 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/02/2023

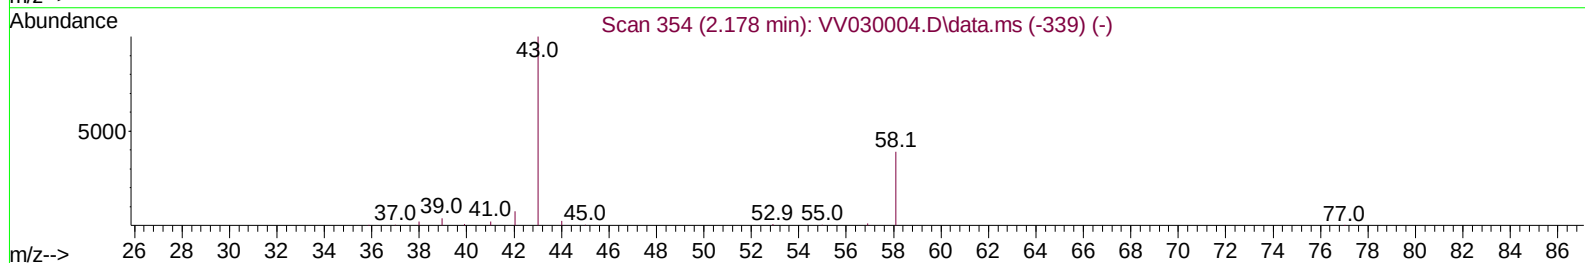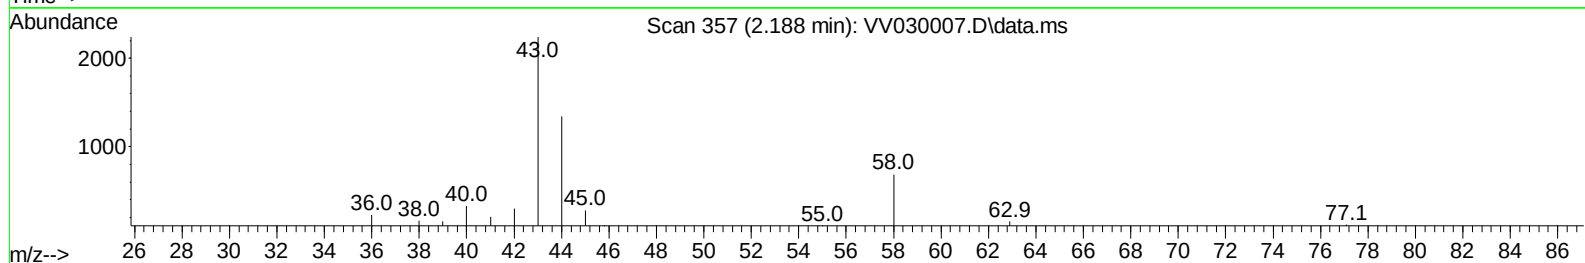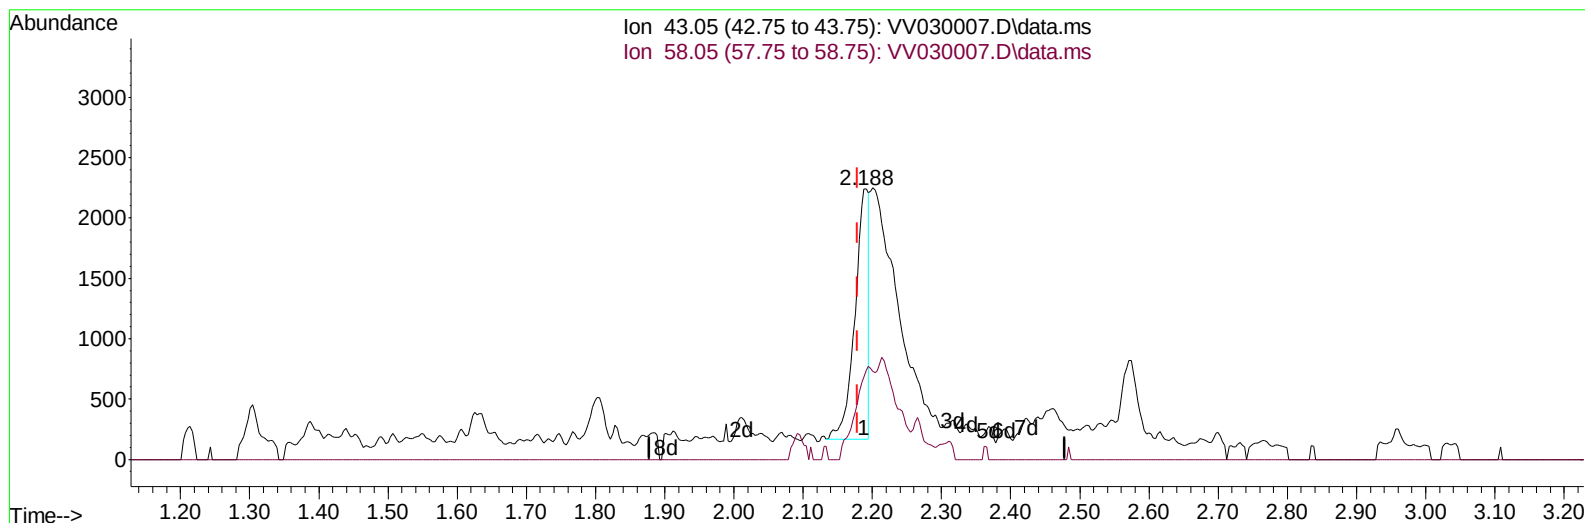

TIC: VV030007.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 1.31 ug/L

response 2908

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	51.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
 Data File : VV030007.D
 Acq On : 31 Jan 2023 11:53
 Operator : SY/MD
 Sample : 01315-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B57

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:14:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 01 00:13:14 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/02/2023

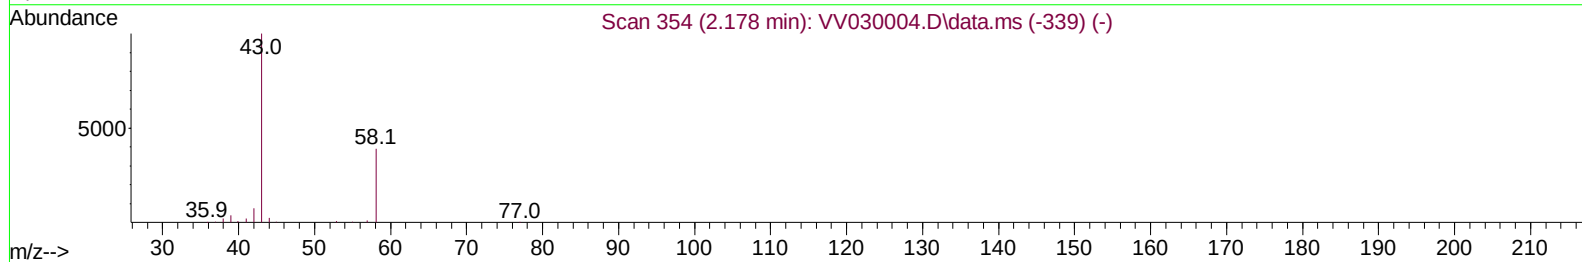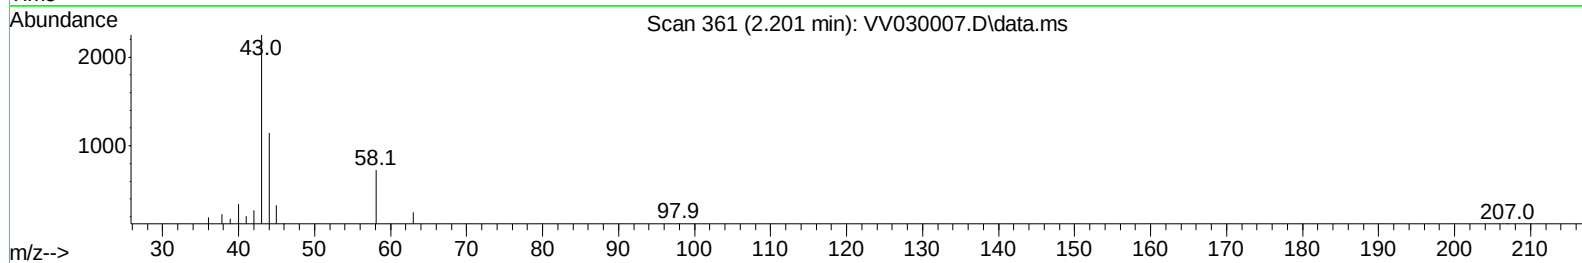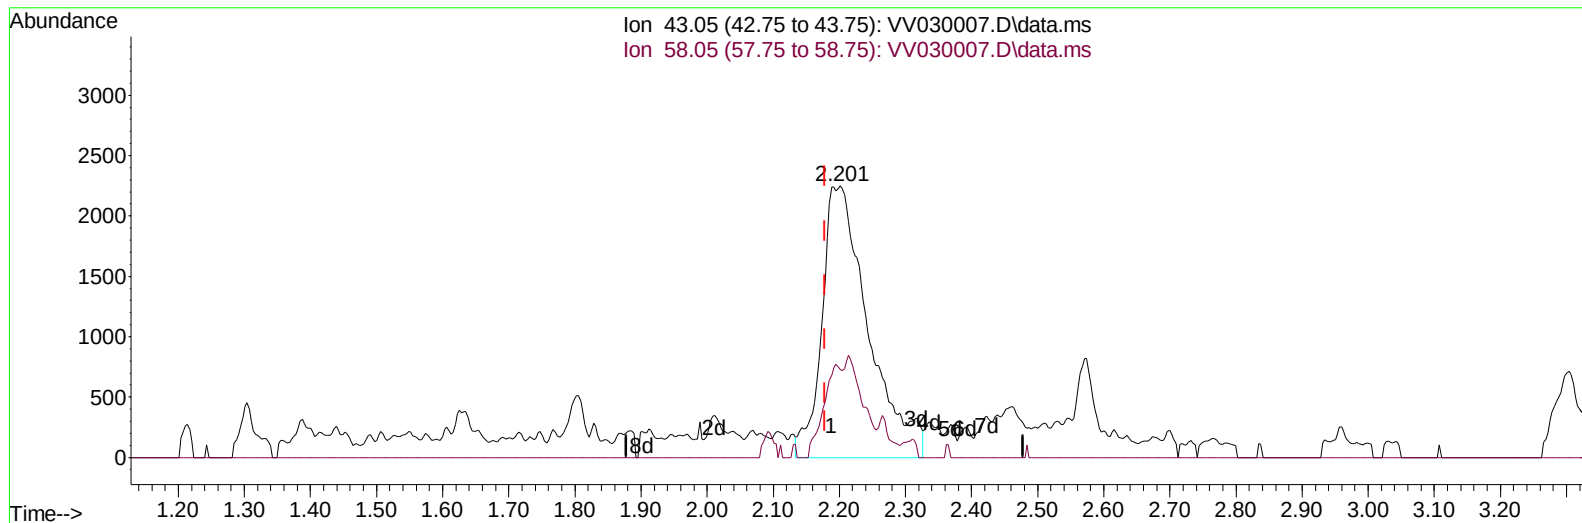

TIC: VV030007.D\data.ms

(13) Acetone (T)

2.201min (+ 0.023) 4.93 ug/L m

response 10972

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	13.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
 Data File : VV030007.D
 Acq On : 31 Jan 2023 11:53
 Operator : SY/MD
 Sample : 01315-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B57

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:14:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 01 00:13:14 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
 Supervised By :Mahesh Dadoda 02/02/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	232034	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	222474	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	110481	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	80443	4.571	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	91.400%		
7) Chloroethane-d5	1.564	69	76125	5.218	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	104.400%		
11) 1,1-Dichloroethene-d2	2.105	63	113623	3.541	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	70.800%		
20) 2-Butanone-d5	3.905	46	160492	51.450	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	102.900%		
24) Chloroform-d	4.339	84	146819	4.548	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	91.000%		
26) 1,2-Dichloroethane-d4	5.027	65	66905	4.893	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.800%		
32) Benzene-d6	5.043	84	314935	4.772	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.400%		
36) 1,2-Dichloropropane-d6	6.063	67	101459	5.253	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	105.000%		
41) Toluene-d8	7.310	98	264858	4.335	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	86.800%		
43) trans-1,3-Dichloroprop...	7.616	79	32141	4.557	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	91.200%		
46) 2-Hexanone-d5	8.085	63	146355	50.965	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	101.940%		
56) 1,1,2,2-Tetrachloroeth...	10.204	84	67558	4.773	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	95.400%		
66) 1,2-Dichlorobenzene-d4	11.612	152	95888	4.774	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	95.400%		
Target Compounds						
13) Acetone	2.201	43	10972m	4.928	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030007.D
Acq On : 31 Jan 2023 11:53
Operator : SY/MD
Sample : 01315-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B57

Manual IntegrationsAPPROVED

Quant Time: Feb 01 00:14:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 01 00:13:14 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 02/01/2023
Supervised By :Mahesh Dadoda 02/02/2023

