

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013123\
 Data File : VW030008.D
 Acq On : 31 Jan 2023 12:48
 Operator : SY/MD
 Sample : 01315-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B58

Quant Time: Feb 01 00:14:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 01 00:13:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	245081	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	231893	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	115462	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	84375	4.539	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.800%
7) Chloroethane-d5	1.564	69	79039	5.129	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.600%
11) 1,1-Dichloroethene-d2	2.101	63	111586	3.293	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.800%
20) 2-Butanone-d5	3.876	46	141802	43.038	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.080%
24) Chloroform-d	4.333	84	146128	4.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
26) 1,2-Dichloroethane-d4	5.018	65	62145	4.303	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
32) Benzene-d6	5.037	84	306456	4.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	6.056	67	98297	4.883	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.304	98	257386	4.042	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.800%
43) trans-1,3-Dichloroprop...	7.609	79	30292	4.120	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	8.079	63	126497	42.261	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.520%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	62538	4.239	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.800%
66) 1,2-Dichlorobenzene-d4	11.609	152	91992	4.382	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.600%
Target Compounds						Qvalue
13) Acetone	2.172	43	7094	3.017	ug/L	92
16) Methylene chloride	2.500	84	6998	0.269	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030008.D
Acq On : 31 Jan 2023 12:48
Operator : SY/MD
Sample : 01315-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B58

Quant Time: Feb 01 00:14:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 01 00:13:14 2023
Response via : Initial Calibration

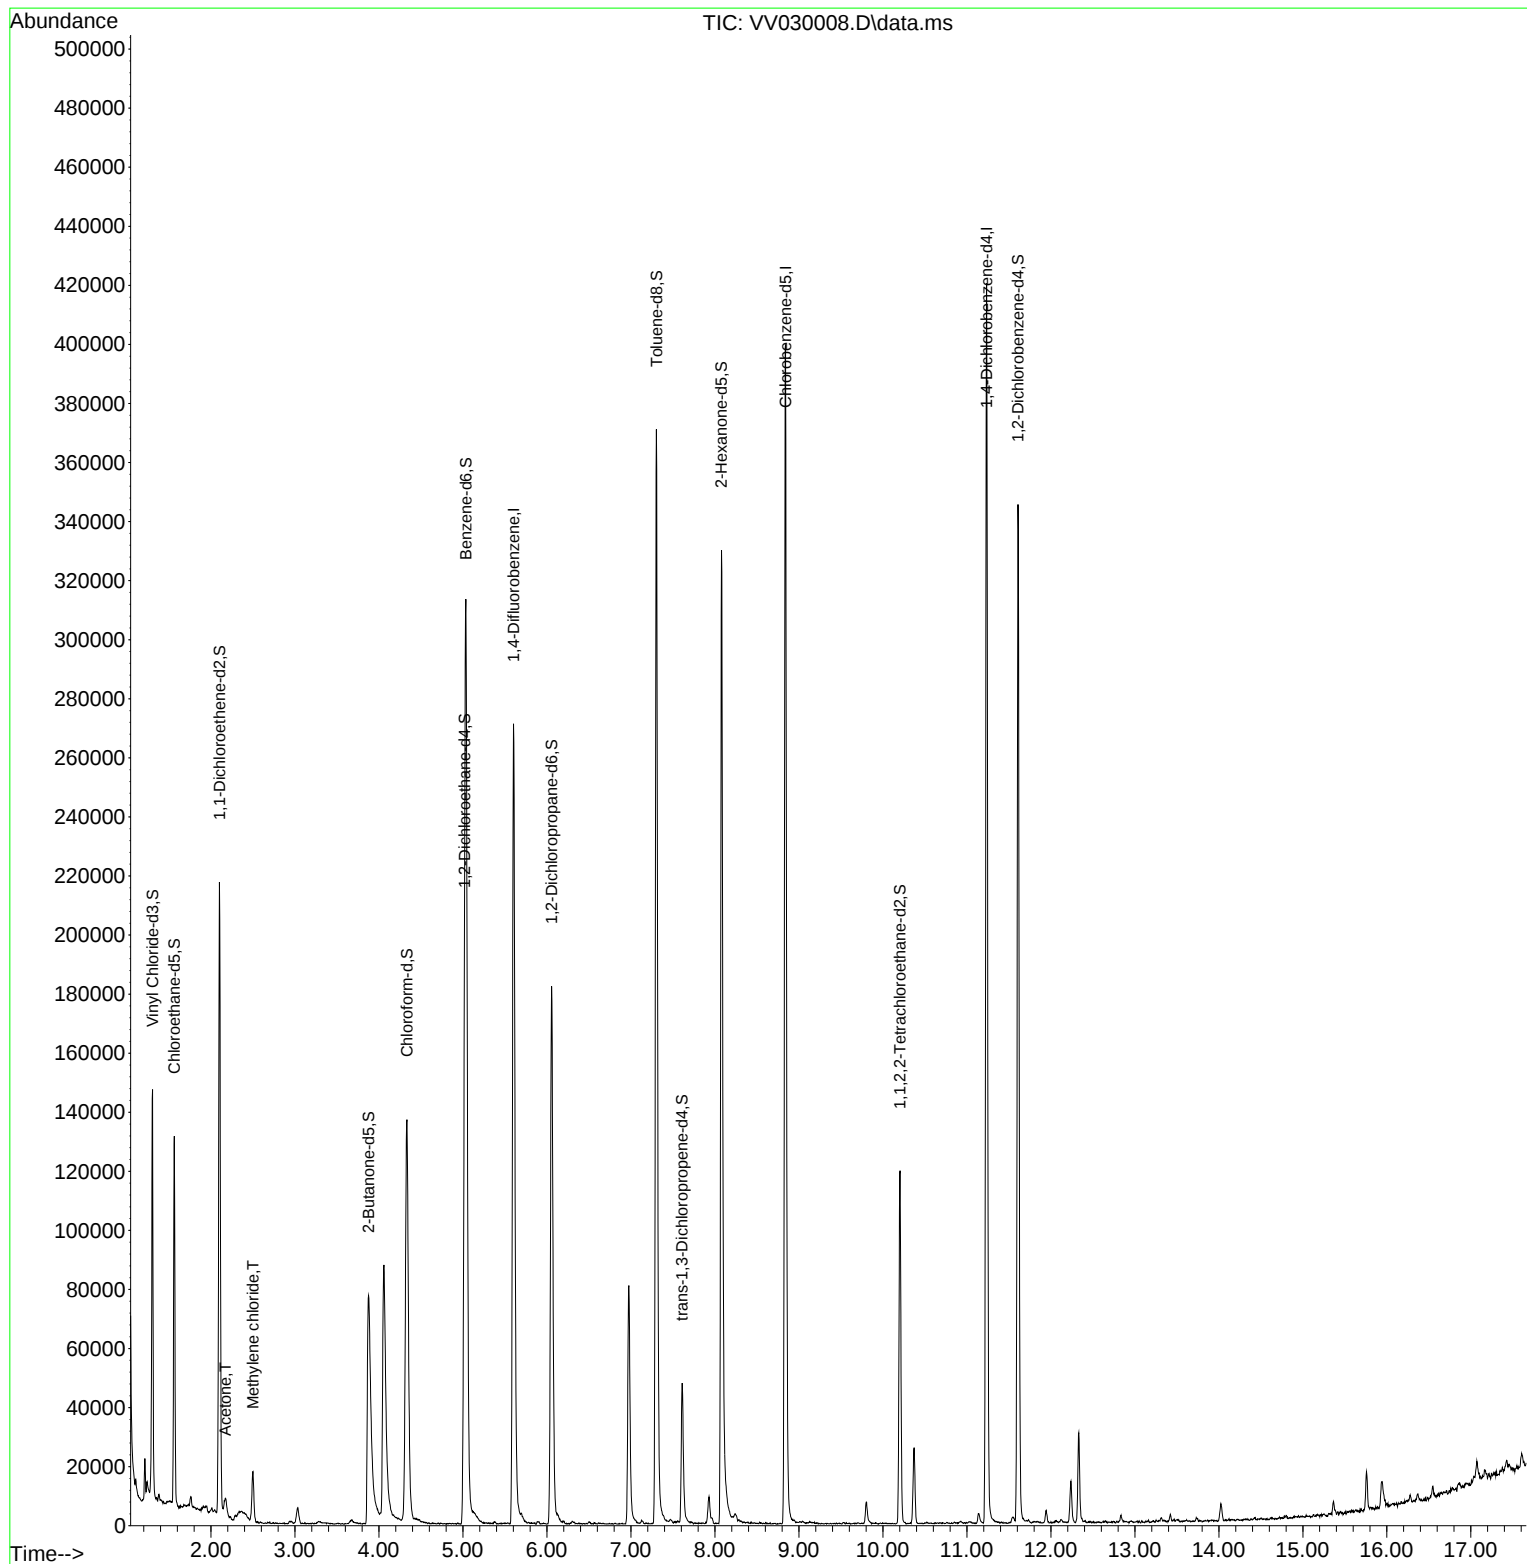

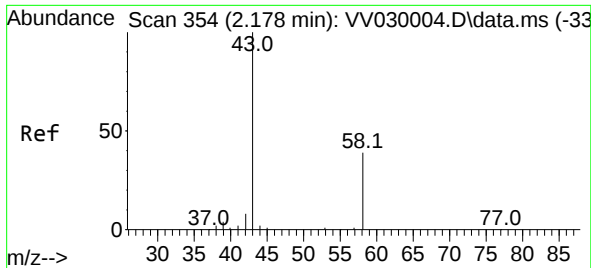

#13

Acetone

Concen: 3.017 ug/L

RT: 2.172 min Scan# 3

Delta R.T. -0.006 min

Lab File: VV030008.D

Acq: 31 Jan 2023 12:48

Instrument :

MSVOA_V

ClientSampleId :





C0B58

Tgt Ion: 43 Resp: 7094

Ion Ratio Lower Upper

43 100

58 39.0 0.0 68.8

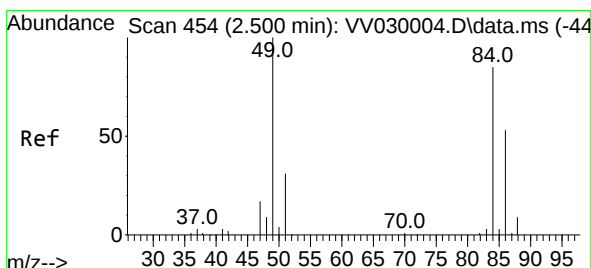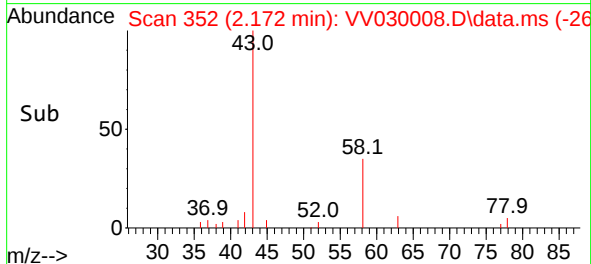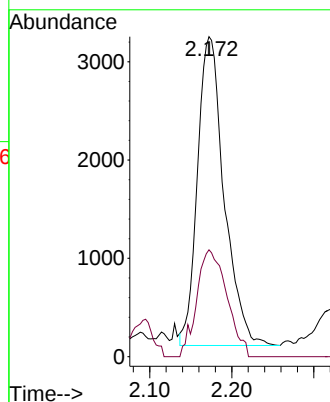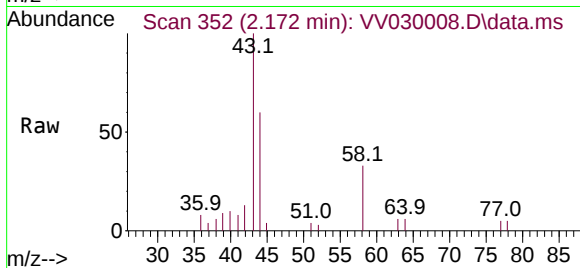

#16

Methylene chloride

Concen: 0.269 ug/L

RT: 2.500 min Scan# 454

Delta R.T. 0.000 min

Lab File: VV030008.D

Acq: 31 Jan 2023 12:48

Tgt Ion: 84 Resp: 6998

Ion Ratio Lower Upper

84 100

86 63.0 45.0 83.6

49 116.3 71.5 132.7

