

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
 Data File : VV030009.D
 Acq On : 31 Jan 2023 13:12
 Operator : SY/MD
 Sample : 01315-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B56

Quant Time: Feb 01 00:15:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 01 00:13:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	237403	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	220100	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	109371	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	85564	4.752	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.564	69	79628	5.335	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.600%
11) 1,1-Dichloroethene-d2	2.101	63	114476	3.487	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.800%
20) 2-Butanone-d5	3.879	46	157800	49.443	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.880%
24) Chloroform-d	4.336	84	151285	4.580	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.021	65	65172	4.659	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.040	84	319218	4.889	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	6.059	67	101003	5.286	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.800%
41) Toluene-d8	7.307	98	264198	4.371	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.612	79	31095	4.456	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.082	63	137055	48.241	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.480%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	64649	4.617	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.400%
66) 1,2-Dichlorobenzene-d4	11.612	152	94101	4.732	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.600%
Target Compounds					Qvalue	
13) Acetone	2.172	43	11056	4.853	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030009.D
Acq On : 31 Jan 2023 13:12
Operator : SY/MD
Sample : 01315-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B56

Quant Time: Feb 01 00:15:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 01 00:13:14 2023
Response via : Initial Calibration

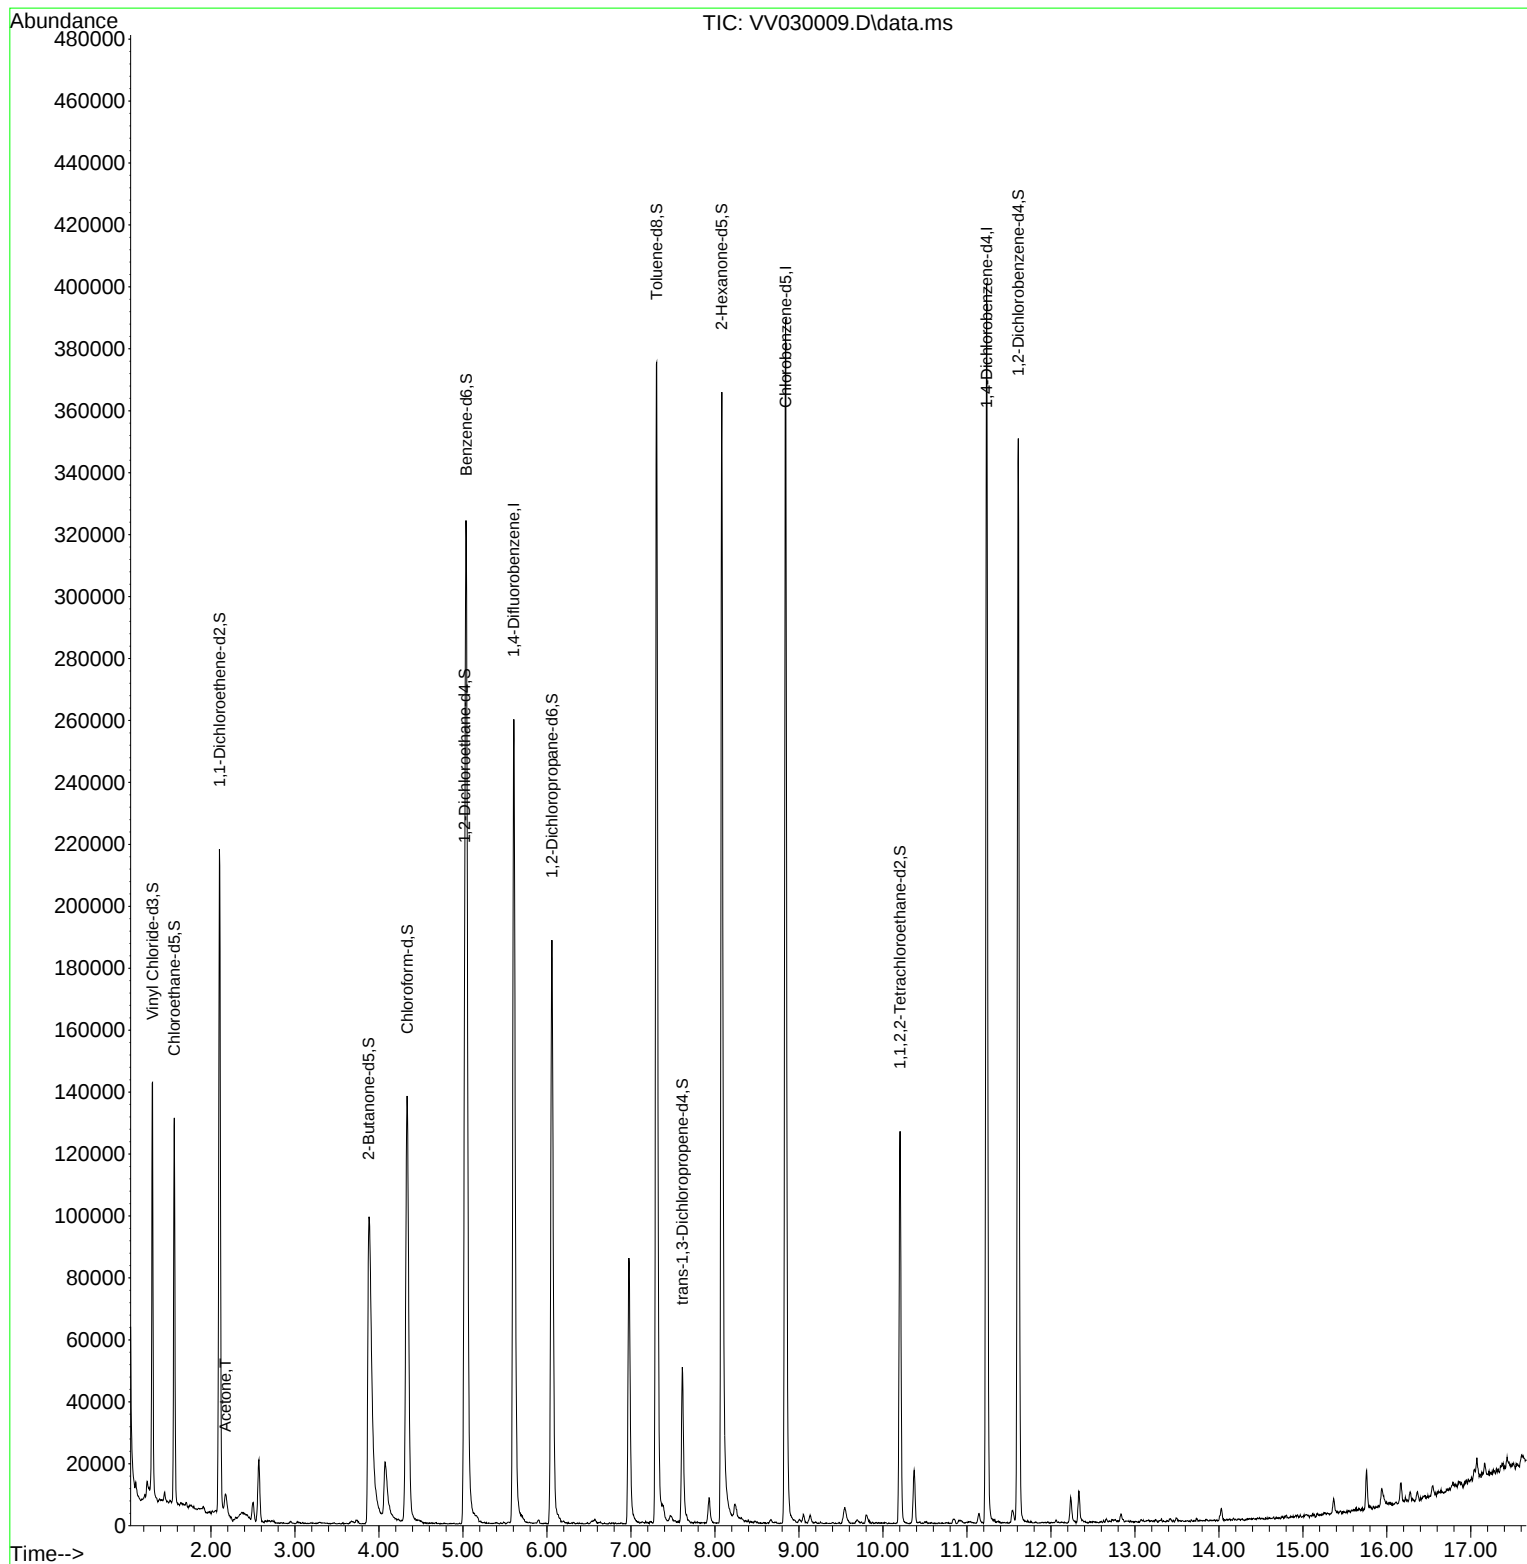

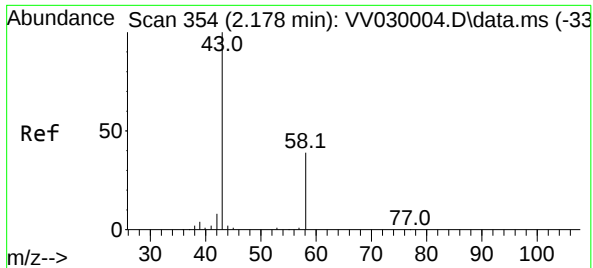

#13

Acetone

Concen: 4.853 ug/L

RT: 2.172 min Scan# 31

Delta R.T. -0.006 min

Lab File: VV030009.D


Acq: 31 Jan 2023 13:12

Instrument :

MSVOA_V

ClientSampleId :

C0B56

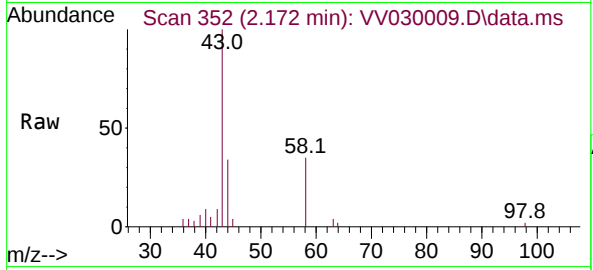

Tgt Ion: 43 Resp: 11056

Ion Ratio Lower Upper

43 100

58 39.6 0.0 68.8

