

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
 Data File : VV030005.D
 Acq On : 31 Jan 2023 11:05
 Operator : SY/MD
 Sample : VV0131WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK300

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	131379	136024	16.92%	2.071%
2	1.565	155	163	175	rVB	123787	138721	17.25%	2.112%
3	2.102	320	330	346	rBV	217204	311702	38.77%	4.746%
4	2.500	446	454	465	rVB2	6046	10075	1.25%	0.153%
5	3.886	874	885	917	rBV	77325	252361	31.39%	3.842%
6	4.336	1003	1025	1048	rBV2	135771	340710	42.38%	5.188%
7	5.037	1225	1243	1276	rBV2	317516	804002	100.00%	12.241%
8	5.606	1404	1420	1447	rBV	264429	537085	66.80%	8.177%
9	6.060	1544	1561	1593	rBV	187454	388234	48.29%	5.911%
10	6.976	1835	1846	1870	rBV	84817	157182	19.55%	2.393%
11	7.307	1936	1949	1975	rBV	377650	670965	83.45%	10.216%
12	7.613	2033	2044	2068	rBV	50862	90331	11.24%	1.375%
13	8.082	2179	2190	2221	rBV	361557	643645	80.06%	9.800%
14	8.413	2283	2293	2307	rBV2	5423	9894	1.23%	0.151%
15	8.841	2412	2426	2452	rBV	382898	640947	79.72%	9.759%
16	10.204	2839	2850	2863	rBV	128579	203105	25.26%	3.092%
17	11.236	3159	3171	3197	rBV	411055	635914	79.09%	9.682%
18	11.609	3276	3287	3308	rBV	351163	558153	69.42%	8.498%
19	15.368	4447	4456	4467	rBV	5807	9733	1.21%	0.148%
20	15.757	4571	4577	4587	rVB4	11853	17295	2.15%	0.263%
21	15.940	4626	4634	4641	rBV9	6475	11824	1.47%	0.180%


Sum of corrected areas: 6567902

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030005.D
Acq On : 31 Jan 2023 11:05
Operator : SY/MD
Sample : VV0131WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

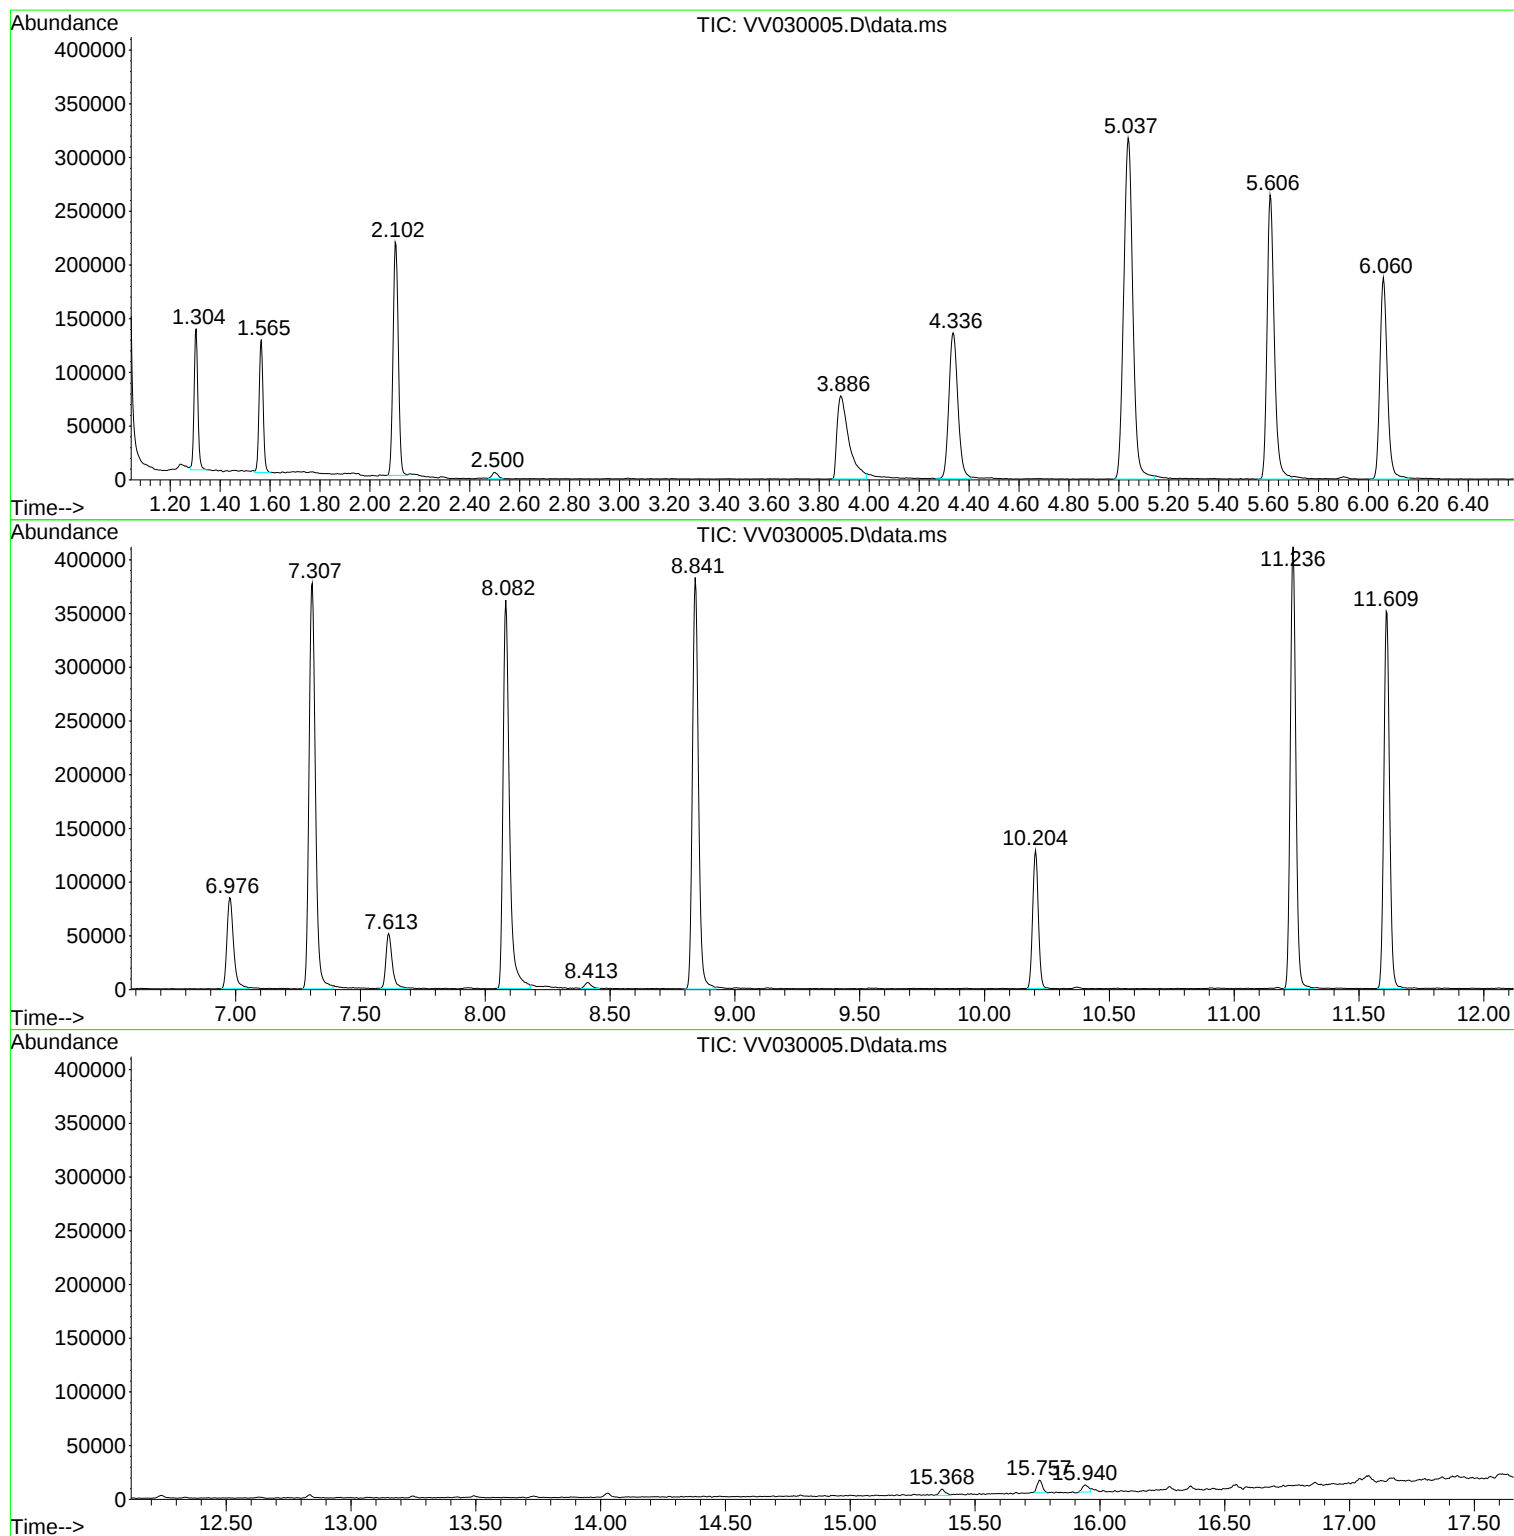

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030005.D
Acq On : 31 Jan 2023 11:05
Operator : SY/MD
Sample : VV0131WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030005.D
Acq On : 31 Jan 2023 11:05
Operator : SY/MD
Sample : VV0131WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc