

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
 Data File : VV030006.D
 Acq On : 31 Jan 2023 11:32
 Operator : SY/MD
 Sample : 01315-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B42

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	14	20	38	rVB	252296	250002	3.24%	1.461%
2	1.301	72	81	93	rBV2	211581	288280	3.73%	1.684%
3	1.564	154	163	174	rVB	125963	146780	1.90%	0.858%
4	2.101	319	330	343	rBV2	219980	323045	4.18%	1.887%
5	3.896	871	888	927	rBV2	213778	656275	8.50%	3.834%
6	4.333	1006	1024	1052	rBV	138646	358882	4.65%	2.097%
7	5.037	1225	1243	1276	rBV2	327172	865094	11.20%	5.055%
8	5.606	1407	1420	1447	rBV	278278	583174	7.55%	3.407%
9	5.902	1494	1512	1546	rBV	419176	835788	10.82%	4.883%
10	6.056	1547	1560	1585	rVV	190472	399826	5.18%	2.336%
11	6.976	1835	1846	1870	rBV	84572	159250	2.06%	0.930%
12	7.304	1936	1948	1960	rBV	388223	671478	8.69%	3.923%
13	7.378	1960	1971	1994	rVB	537996	932276	12.07%	5.447%
14	7.612	2032	2044	2068	rVB	52108	95142	1.23%	0.556%
15	7.963	2133	2153	2179	rBV	4665325	7723967	100.00%	45.129%
16	8.082	2180	2190	2222	rVB	377470	673945	8.73%	3.938%
17	8.841	2413	2426	2450	rBV	420295	687781	8.90%	4.019%
18	10.204	2839	2850	2863	rBV	128509	203987	2.64%	1.192%
19	11.236	3160	3171	3188	rVB	448387	688953	8.92%	4.025%
20	11.609	3276	3287	3305	rVB	360749	571279	7.40%	3.338%




Sum of corrected areas: 17115204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030006.D
Acq On : 31 Jan 2023 11:32
Operator : SY/MD
Sample : 01315-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

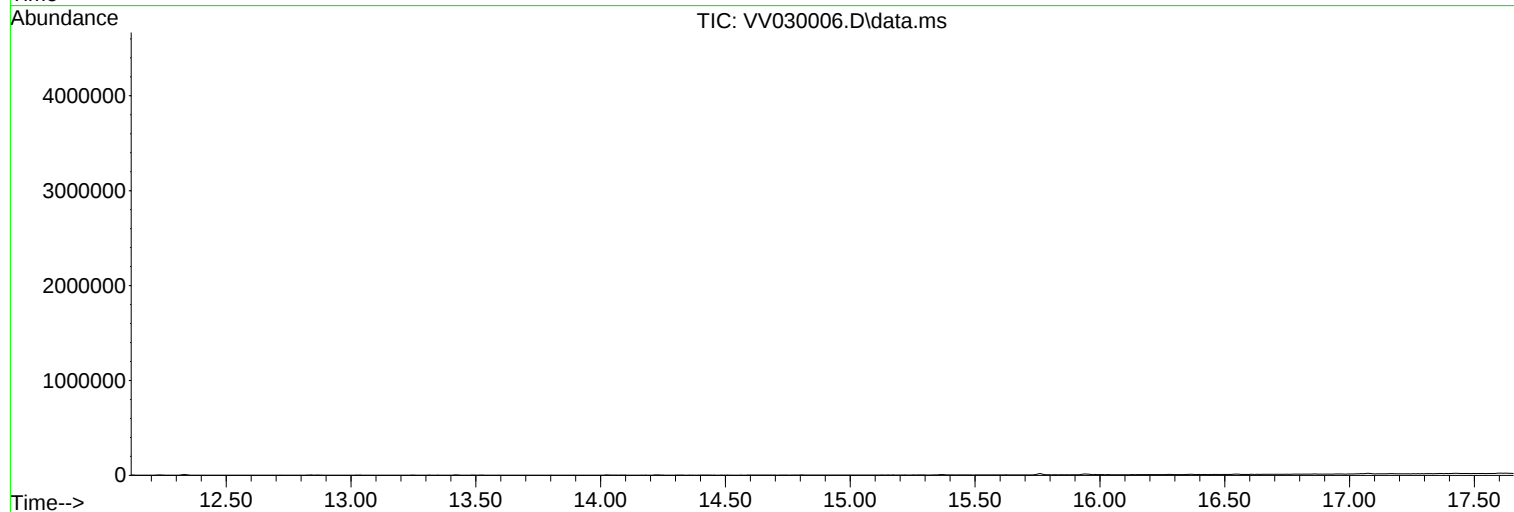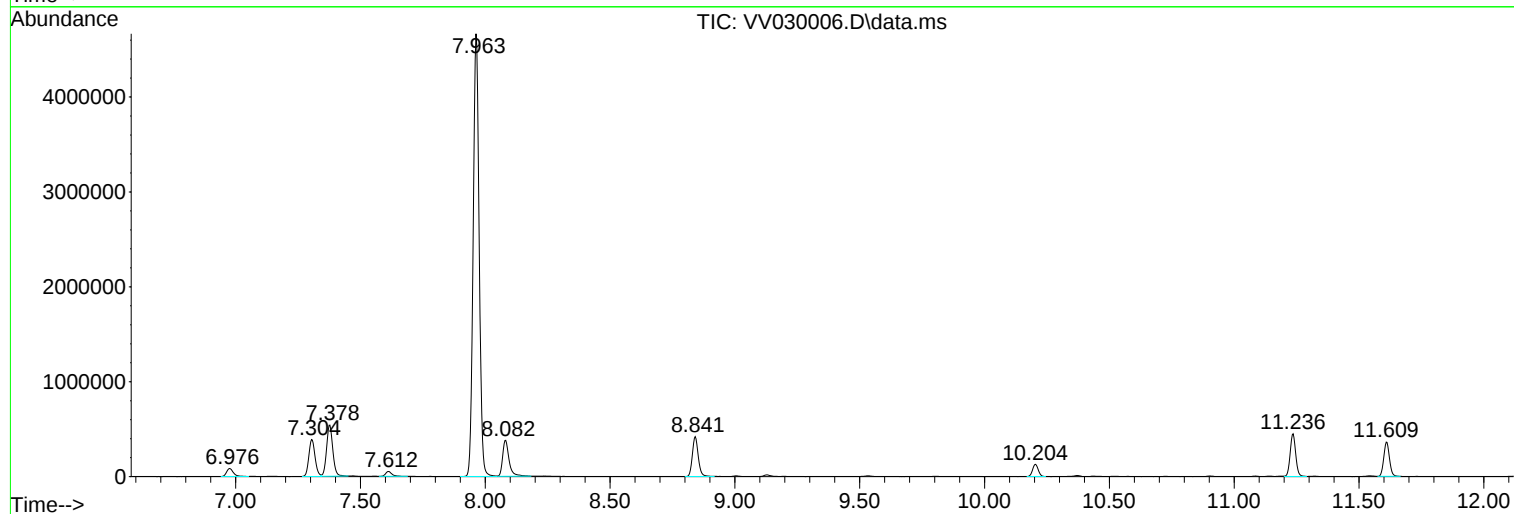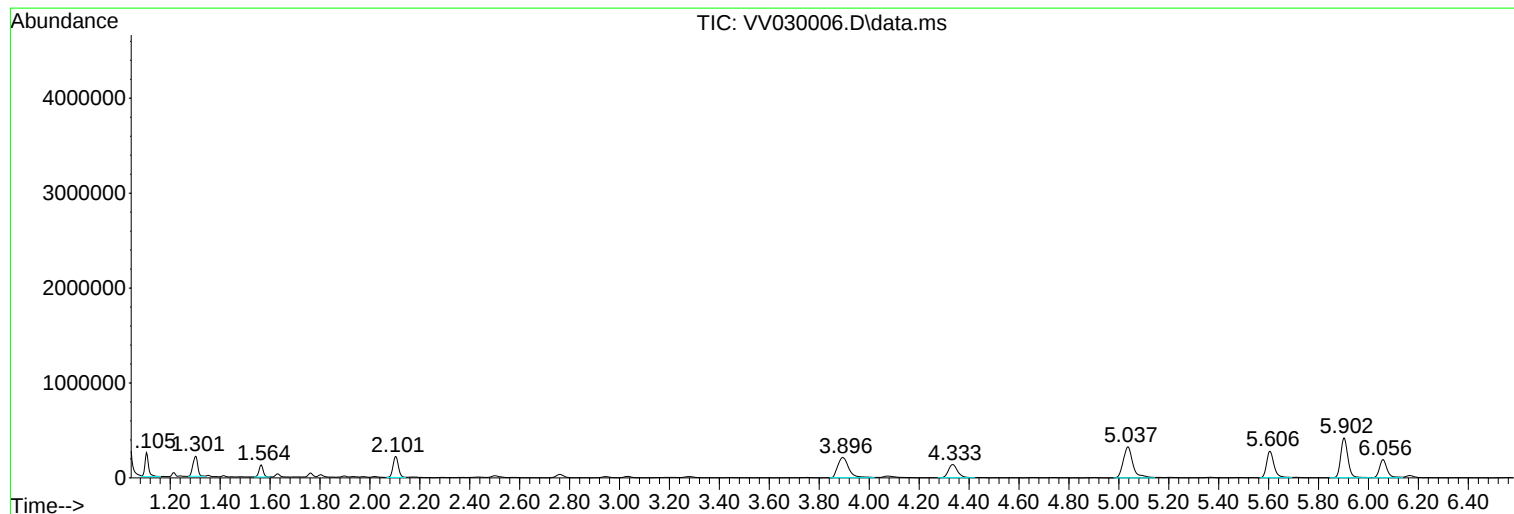

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030006.D
Acq On : 31 Jan 2023 11:32
Operator : SY/MD
Sample : 01315-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B42










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.105	2.14 ug/L	250002	1,4-Difluorobenzene	5.606

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	90
2			Propene	42	C3H6	000115-07-1	56
3			Cyclopropane	42	C3H6	000075-19-4	10
4			Cyclopropane	42	C3H6	000075-19-4	8
5			Cyclopropane	42	C3H6	000075-19-4	4

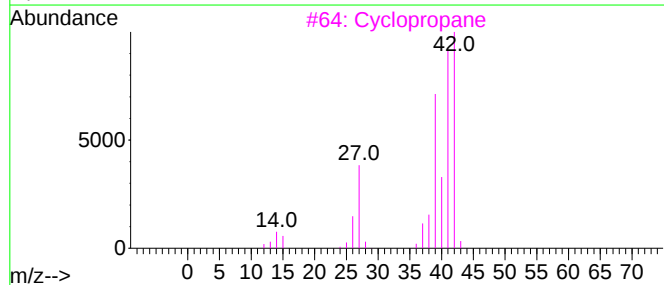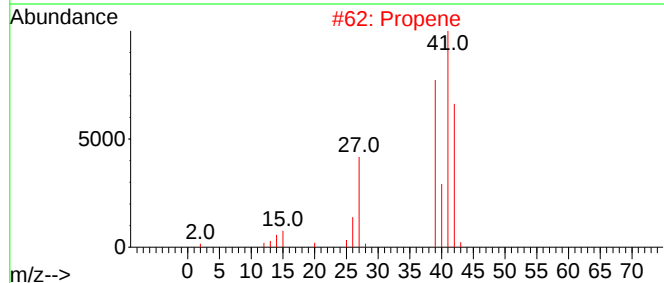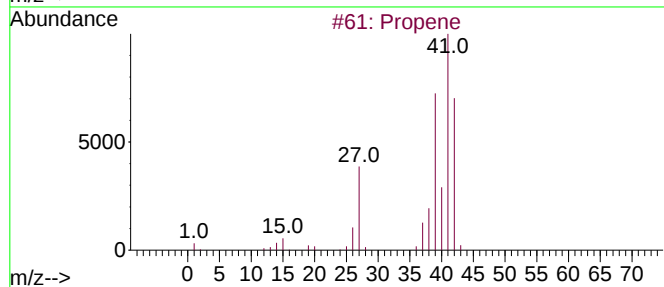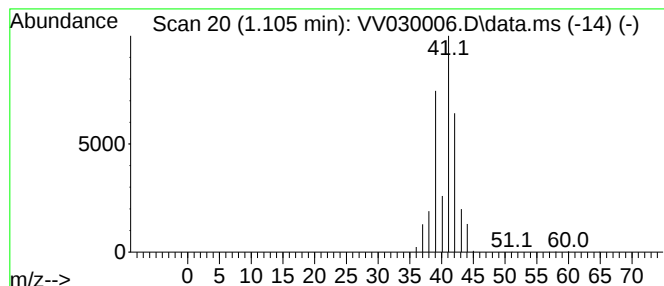

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030006.D
Acq On : 31 Jan 2023 11:32
Operator : SY/MD
Sample : 01315-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.105	2.1	ug/L	250002	1	5.606	583174	5.0