

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
 Data File : VV030011.D
 Acq On : 31 Jan 2023 15:51
 Operator : SY/MD
 Sample : 01315-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	102	rVB	130841	144789	18.75%	2.257%
2	1.565	155	163	177	rVB	119042	134445	17.41%	2.096%
3	2.105	320	331	344	rBV	204580	294417	38.12%	4.589%
4	2.500	444	454	466	rBV	23737	38291	4.96%	0.597%
5	3.886	872	885	933	rBV	75991	255039	33.02%	3.975%
6	4.336	1008	1025	1055	rBV	131307	331493	42.92%	5.167%
7	5.037	1226	1243	1271	rBV2	311601	772383	100.00%	12.040%
8	5.606	1404	1420	1444	rBV	255111	519189	67.22%	8.093%
9	6.060	1546	1561	1583	rBV	184465	374458	48.48%	5.837%
10	6.979	1830	1847	1871	rBV	79879	152198	19.70%	2.372%
11	7.307	1936	1949	1970	rBV	362262	636098	82.36%	9.915%
12	7.613	2034	2044	2063	rBV	47295	86451	11.19%	1.348%
13	8.082	2175	2190	2230	rBV	358255	645386	83.56%	10.060%
14	8.841	2413	2426	2448	rBV	379902	628430	81.36%	9.796%
15	10.204	2839	2850	2866	rBV	126548	198549	25.71%	3.095%
16	10.371	2890	2902	2910	rBV2	5157	8023	1.04%	0.125%
17	11.236	3158	3171	3189	rBV	399523	624292	80.83%	9.731%
18	11.609	3275	3287	3308	rBV	344898	545498	70.63%	8.503%
19	14.027	4027	4039	4048	rBV	5088	9465	1.23%	0.148%
20	15.760	4570	4578	4584	rBV5	11525	16410	2.12%	0.256%


Sum of corrected areas: 6415304

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030011.D
Acq On : 31 Jan 2023 15:51
Operator : SY/MD
Sample : 01315-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

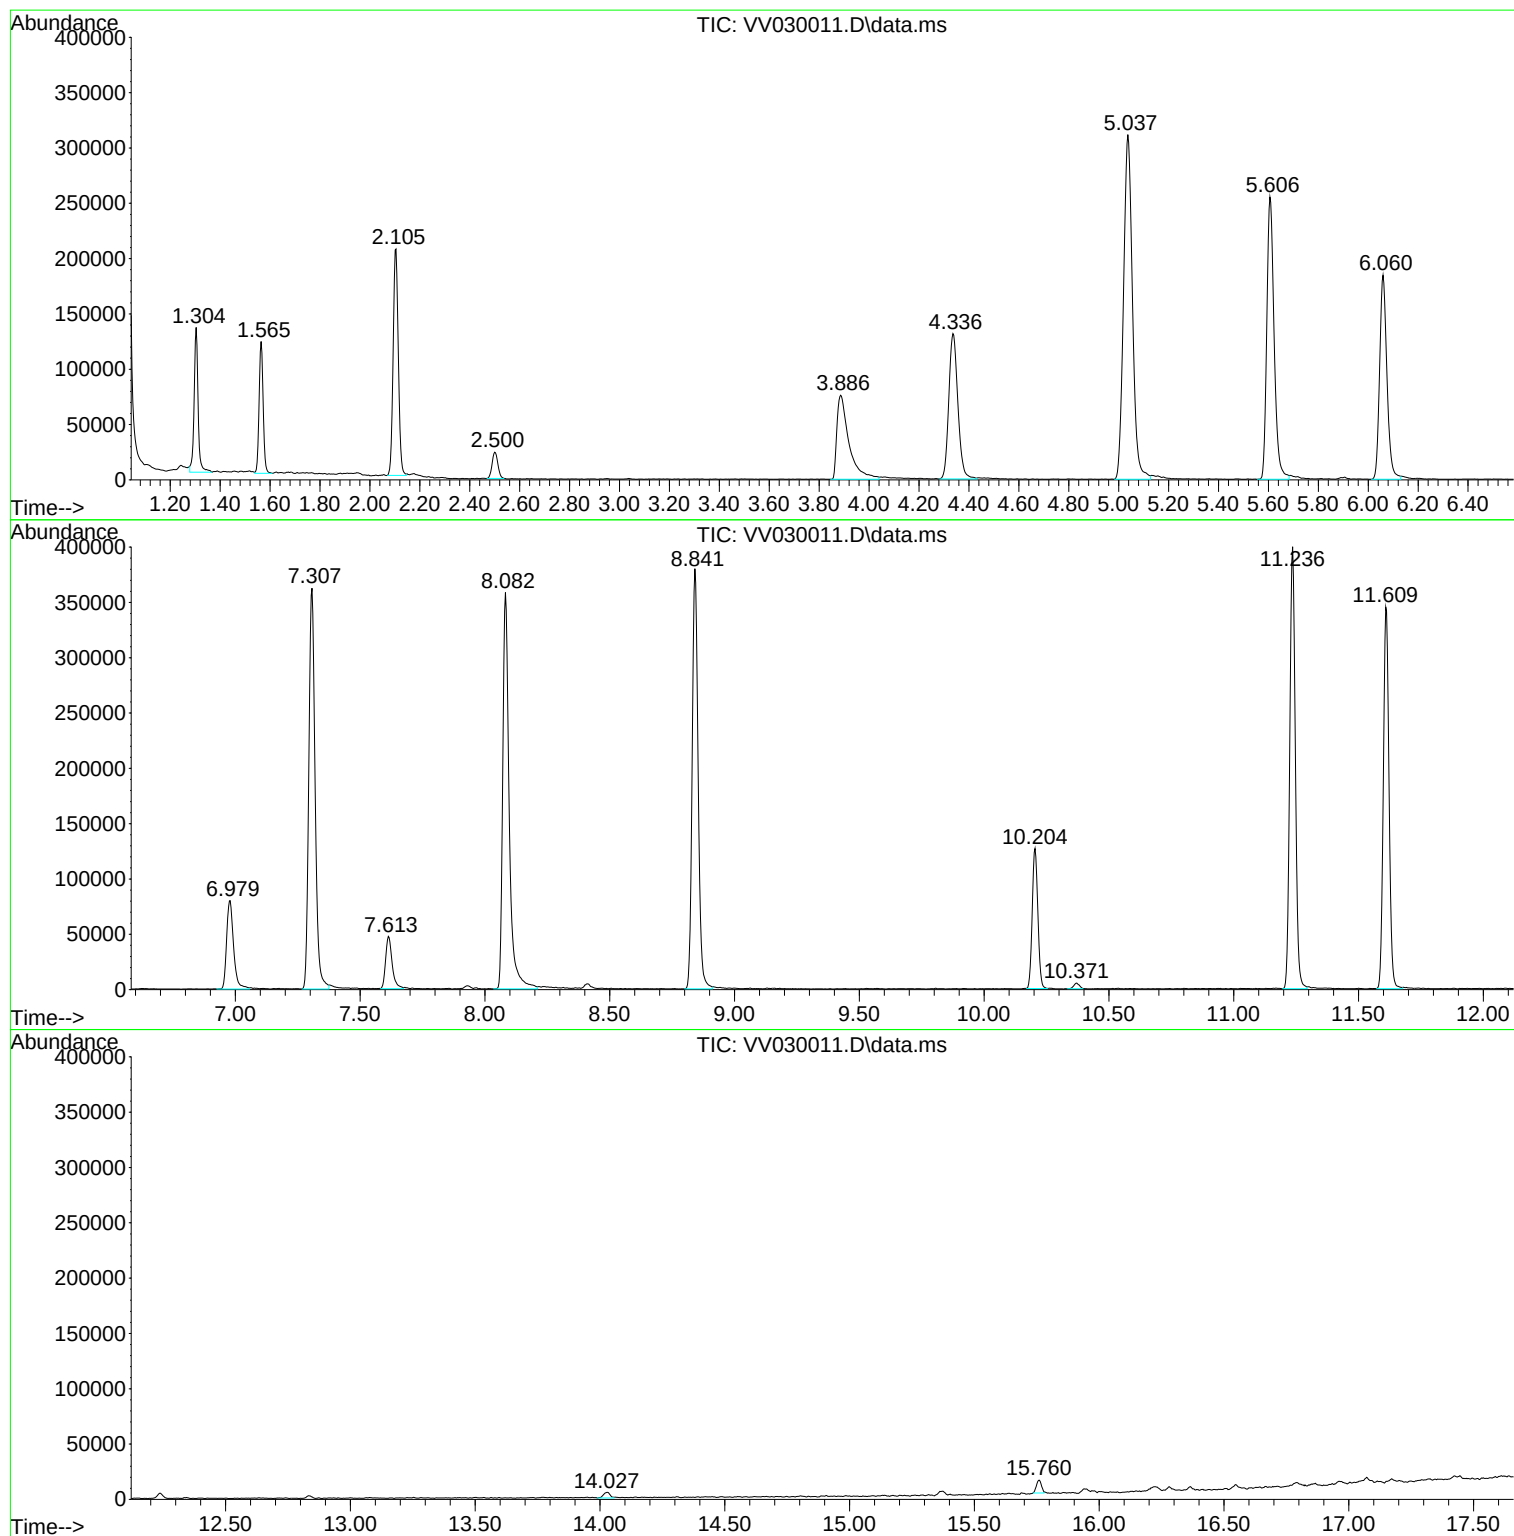

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030011.D
Acq On : 31 Jan 2023 15:51
Operator : SY/MD
Sample : 01315-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030011.D
Acq On : 31 Jan 2023 15:51
Operator : SY/MD
Sample : 01315-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc