
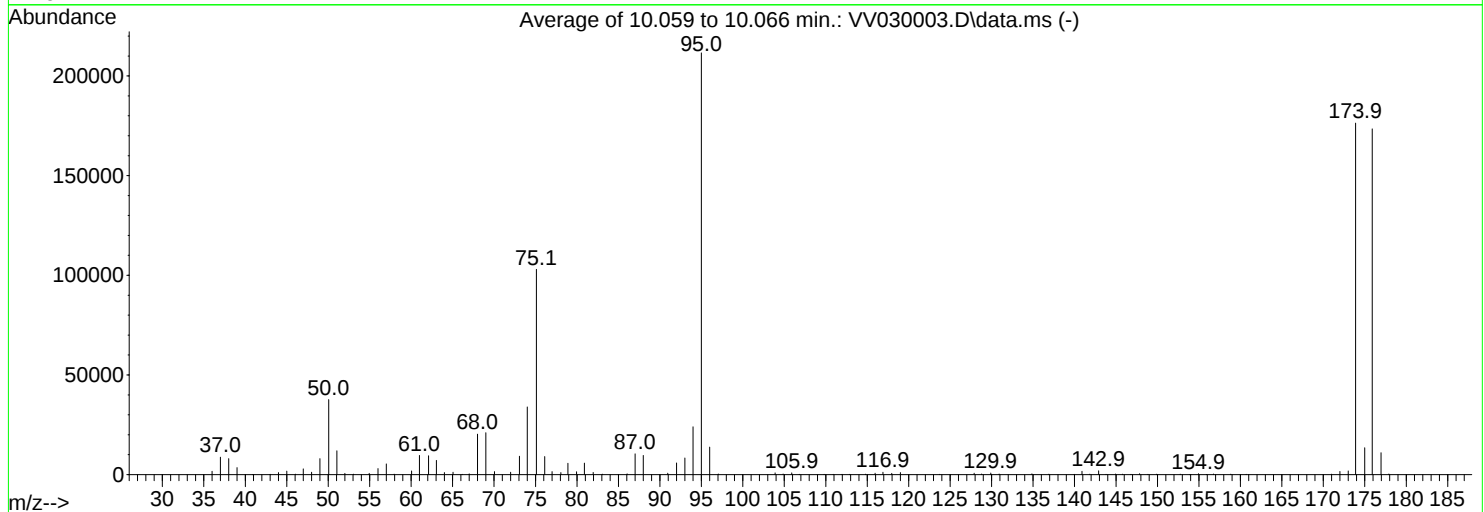


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013123\
Data File : VV030003.D
Acq On : 31 Jan 2023 09:45
Operator : SY/MD
Sample : BFB219
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB219

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Feb 01 00:13:14 2023

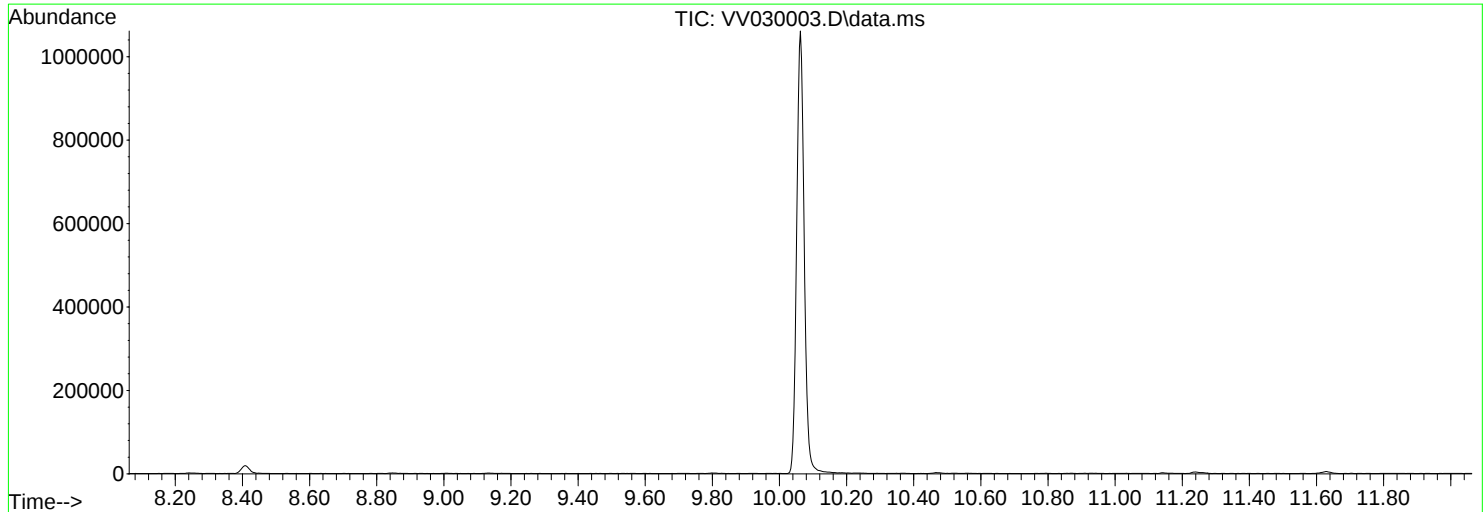

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	37677	PASS
75	95	30	80	48.7	102949	PASS
95	95	100	100	100.0	211584	PASS
96	95	5	9	6.5	13801	PASS
173	174	0.00	2	1.1	1878	PASS
174	95	50	120	83.4	176363	PASS
175	174	5	9	7.6	13490	PASS
176	174	95	105	98.3	173440	PASS
177	176	5	10	6.3	11012	PASS

m/z	Abundance
40.00	379.0
44.00	454.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
36.00	1643.0
37.00	8802.0
38.00	8284.0
39.00	3840.0
40.00	442.0
40.90	112.0
43.00	187.0
44.00	1489.0
45.00	1809.0
46.00	258.0
47.00	2992.0
48.00	1248.0
49.00	8192.0
50.10	37912.0
51.10	12044.0
52.00	646.0
53.10	218.0
54.90	601.0
56.00	3017.0
57.00	5531.0
58.00	270.0
60.00	2010.0
61.00	9803.0
62.10	9776.0
63.10	7414.0
64.00	1051.0
65.00	1242.0
66.20	157.0
67.00	443.0
68.00	20544.0
69.00	21056.0
70.10	1593.0
72.00	1240.0
73.00	9482.0
74.00	34368.0
75.10	102736.0
76.10	9175.0
77.00	1431.0
78.00	973.0
78.90	5721.0
80.00	1552.0
80.90	6078.0
81.90	1178.0
83.10	208.0
86.00	390.0
87.00	10530.0
88.00	9816.0
90.90	778.0
92.00	5889.0
93.00	8521.0
94.00	24504.0
95.00	211136.0
96.00	14172.0
97.10	354.0
103.90	897.0
104.80	348.0
105.90	838.0
106.80	167.0
109.80	177.0
110.90	169.0
111.90	185.0
112.90	154.0
114.80	214.0
116.00	760.0
116.90	1282.0
117.90	733.0
119.00	1037.0
123.80	124.0
127.90	677.0
128.80	311.0
129.90	803.0
130.90	281.0
134.80	376.0
136.90	304.0
139.90	126.0
140.90	1656.0
141.90	189.0
142.90	2081.0
143.80	138.0
144.90	371.0
145.80	227.0
146.80	120.0
147.80	563.0
148.90	163.0
149.90	190.0
152.70	188.0
154.90	424.0
156.80	361.0
158.80	242.0
160.70	196.0
171.00	225.0
172.00	1631.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

173.00	1799.0
173.90	172288.0
175.00	13231.0
175.90	169344.0
176.90	11156.0
177.90	352.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
36.00	1737.0
37.00	9093.0
38.00	8317.0
39.00	3680.0
40.00	430.0
43.00	215.0
44.00	1563.0
45.00	1877.0
46.00	272.0
47.00	2909.0
48.00	1257.0
49.00	8343.0
50.10	39016.0
51.00	12369.0
52.00	656.0
53.10	238.0
55.00	671.0
56.00	3169.0
57.00	5613.0
57.90	273.0
60.10	1905.0
61.00	9966.0
62.10	9828.0
63.10	7274.0
64.00	1103.0
65.10	1251.0
66.20	169.0
67.00	442.0
68.00	21000.0
69.00	21864.0
70.00	1615.0
72.00	1196.0
73.00	9602.0
74.00	35224.0
75.10	106632.0
76.10	9428.0
77.00	1534.0
78.00	1034.0
78.90	5892.0
80.00	1484.0
80.90	5997.0
81.90	1192.0
83.10	221.0
86.00	366.0
87.00	10738.0
88.00	9953.0
90.90	781.0
92.00	6099.0
93.00	8597.0
94.00	24744.0
95.00	218880.0
96.00	14345.0
97.00	359.0
103.90	870.0
104.90	349.0
105.90	912.0
106.80	174.0
109.80	169.0
110.90	173.0
111.90	187.0
112.90	153.0
114.80	231.0
115.90	705.0
116.90	1205.0
117.90	704.0
119.00	1130.0
123.70	154.0
127.90	712.0
128.80	306.0
129.90	807.0
130.90	315.0
134.90	387.0
136.90	295.0
139.90	139.0
140.90	1754.0
141.80	228.0
142.90	2034.0
143.80	159.0
145.00	379.0
145.80	267.0
146.80	134.0
147.90	510.0
148.80	151.0
149.90	242.0
152.80	213.0
155.00	508.0
155.90	101.0
156.70	391.0
158.90	228.0
160.70	163.0
171.00	243.0
172.00	1655.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

173.00	1933.0
173.90	182336.0
175.00	13944.0
175.90	179904.0
177.00	11287.0
177.90	345.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
36.00	1589.0
37.00	8263.0
38.00	7495.0
39.00	3158.0
40.00	408.0
43.00	219.0
44.00	1517.0
45.00	1678.0
46.10	249.0
47.00	2750.0
48.00	1195.0
49.00	7591.0
50.00	36104.0
51.00	11454.0
52.00	601.0
53.00	228.0
55.00	636.0
56.00	2981.0
57.00	5054.0
57.90	262.0
60.00	1593.0
61.00	9097.0
62.10	8874.0
63.00	6731.0
64.00	1009.0
65.10	1189.0
66.10	162.0
67.00	428.0
68.00	19448.0
69.00	20144.0
70.00	1489.0
72.00	1118.0
73.10	8627.0
74.00	32384.0
75.10	99480.0
76.10	8558.0
77.00	1546.0
78.10	1048.0
78.90	5425.0
79.90	1394.0
80.90	5380.0
82.00	1084.0
83.00	204.0
86.10	352.0
87.00	9964.0
88.00	9201.0
91.00	702.0
92.00	5543.0
93.00	7955.0
94.00	22752.0
95.00	204736.0
96.00	12886.0
97.00	342.0
103.90	800.0
104.90	320.0
105.90	831.0
106.80	165.0
109.80	136.0
110.90	153.0
112.00	146.0
112.90	152.0
114.80	213.0
115.90	619.0
116.90	1108.0
118.00	612.0
119.00	1048.0
123.80	144.0
127.90	684.0
128.80	282.0
129.90	732.0
130.90	309.0
134.90	378.0
136.90	254.0
140.00	121.0
140.90	1702.0
141.90	245.0
142.90	1794.0
143.80	161.0
144.90	343.0
145.80	331.0
146.80	141.0
147.90	442.0
148.80	151.0
149.90	252.0
152.80	237.0
153.90	130.0
154.90	555.0
155.90	100.0
156.80	307.0
158.90	219.0
160.70	147.0
161.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

171.00	244.0
172.00	1559.0
173.00	1901.0
173.90	174464.0
175.00	13294.0
175.90	171072.0
177.00	10594.0
177.90	294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219