

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033924.D
 Acq On : 31 Jan 2024 16:40
 Operator : SY/MD
 Sample : P1309-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH903

Quant Time: Feb 01 05:31:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 01 04:45:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	218308	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	203480	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	100417	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	62124	37.027	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.060%
7) Chloroethane-d5	1.529	69	52133	39.236	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.480%
11) 1,1-Dichloroethene-d2	2.060	65	29417	40.740	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.480%
21) 2-Butanone-d5	3.783	46	82939	72.070	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	72.070%
24) Chloroform-d	4.249	84	118233	39.410	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.820%
26) 1,2-Dichloroethane-d4	4.941	65	82132	42.370	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.740%
32) Benzene-d6	4.960	84	230129	39.782	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.560%
36) 1,2-Dichloropropane-d6	5.989	67	71399	37.496	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	75.000%
41) Toluene-d8	7.243	98	209499	40.194	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.380%
43) trans-1,3-Dichloroprop...	7.555	79	36897	39.207	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.420%
47) 2-Hexanone-d5	8.021	63	59316	75.098	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.100%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	96871	39.850	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.700%
66) 1,2-Dichlorobenzene-d4	11.561	152	81556	42.807	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.620%
Target Compounds						
					Qvalue	
13) Acetone	2.111	43	6361	5.781	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033924.D
Acq On : 31 Jan 2024 16:40
Operator : SY/MD
Sample : P1309-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH903

Quant Time: Feb 01 05:31:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 01 04:45:22 2024
Response via : Initial Calibration

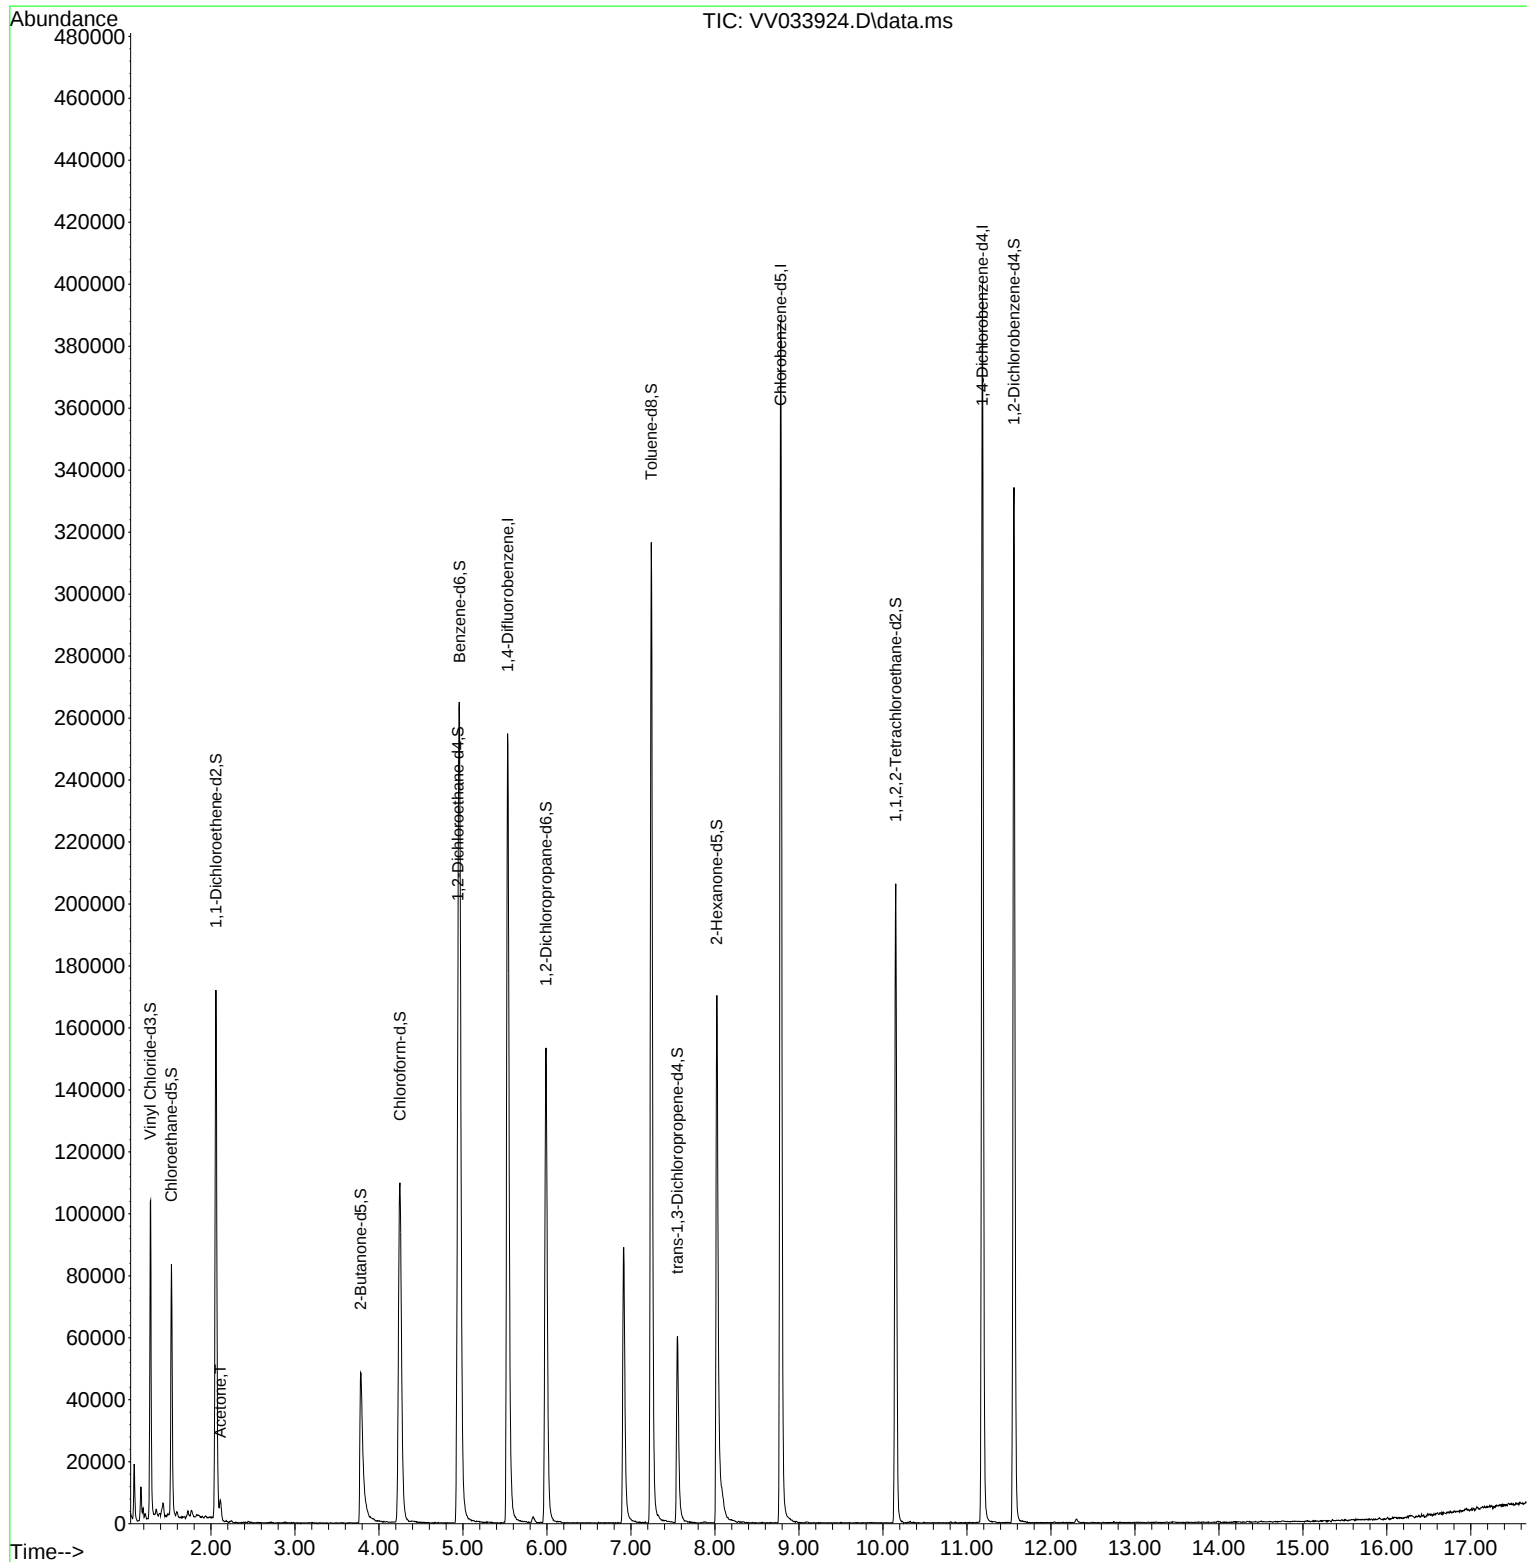

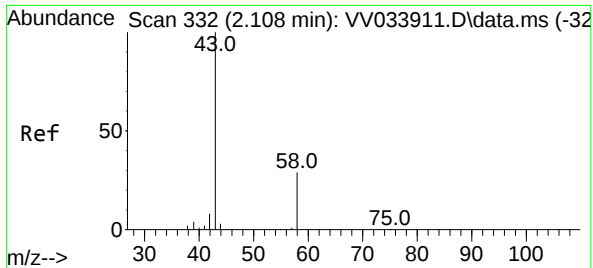

#13

Acetone

Concen: 5.781 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV033924.D

Acq: 31 Jan 2024 16:40

Instrument :

MSVOA_V

ClientSampleId :

BH903

Tgt Ion: 43 Resp: 6361

Ion Ratio Lower Upper

43 100

58 23.8 0.0 57.2

