

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033912.D
 Acq On : 31 Jan 2024 09:48
 Operator : SY/MD
 Sample : VV0131WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK226

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	36	41	50	rBV2	3316	5774	0.76%	0.094%
2	1.278	68	74	91	rVB	104815	116927	15.45%	1.903%
3	1.526	144	151	169	rVB	91470	110953	14.66%	1.806%
4	2.056	306	316	335	rVB	195239	281560	37.20%	4.583%
5	2.182	350	355	364	rVB4	657	882	0.12%	0.014%
6	2.243	367	374	379	rBV2	860	1153	0.15%	0.019%
7	2.333	397	402	406	rBV	286	311	0.04%	0.005%
8	2.355	406	409	412	rVB3	337	235	0.03%	0.004%
9	2.397	420	422	427	rVB	252	236	0.03%	0.004%
10	2.442	432	436	437	rBV2	504	317	0.04%	0.005%
11	2.632	492	495	500	rVB2	238	229	0.03%	0.004%
12	2.767	532	537	539	rBV2	207	197	0.03%	0.003%
13	2.825	551	555	559	rVV	179	191	0.03%	0.003%
14	2.844	559	561	567	rVV2	182	201	0.03%	0.003%
15	2.934	583	589	594	rVV2	243	293	0.04%	0.005%
16	2.973	594	601	607	rVB	245	343	0.05%	0.006%
17	3.066	624	630	634	rVB2	213	198	0.03%	0.003%
18	3.214	668	676	677	rBV	147	226	0.03%	0.004%
19	3.317	703	708	711	rBV2	296	397	0.05%	0.006%
20	3.478	755	758	761	rVB2	271	201	0.03%	0.003%
21	3.523	767	772	774	rBV	289	284	0.04%	0.005%
22	3.564	782	785	788	rBV	289	273	0.04%	0.004%
23	3.645	805	810	814	rVB2	294	369	0.05%	0.006%
24	3.674	815	819	823	rBV2	288	353	0.05%	0.006%
25	3.783	845	853	892	rBV	50315	136033	17.97%	2.214%
26	4.146	963	966	970	rBV	237	264	0.03%	0.004%
27	4.246	981	997	1026	rBV	119023	304485	40.23%	4.956%
28	4.365	1032	1034	1040	rVB2	403	333	0.04%	0.005%
29	4.436	1054	1056	1059	rBV2	389	324	0.04%	0.005%
30	4.516	1078	1081	1082	rBV	348	198	0.03%	0.003%
31	4.526	1082	1084	1088	rVV3	304	226	0.03%	0.004%
32	4.603	1105	1108	1111	rBV2	263	211	0.03%	0.003%
33	4.664	1124	1127	1130	rBV	268	209	0.03%	0.003%
34	4.719	1139	1144	1146	rBV2	213	213	0.03%	0.003%
35	4.828	1174	1178	1182	rBV	181	205	0.03%	0.003%
36	4.876	1189	1193	1198	rBV	211	281	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033912.D
 Acq On : 31 Jan 2024 09:48
 Operator : SY/MD
 Sample : VV0131WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK226

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	4.953	1201	1217	1254	rBV2	285889	756862	100.00%	12.320%
38	5.108	1263	1265	1269	rVB2	520	292	0.04%	0.005%
39	5.416	1357	1361	1363	rBV2	384	208	0.03%	0.003%
40	5.481	1377	1381	1385	rVB	206	174	0.02%	0.003%
41	5.532	1385	1397	1429	rBV	260357	533454	70.48%	8.684%
42	5.831	1483	1490	1503	rBV4	2088	3934	0.52%	0.064%
43	5.892	1507	1509	1512	rBV	284	212	0.03%	0.003%
44	5.918	1512	1517	1518	rBV2	209	187	0.02%	0.003%
45	5.985	1525	1538	1565	rBV	161898	339348	44.84%	5.524%
46	6.153	1587	1590	1596	rVB4	642	708	0.09%	0.012%
47	6.310	1637	1639	1643	rVB2	285	176	0.02%	0.003%
48	6.477	1685	1691	1693	rBV	181	208	0.03%	0.003%
49	6.513	1699	1702	1707	rBB2	302	373	0.05%	0.006%
50	6.542	1707	1711	1715	rBV2	299	362	0.05%	0.006%
51	6.911	1816	1826	1855	rBV	97890	184416	24.37%	3.002%
52	7.239	1916	1928	1956	rBV	347126	610612	80.68%	9.940%
53	7.513	2007	2013	2015	rBV	391	450	0.06%	0.007%
54	7.551	2015	2025	2047	rVV	67950	120118	15.87%	1.955%
55	7.751	2084	2087	2090	rVB2	327	186	0.02%	0.003%
56	7.783	2091	2097	2102	rVB	318	429	0.06%	0.007%
57	8.021	2163	2171	2189	rBV	173449	317493	41.95%	5.168%
58	8.419	2291	2295	2298	rBV	220	202	0.03%	0.003%
59	8.464	2306	2309	2313	rVB2	294	224	0.03%	0.004%
60	8.783	2397	2408	2434	rBV	394423	643959	85.08%	10.482%
61	9.079	2494	2500	2501	rBV	385	344	0.05%	0.006%
62	9.249	2549	2553	2556	rBV	235	223	0.03%	0.004%
63	9.493	2622	2629	2633	rVV3	446	565	0.07%	0.009%
64	9.876	2743	2748	2753	rBV2	545	542	0.07%	0.009%
65	9.947	2764	2770	2772	rBV	157	174	0.02%	0.003%
66	10.153	2823	2834	2856	rBV	215231	337695	44.62%	5.497%
67	10.365	2896	2900	2902	rBV	199	180	0.02%	0.003%
68	10.439	2919	2923	2928	rBV2	168	210	0.03%	0.003%
69	10.484	2930	2937	2943	rBV3	875	1395	0.18%	0.023%
70	10.725	3007	3012	3020	rBV2	218	347	0.05%	0.006%
71	10.860	3047	3054	3056	rBV2	793	837	0.11%	0.014%
72	10.921	3068	3073	3076	rBV2	193	222	0.03%	0.004%
73	11.046	3108	3112	3114	rBV	257	219	0.03%	0.004%
74	11.127	3132	3137	3144	rVB3	1548	2027	0.27%	0.033%
75	11.185	3144	3155	3180	rBV	416491	658200	86.96%	10.714%
76	11.503	3251	3254	3260	rBV	233	269	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033912.D
 Acq On : 31 Jan 2024 09:48
 Operator : SY/MD
 Sample : VV0131WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK226

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.561	3260	3272	3295	rBV	360211	574814	75.95%	9.357%
78	11.693	3312	3313	3320	rVB2	354	205	0.03%	0.003%
79	12.246	3482	3485	3490	rVB2	190	208	0.03%	0.003%
80	12.371	3521	3524	3527	rBV	337	214	0.03%	0.003%
81	12.496	3560	3563	3567	rBV2	164	199	0.03%	0.003%
82	12.558	3579	3582	3585	rVB	294	202	0.03%	0.003%
83	12.590	3585	3592	3601	rBV4	2792	4208	0.56%	0.068%
84	12.664	3610	3615	3618	rBV2	167	193	0.03%	0.003%
85	13.120	3755	3757	3762	rVB2	169	173	0.02%	0.003%
86	13.149	3762	3766	3769	rBV2	214	213	0.03%	0.003%
87	13.204	3775	3783	3796	rVB3	7117	10288	1.36%	0.167%
88	13.300	3810	3813	3816	rBV2	257	185	0.02%	0.003%
89	13.355	3821	3830	3831	rBV2	210	295	0.04%	0.005%
90	13.442	3846	3857	3872	rBV	30926	51251	6.77%	0.834%
91	13.683	3923	3932	3941	rBV3	9385	14441	1.91%	0.235%
92	13.763	3950	3957	3964	rBV2	236	450	0.06%	0.007%
93	13.963	4016	4019	4023	rBV3	371	377	0.05%	0.006%
94	14.030	4036	4040	4044	rBV2	348	366	0.05%	0.006%
95	14.242	4104	4106	4108	rBV	256	184	0.02%	0.003%
96	14.451	4168	4171	4173	rBV	292	211	0.03%	0.003%
97	14.619	4221	4223	4229	rVB2	388	269	0.04%	0.004%
98	14.885	4303	4306	4311	rBV2	244	253	0.03%	0.004%
99	15.525	4503	4505	4507	rBV	357	186	0.02%	0.003%
100	16.168	4703	4705	4709	rBV4	890	754	0.10%	0.012%




Sum of corrected areas: 6143260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033912.D
Acq On : 31 Jan 2024 09:48
Operator : SY/MD
Sample : VV0131WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK226

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

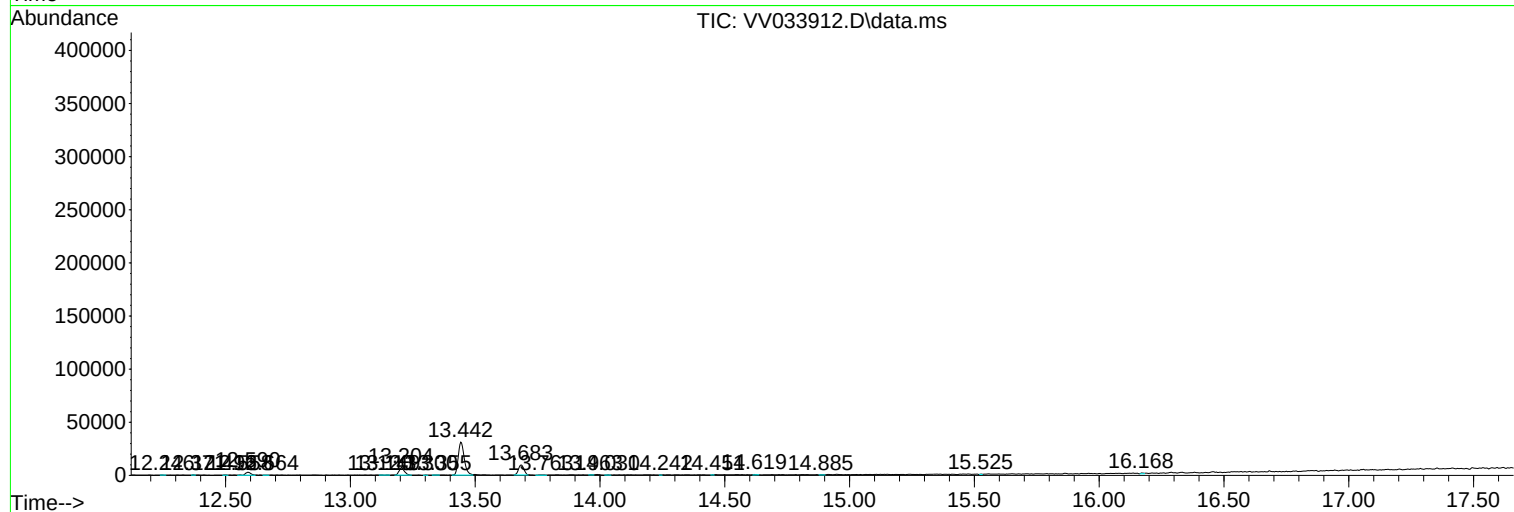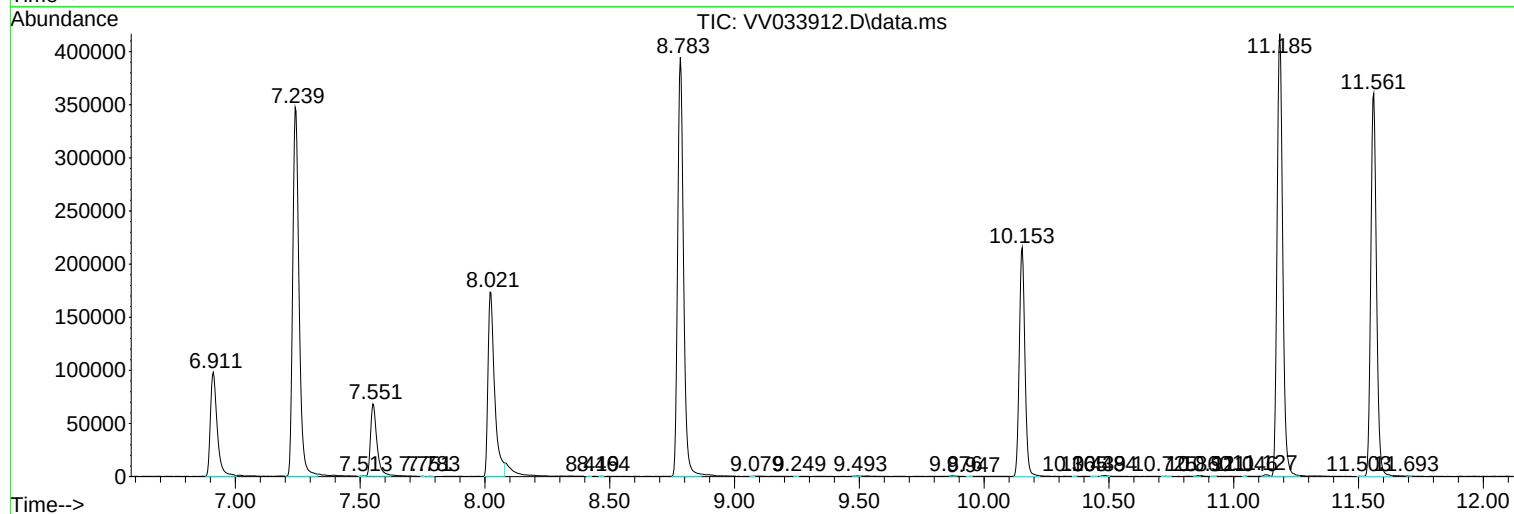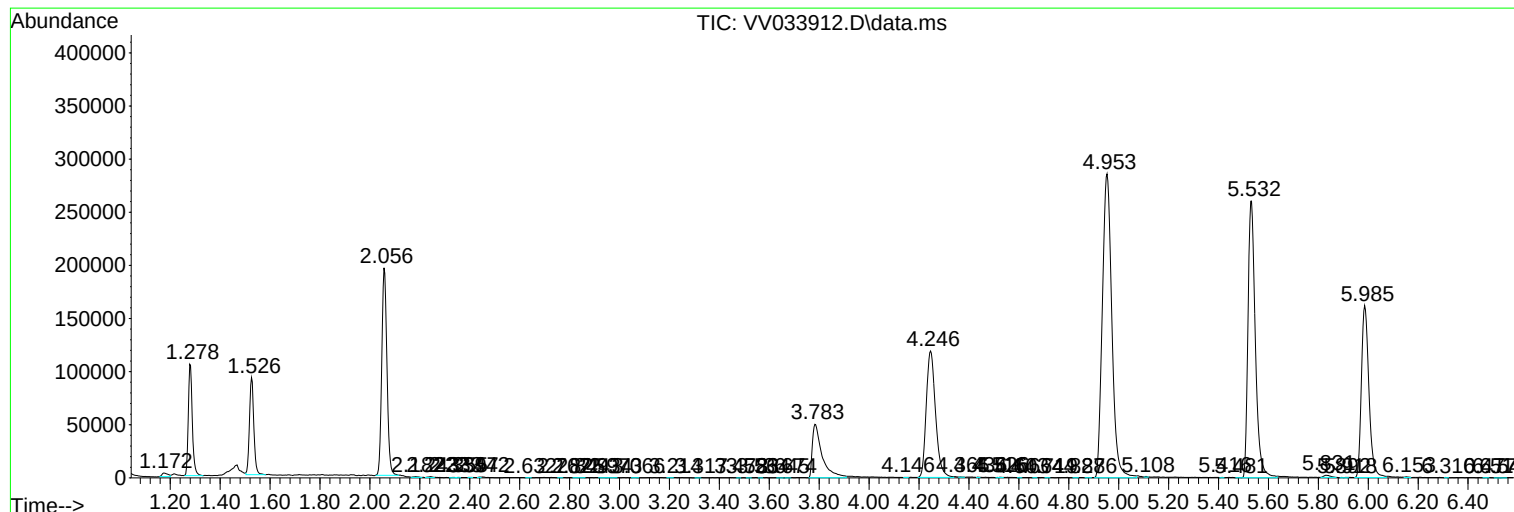

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033912.D
Acq On : 31 Jan 2024 09:48
Operator : SY/MD
Sample : VV0131WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK226

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033912.D
Acq On : 31 Jan 2024 09:48
Operator : SY/MD
Sample : VV0131WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK226

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------