

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033913.D
 Acq On : 31 Jan 2024 10:12
 Operator : SY/MD
 Sample : VV0131MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	33	40	51	rBV	15289	18976	2.48%	0.308%
2	1.282	68	75	87	rBV	112211	116255	15.17%	1.888%
3	1.529	145	152	171	rVB	88762	110350	14.40%	1.792%
4	2.060	307	317	342	rVB	190918	283238	36.95%	4.600%
5	2.233	368	371	372	rBV2	269	169	0.02%	0.003%
6	2.404	422	424	427	rBV	324	223	0.03%	0.004%
7	2.452	433	439	450	rVB4	803	1303	0.17%	0.021%
8	2.532	457	464	469	rBV2	218	362	0.05%	0.006%
9	2.597	481	484	488	rVB2	164	141	0.02%	0.002%
10	2.619	488	491	495	rBV	176	204	0.03%	0.003%
11	2.703	511	517	519	rBV	186	224	0.03%	0.004%
12	3.089	634	637	641	rBV2	166	167	0.02%	0.003%
13	3.108	641	643	646	rVB	167	133	0.02%	0.002%
14	3.195	667	670	672	rBV2	203	149	0.02%	0.002%
15	3.433	741	744	747	rBV2	273	227	0.03%	0.004%
16	3.452	748	750	755	rVV2	189	195	0.03%	0.003%
17	3.568	783	786	790	rBV	134	139	0.02%	0.002%
18	3.590	790	793	797	rVB2	212	188	0.02%	0.003%
19	3.635	804	807	810	rBV	185	175	0.02%	0.003%
20	3.783	845	853	887	rBV	53699	141368	18.44%	2.296%
21	3.970	909	911	914	rBV3	380	255	0.03%	0.004%
22	4.249	982	998	1030	rBV	120586	306372	39.97%	4.976%
23	4.584	1100	1102	1106	rBV2	213	160	0.02%	0.003%
24	4.680	1127	1132	1137	rBV2	358	415	0.05%	0.007%
25	4.841	1180	1182	1185	rBV	236	145	0.02%	0.002%
26	4.957	1202	1218	1252	rBV2	287572	766540	100.00%	12.450%
27	5.114	1265	1267	1270	rVB2	645	293	0.04%	0.005%
28	5.249	1305	1309	1310	rBV	225	187	0.02%	0.003%
29	5.532	1386	1397	1431	rBV	262035	536061	69.93%	8.707%
30	5.770	1467	1471	1474	rBV3	226	222	0.03%	0.004%
31	5.825	1483	1488	1490	rBV2	1732	1627	0.21%	0.026%
32	5.989	1523	1539	1568	rBV	167965	346566	45.21%	5.629%
33	6.146	1585	1588	1589	rBV2	304	207	0.03%	0.003%
34	6.211	1605	1608	1612	rBV2	177	160	0.02%	0.003%
35	6.500	1695	1698	1703	rVV2	198	219	0.03%	0.004%
36	6.651	1741	1745	1750	rBV2	123	169	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033913.D
 Acq On : 31 Jan 2024 10:12
 Operator : SY/MD
 Sample : VV0131MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.802	1788	1792	1797	rBV2	195	282	0.04%	0.005%
38	6.873	1811	1814	1816	rBV	150	125	0.02%	0.002%
39	6.912	1816	1826	1854	rBV	97137	182679	23.83%	2.967%
40	7.143	1894	1898	1899	rBV	203	160	0.02%	0.003%
41	7.172	1904	1907	1910	rVV	137	131	0.02%	0.002%
42	7.243	1918	1929	1958	rBV	348374	614717	80.19%	9.984%
43	7.555	2014	2026	2050	rBV	67160	121100	15.80%	1.967%
44	7.741	2081	2084	2087	rVB2	309	219	0.03%	0.004%
45	7.760	2087	2090	2095	rBV	294	190	0.02%	0.003%
46	8.024	2163	2172	2215	rBV	187175	363698	47.45%	5.907%
47	8.233	2235	2237	2241	rVB2	428	235	0.03%	0.004%
48	8.252	2241	2243	2247	rBV3	297	202	0.03%	0.003%
49	8.423	2293	2296	2299	rBV2	156	145	0.02%	0.002%
50	8.465	2305	2309	2312	rBV2	182	131	0.02%	0.002%
51	8.519	2324	2326	2330	rVB2	205	143	0.02%	0.002%
52	8.555	2335	2337	2341	rVB2	206	128	0.02%	0.002%
53	8.600	2346	2351	2353	rBV2	287	198	0.03%	0.003%
54	8.741	2389	2395	2397	rBV	236	244	0.03%	0.004%
55	8.783	2397	2408	2443	rBV	394192	650514	84.86%	10.566%
56	9.111	2506	2510	2513	rBV2	243	236	0.03%	0.004%
57	9.130	2513	2516	2518	rBV2	181	148	0.02%	0.002%
58	9.198	2534	2537	2540	rBV2	134	126	0.02%	0.002%
59	9.551	2644	2647	2650	rBV2	178	144	0.02%	0.002%
60	9.616	2662	2667	2669	rBV2	217	248	0.03%	0.004%
61	9.748	2704	2708	2712	rBV	195	190	0.02%	0.003%
62	9.776	2714	2717	2723	rBV	216	246	0.03%	0.004%
63	9.886	2748	2751	2754	rVB2	234	167	0.02%	0.003%
64	9.915	2754	2760	2765	rVB2	154	224	0.03%	0.004%
65	9.940	2765	2768	2771	rBV	166	138	0.02%	0.002%
66	10.040	2795	2799	2805	rBV2	186	243	0.03%	0.004%
67	10.069	2805	2808	2812	rBV2	163	160	0.02%	0.003%
68	10.153	2821	2834	2860	rBV	225314	352962	46.05%	5.733%
69	10.326	2885	2888	2891	rVB2	179	147	0.02%	0.002%
70	10.609	2973	2976	2981	rBV	120	138	0.02%	0.002%
71	10.738	3012	3016	3018	rBV	159	147	0.02%	0.002%
72	10.879	3058	3060	3062	rBV2	256	161	0.02%	0.003%
73	11.114	3127	3133	3135	rBV	189	215	0.03%	0.003%
74	11.185	3144	3155	3184	rVV	412253	644772	84.11%	10.473%
75	11.423	3226	3229	3233	rBV	333	216	0.03%	0.004%
76	11.561	3260	3272	3296	rBV	352215	567192	73.99%	9.212%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033913.D
 Acq On : 31 Jan 2024 10:12
 Operator : SY/MD
 Sample : VV0131MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.741	3326	3328	3336	rVV3	216	203	0.03%	0.003%
78	11.860	3361	3365	3368	rBV2	195	188	0.02%	0.003%
79	11.979	3399	3402	3407	rVB2	220	180	0.02%	0.003%
80	12.593	3591	3593	3596	rBV2	379	227	0.03%	0.004%
81	12.641	3603	3608	3610	rBV2	158	155	0.02%	0.003%
82	12.918	3691	3694	3699	rBV	218	168	0.02%	0.003%
83	12.940	3699	3701	3704	rBV2	210	125	0.02%	0.002%
84	13.062	3736	3739	3742	rBV2	142	142	0.02%	0.002%
85	13.098	3747	3750	3754	rVB	313	224	0.03%	0.004%
86	13.136	3754	3762	3764	rBV2	208	307	0.04%	0.005%
87	13.207	3778	3784	3792	rVB3	1326	1555	0.20%	0.025%
88	13.365	3828	3833	3835	rBV	224	230	0.03%	0.004%
89	13.448	3852	3859	3873	rVB	6113	10010	1.31%	0.163%
90	13.574	3895	3898	3903	rBV2	168	179	0.02%	0.003%
91	13.686	3926	3933	3943	rBV3	2066	2841	0.37%	0.046%
92	13.789	3962	3965	3968	rBV2	263	211	0.03%	0.003%
93	13.924	4004	4007	4009	rBV2	318	212	0.03%	0.003%
94	14.156	4075	4079	4083	rBV2	329	358	0.05%	0.006%
95	14.271	4112	4115	4122	rBV2	278	376	0.05%	0.006%
96	14.487	4180	4182	4186	rBV	281	213	0.03%	0.003%
97	15.014	4342	4346	4347	rBV2	351	263	0.03%	0.004%
98	15.124	4378	4380	4384	rBV2	344	223	0.03%	0.004%
99	15.271	4422	4426	4429	rBV2	506	502	0.07%	0.008%
100	15.950	4633	4637	4640	rBV4	520	440	0.06%	0.007%




Sum of corrected areas: 6156777

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033913.D
Acq On : 31 Jan 2024 10:12
Operator : SY/MD
Sample : VV0131MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

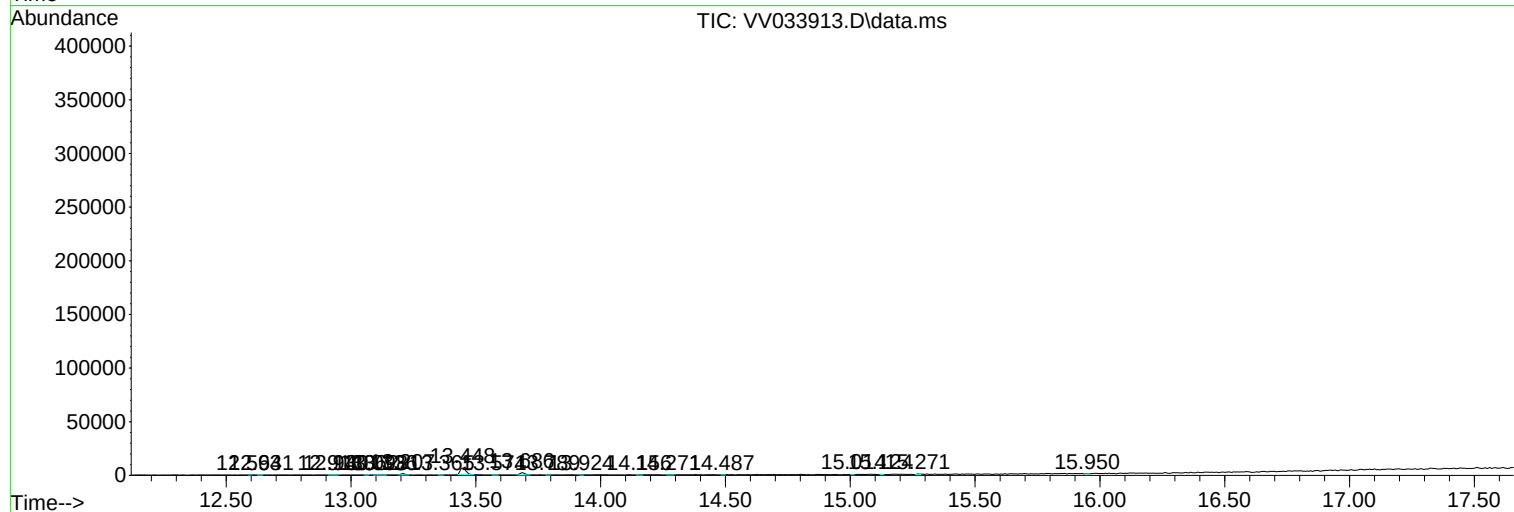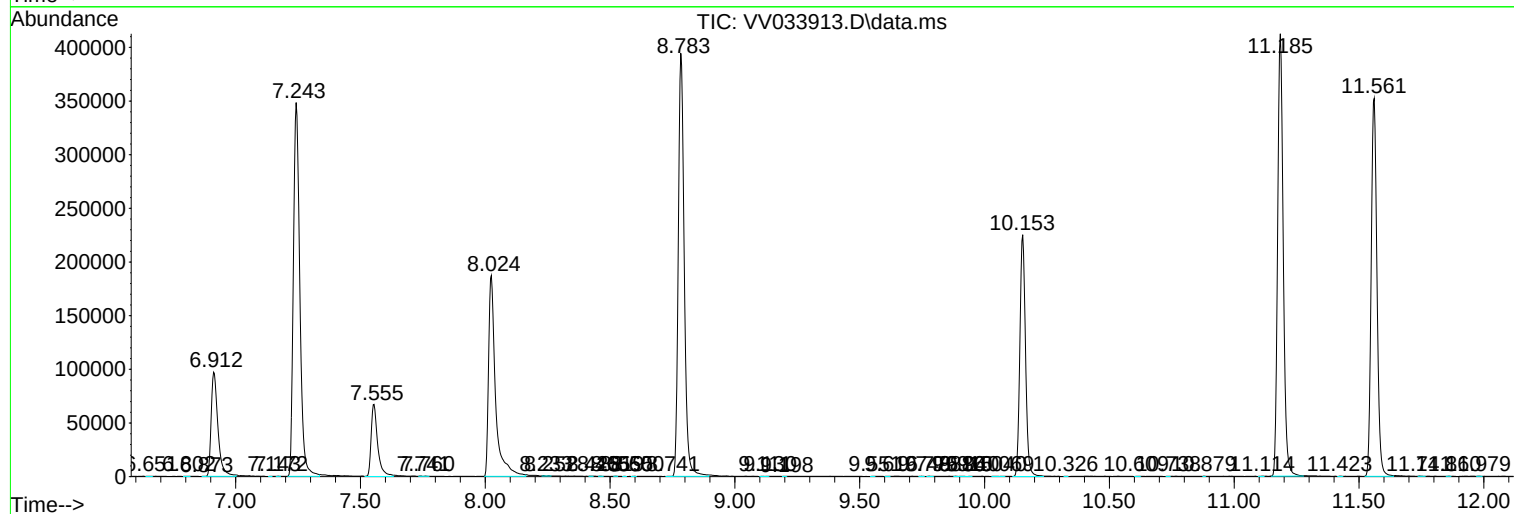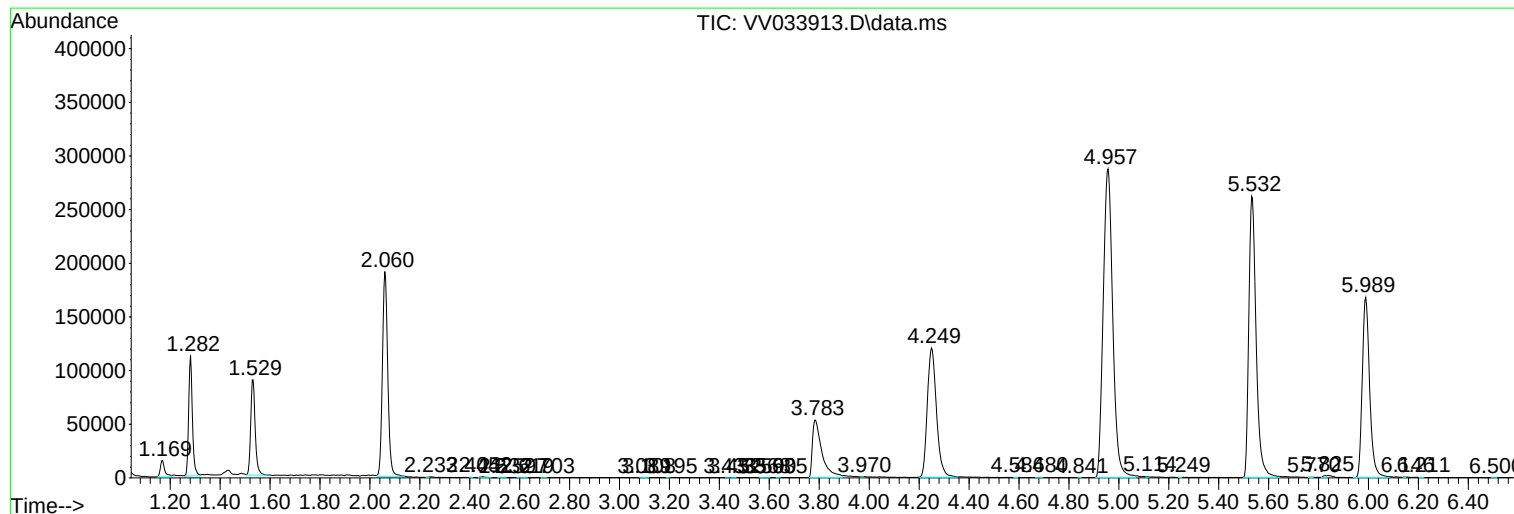

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033913.D
Acq On : 31 Jan 2024 10:12
Operator : SY/MD
Sample : VV0131MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033913.D
Acq On : 31 Jan 2024 10:12
Operator : SY/MD
Sample : VV0131MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------