

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033917.D
 Acq On : 31 Jan 2024 13:30
 Operator : SY/MD
 Sample : P1299-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	51	rBV	13061	15731	2.15%	0.264%
2	1.281	67	75	88	rBV	103185	110951	15.17%	1.864%
3	1.532	145	153	171	rVB	86061	104163	14.25%	1.750%
4	2.060	307	317	346	rVB	185364	278203	38.05%	4.674%
5	2.188	352	357	362	rVB2	437	526	0.07%	0.009%
6	2.413	425	427	432	rVB2	317	173	0.02%	0.003%
7	2.445	432	437	442	rBV2	542	533	0.07%	0.009%
8	2.503	452	455	457	rBV2	169	141	0.02%	0.002%
9	2.561	461	473	492	rBV	10191	21034	2.88%	0.353%
10	2.625	492	493	499	rVB3	334	260	0.04%	0.004%
11	2.725	521	524	527	rBV2	145	142	0.02%	0.002%
12	2.764	531	536	538	rBV2	186	170	0.02%	0.003%
13	2.960	595	597	600	rVB	312	192	0.03%	0.003%
14	2.982	600	604	608	rBV2	295	346	0.05%	0.006%
15	3.326	709	711	714	rVB	298	182	0.02%	0.003%
16	3.352	714	719	722	rBV2	351	418	0.06%	0.007%
17	3.461	748	753	755	rBV	214	218	0.03%	0.004%
18	3.506	765	767	772	rVB2	156	135	0.02%	0.002%
19	3.548	778	780	784	rBV2	130	138	0.02%	0.002%
20	3.629	802	805	808	rBV2	205	187	0.03%	0.003%
21	3.706	824	829	832	rBV2	281	334	0.05%	0.006%
22	3.786	845	854	894	rBV	46115	125871	17.22%	2.115%
23	4.249	982	998	1030	rBV	115881	295601	40.43%	4.966%
24	4.503	1071	1077	1079	rBV2	214	235	0.03%	0.004%
25	4.622	1111	1114	1118	rVB2	187	151	0.02%	0.003%
26	4.651	1118	1123	1125	rBV	285	246	0.03%	0.004%
27	4.957	1202	1218	1244	rBV2	277429	731151	100.00%	12.283%
28	5.256	1308	1311	1312	rBV2	393	224	0.03%	0.004%
29	5.362	1340	1344	1347	rBB	178	145	0.02%	0.002%
30	5.471	1371	1378	1380	rBV3	324	359	0.05%	0.006%
31	5.532	1385	1397	1428	rBV	263789	538753	73.69%	9.051%
32	5.834	1484	1491	1504	rVB3	2329	4265	0.58%	0.072%
33	5.989	1526	1539	1566	rBV	158827	329900	45.12%	5.542%
34	6.506	1688	1700	1718	rVV2	4784	11126	1.52%	0.187%
35	6.609	1729	1732	1735	rBV	135	141	0.02%	0.002%
36	6.657	1744	1747	1749	rBV	164	136	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013124\
 Data File : VW033917.D
 Acq On : 31 Jan 2024 13:30
 Operator : SY/MD
 Sample : P1299-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.802	1788	1792	1798	rBV2	229	321	0.04%	0.005%
38	6.847	1802	1806	1810	rBV	265	325	0.04%	0.005%
39	6.911	1816	1826	1858	rBV	90662	174581	23.88%	2.933%
40	7.243	1918	1929	1951	rBV	332461	584895	80.00%	9.826%
41	7.551	2016	2025	2054	rBV	62869	114666	15.68%	1.926%
42	7.873	2118	2125	2135	rVB2	550	986	0.13%	0.017%
43	7.973	2153	2156	2159	rBV	205	192	0.03%	0.003%
44	8.024	2162	2172	2214	rBV	163954	329086	45.01%	5.528%
45	8.442	2299	2302	2304	rBV2	308	200	0.03%	0.003%
46	8.497	2316	2319	2324	rBV2	180	213	0.03%	0.004%
47	8.558	2334	2338	2339	rBV2	159	142	0.02%	0.002%
48	8.693	2373	2380	2384	rBV2	234	361	0.05%	0.006%
49	8.783	2396	2408	2438	rBV	393949	649194	88.79%	10.906%
50	9.082	2498	2501	2503	rBV2	232	186	0.03%	0.003%
51	9.143	2516	2520	2523	rBV2	234	271	0.04%	0.005%
52	9.223	2542	2545	2551	rBV	211	298	0.04%	0.005%
53	9.378	2589	2593	2594	rBV2	178	153	0.02%	0.003%
54	9.841	2734	2737	2739	rBV	194	156	0.02%	0.003%
55	10.027	2792	2795	2798	rBV	141	144	0.02%	0.002%
56	10.153	2822	2834	2855	rBV	209785	330778	45.24%	5.557%
57	10.316	2881	2885	2886	rBV	380	307	0.04%	0.005%
58	10.326	2886	2888	2891	rVB2	479	361	0.05%	0.006%
59	10.468	2928	2932	2935	rBV	207	192	0.03%	0.003%
60	10.538	2951	2954	2958	rBV2	129	145	0.02%	0.002%
61	10.619	2976	2979	2982	rBV2	236	212	0.03%	0.004%
62	10.702	3002	3005	3008	rVB	221	172	0.02%	0.003%
63	11.001	3094	3098	3101	rVB2	240	195	0.03%	0.003%
64	11.027	3101	3106	3108	rBV2	246	248	0.03%	0.004%
65	11.185	3144	3155	3177	rBV	412956	636356	87.03%	10.690%
66	11.355	3204	3208	3212	rVB2	396	382	0.05%	0.006%
67	11.378	3212	3215	3219	rVB2	305	166	0.02%	0.003%
68	11.397	3219	3221	3224	rBV2	326	250	0.03%	0.004%
69	11.561	3258	3272	3297	rBV	347150	545303	74.58%	9.161%
70	11.718	3318	3321	3324	rVB	278	192	0.03%	0.003%
71	11.741	3324	3328	3332	rBV	318	286	0.04%	0.005%
72	11.757	3332	3333	3338	rVB2	215	156	0.02%	0.003%
73	11.828	3350	3355	3357	rBV	234	243	0.03%	0.004%
74	11.869	3364	3368	3372	rBV2	231	223	0.03%	0.004%
75	12.008	3407	3411	3413	rBV2	232	219	0.03%	0.004%
76	12.085	3431	3435	3438	rBV2	163	143	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033917.D
 Acq On : 31 Jan 2024 13:30
 Operator : SY/MD
 Sample : P1299-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.130	3446	3449	3452	rBV2	157	140	0.02%	0.002%
78	12.259	3486	3489	3495	rBV	151	189	0.03%	0.003%
79	12.307	3500	3504	3508	rBV2	230	286	0.04%	0.005%
80	12.423	3536	3540	3544	rBV2	175	138	0.02%	0.002%
81	12.590	3590	3592	3596	rVB2	201	165	0.02%	0.003%
82	12.638	3604	3607	3610	rBV2	179	161	0.02%	0.003%
83	12.821	3659	3664	3670	rBV2	266	391	0.05%	0.007%
84	12.898	3684	3688	3690	rBV	168	162	0.02%	0.003%
85	12.934	3694	3699	3703	rBV2	207	265	0.04%	0.004%
86	13.114	3752	3755	3759	rBV	237	222	0.03%	0.004%
87	13.297	3809	3812	3817	rVB2	256	267	0.04%	0.004%
88	13.326	3817	3821	3824	rBV	261	262	0.04%	0.004%
89	13.403	3842	3845	3849	rBV2	258	201	0.03%	0.003%
90	13.432	3849	3854	3857	rBV2	299	308	0.04%	0.005%
91	13.455	3857	3861	3863	rBV2	353	325	0.04%	0.005%
92	13.516	3878	3880	3884	rVB3	232	151	0.02%	0.003%
93	13.693	3930	3935	3940	rBV2	1419	1676	0.23%	0.028%
94	13.869	3987	3990	3997	rBV2	169	195	0.03%	0.003%
95	13.982	4022	4025	4030	rBV4	430	409	0.06%	0.007%
96	14.037	4037	4042	4045	rBV3	387	325	0.04%	0.005%
97	14.114	4063	4066	4070	rVB2	237	191	0.03%	0.003%
98	14.721	4250	4255	4258	rBV3	277	279	0.04%	0.005%
99	14.934	4318	4321	4324	rBV3	329	312	0.04%	0.005%
100	15.638	4537	4540	4541	rBV3	371	229	0.03%	0.004%




Sum of corrected areas: 5952629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033917.D
Acq On : 31 Jan 2024 13:30
Operator : SY/MD
Sample : P1299-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

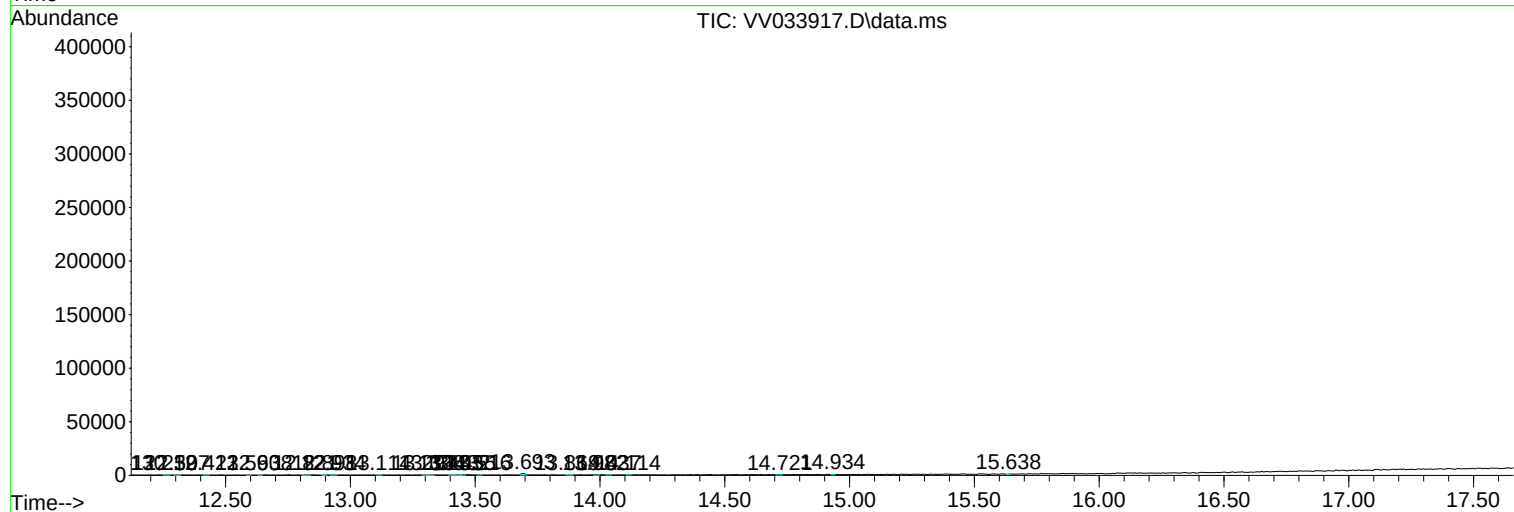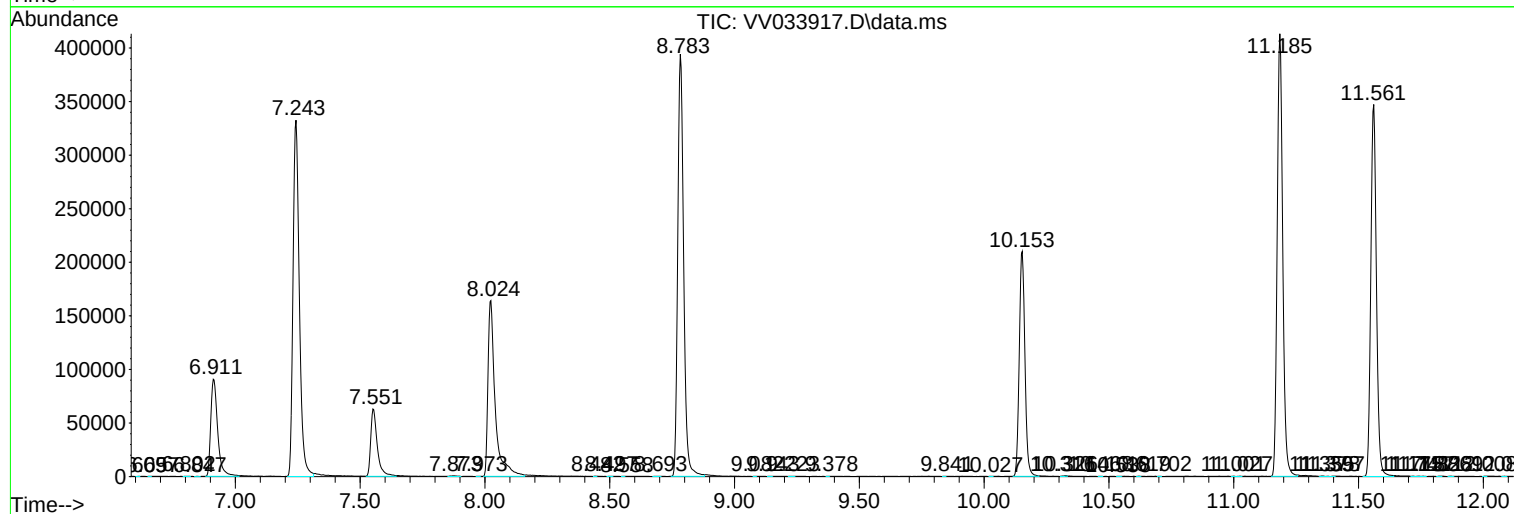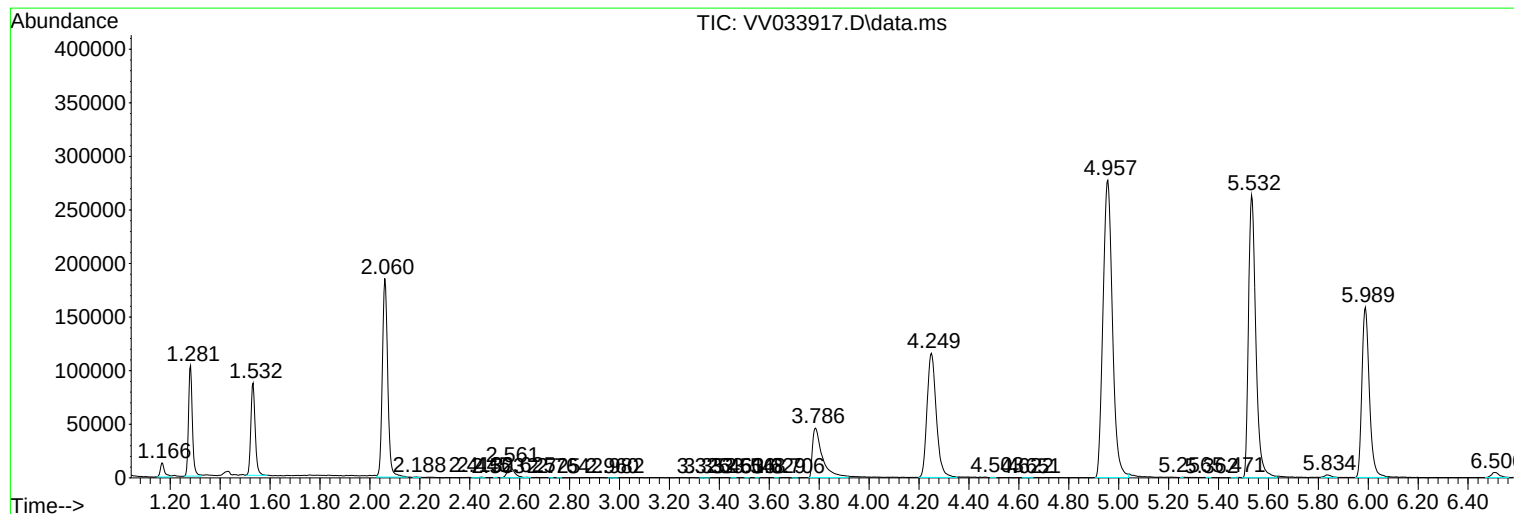

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033917.D
Acq On : 31 Jan 2024 13:30
Operator : SY/MD
Sample : P1299-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033917.D
Acq On : 31 Jan 2024 13:30
Operator : SY/MD
Sample : P1299-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
