

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033918.D
 Acq On : 31 Jan 2024 13:54
 Operator : SY/MD
 Sample : P1299-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Z6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	45	rBV	13793	14994	2.10%	0.260%
2	1.281	68	75	90	rBV	97021	105594	14.80%	1.834%
3	1.532	145	153	167	rVB	82637	99869	14.00%	1.735%
4	2.059	307	317	337	rBV	176141	257684	36.12%	4.476%
5	2.249	367	376	383	rVB4	1014	1858	0.26%	0.032%
6	2.288	383	388	391	rBV	195	200	0.03%	0.003%
7	2.448	431	438	443	rBV2	352	546	0.08%	0.009%
8	2.584	477	480	483	rVB2	176	147	0.02%	0.003%
9	2.606	483	487	490	rVB	226	174	0.02%	0.003%
10	2.703	512	517	520	rBV	198	211	0.03%	0.004%
11	2.825	550	555	559	rBV2	268	324	0.05%	0.006%
12	3.272	691	694	697	rBV2	293	284	0.04%	0.005%
13	3.375	723	726	729	rVB2	189	155	0.02%	0.003%
14	3.532	772	775	779	rVB2	184	152	0.02%	0.003%
15	3.635	803	807	810	rBV	285	263	0.04%	0.005%
16	3.664	813	816	819	rVB	185	148	0.02%	0.003%
17	3.683	819	822	828	rBV	243	288	0.04%	0.005%
18	3.783	845	853	887	rBV	47248	125386	17.57%	2.178%
19	4.249	982	998	1027	rBV	110756	285297	39.99%	4.956%
20	4.442	1054	1058	1061	rBV3	294	258	0.04%	0.004%
21	4.519	1080	1082	1085	rBV2	254	200	0.03%	0.003%
22	4.574	1095	1099	1104	rBV2	408	442	0.06%	0.008%
23	4.686	1131	1134	1136	rBV2	233	157	0.02%	0.003%
24	4.728	1141	1147	1150	rBV2	215	289	0.04%	0.005%
25	4.809	1170	1172	1175	rBV	244	156	0.02%	0.003%
26	4.956	1202	1218	1256	rBV2	270573	713438	100.00%	12.392%
27	5.175	1284	1286	1288	rBV2	219	150	0.02%	0.003%
28	5.464	1369	1376	1379	rBV3	319	410	0.06%	0.007%
29	5.532	1386	1397	1424	rBV	254115	521200	73.05%	9.053%
30	5.831	1483	1490	1503	rVB5	1891	3956	0.55%	0.069%
31	5.989	1525	1539	1567	rBV	156755	323877	45.40%	5.626%
32	6.143	1585	1587	1591	rVV3	329	227	0.03%	0.004%
33	6.210	1606	1608	1612	rVV2	246	144	0.02%	0.003%
34	6.297	1631	1635	1640	rBV2	294	282	0.04%	0.005%
35	6.509	1698	1701	1705	rBV2	221	183	0.03%	0.003%
36	6.548	1711	1713	1718	rVB	175	148	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013124\
 Data File : VW033918.D
 Acq On : 31 Jan 2024 13:54
 Operator : SY/MD
 Sample : P1299-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Z6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.577	1718	1722	1724	rBV	271	197	0.03%	0.003%
38	6.657	1742	1747	1754	rBV	180	304	0.04%	0.005%
39	6.722	1762	1767	1769	rBV	171	159	0.02%	0.003%
40	6.911	1816	1826	1853	rBV	91182	168811	23.66%	2.932%
41	7.156	1901	1902	1910	rVB4	353	243	0.03%	0.004%
42	7.243	1917	1929	1966	rBV	321371	571087	80.05%	9.920%
43	7.554	2017	2026	2051	rBV	61027	110670	15.51%	1.922%
44	7.802	2100	2103	2108	rBV3	187	146	0.02%	0.003%
45	7.870	2121	2124	2126	rBV2	171	150	0.02%	0.003%
46	7.943	2144	2147	2151	rBV	241	237	0.03%	0.004%
47	8.024	2163	2172	2216	rBV	165034	325138	45.57%	5.648%
48	8.468	2303	2310	2312	rBV3	261	278	0.04%	0.005%
49	8.516	2323	2325	2330	rBV2	341	314	0.04%	0.005%
50	8.619	2353	2357	2360	rBV2	222	228	0.03%	0.004%
51	8.783	2397	2408	2441	rBV	381815	632569	88.66%	10.988%
52	9.230	2541	2547	2552	rBV2	232	384	0.05%	0.007%
53	9.506	2627	2633	2636	rBV2	234	265	0.04%	0.005%
54	9.789	2715	2721	2724	rBV2	240	265	0.04%	0.005%
55	10.014	2786	2791	2794	rBV2	216	231	0.03%	0.004%
56	10.101	2814	2818	2820	rBV	170	151	0.02%	0.003%
57	10.152	2823	2834	2856	rVV	207988	327514	45.91%	5.689%
58	10.416	2913	2916	2919	rBV2	176	166	0.02%	0.003%
59	10.596	2969	2972	2975	rBV2	178	178	0.02%	0.003%
60	10.693	3000	3002	3010	rBV2	168	273	0.04%	0.005%
61	10.950	3078	3082	3091	rBV2	275	483	0.07%	0.008%
62	11.184	3144	3155	3184	rBV	403839	622901	87.31%	10.820%
63	11.561	3260	3272	3300	rBV	328725	524495	73.52%	9.110%
64	11.831	3352	3356	3358	rBV2	228	187	0.03%	0.003%
65	11.988	3400	3405	3408	rBV	254	257	0.04%	0.004%
66	12.072	3428	3431	3434	rBV2	174	176	0.02%	0.003%
67	12.168	3458	3461	3466	rVB2	198	235	0.03%	0.004%
68	12.197	3466	3470	3473	rBV2	258	255	0.04%	0.004%
69	12.300	3497	3502	3513	rBV4	1129	1707	0.24%	0.030%
70	12.368	3520	3523	3528	rVB2	236	190	0.03%	0.003%
71	12.567	3582	3585	3588	rBV	183	162	0.02%	0.003%
72	12.686	3620	3622	3627	rVB2	221	177	0.02%	0.003%
73	12.718	3627	3632	3635	rBV2	197	256	0.04%	0.004%
74	12.770	3644	3648	3650	rBV	217	159	0.02%	0.003%
75	13.004	3719	3721	3727	rBV2	225	191	0.03%	0.003%
76	13.358	3826	3831	3832	rBV	193	158	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033918.D
 Acq On : 31 Jan 2024 13:54
 Operator : SY/MD
 Sample : P1299-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Z6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	13.493	3868	3873	3881	rVB2	297	446	0.06%	0.008%
78	13.532	3882	3885	3890	rBV2	186	172	0.02%	0.003%
79	13.567	3890	3896	3900	rBV2	209	237	0.03%	0.004%
80	13.593	3901	3904	3907	rBV	289	237	0.03%	0.004%
81	13.644	3917	3920	3924	rVB2	225	164	0.02%	0.003%
82	13.670	3924	3928	3931	rBV2	277	256	0.04%	0.004%
83	13.696	3932	3936	3940	rVB2	249	192	0.03%	0.003%
84	13.744	3948	3951	3955	rBV3	326	307	0.04%	0.005%
85	13.766	3955	3958	3962	rVB3	241	189	0.03%	0.003%
86	13.876	3987	3992	3996	rBV3	236	262	0.04%	0.005%
87	13.982	4021	4025	4027	rVB3	325	245	0.03%	0.004%
88	14.027	4036	4039	4043	rBV2	286	230	0.03%	0.004%
89	14.159	4076	4080	4085	rVB3	379	379	0.05%	0.007%
90	14.188	4085	4089	4091	rBV2	292	223	0.03%	0.004%
91	14.297	4121	4123	4125	rBV	301	147	0.02%	0.003%
92	14.557	4201	4204	4211	rBV3	325	270	0.04%	0.005%
93	14.840	4291	4292	4297	rBV3	212	160	0.02%	0.003%
94	14.892	4306	4308	4311	rBV2	349	178	0.02%	0.003%
95	14.924	4315	4318	4321	rVB2	468	294	0.04%	0.005%
96	15.040	4351	4354	4355	rBV2	294	171	0.02%	0.003%
97	15.126	4378	4381	4385	rBV4	650	561	0.08%	0.010%
98	15.216	4407	4409	4412	rBV	293	143	0.02%	0.002%
99	15.297	4432	4434	4436	rBV2	393	200	0.03%	0.003%
100	15.371	4455	4457	4461	rVB2	655	341	0.05%	0.006%

Sum of corrected areas: 5757042




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV03124\
Data File : VV033918.D
Acq On : 31 Jan 2024 13:54
Operator : SY/MD
Sample : P1299-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Z6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

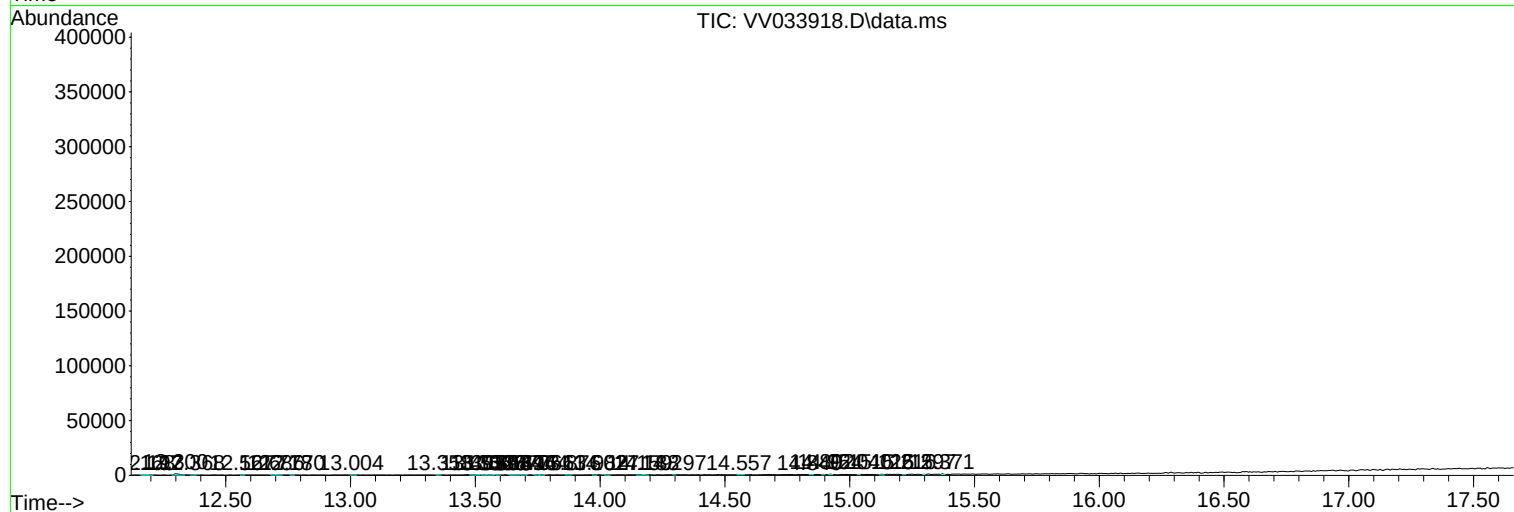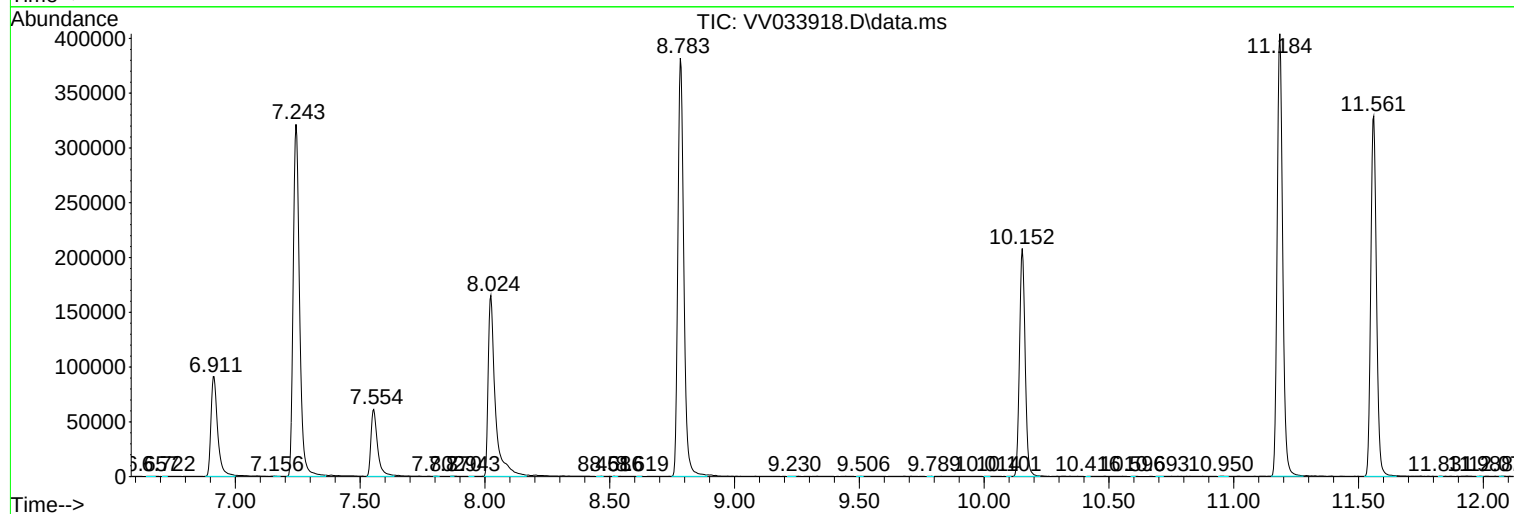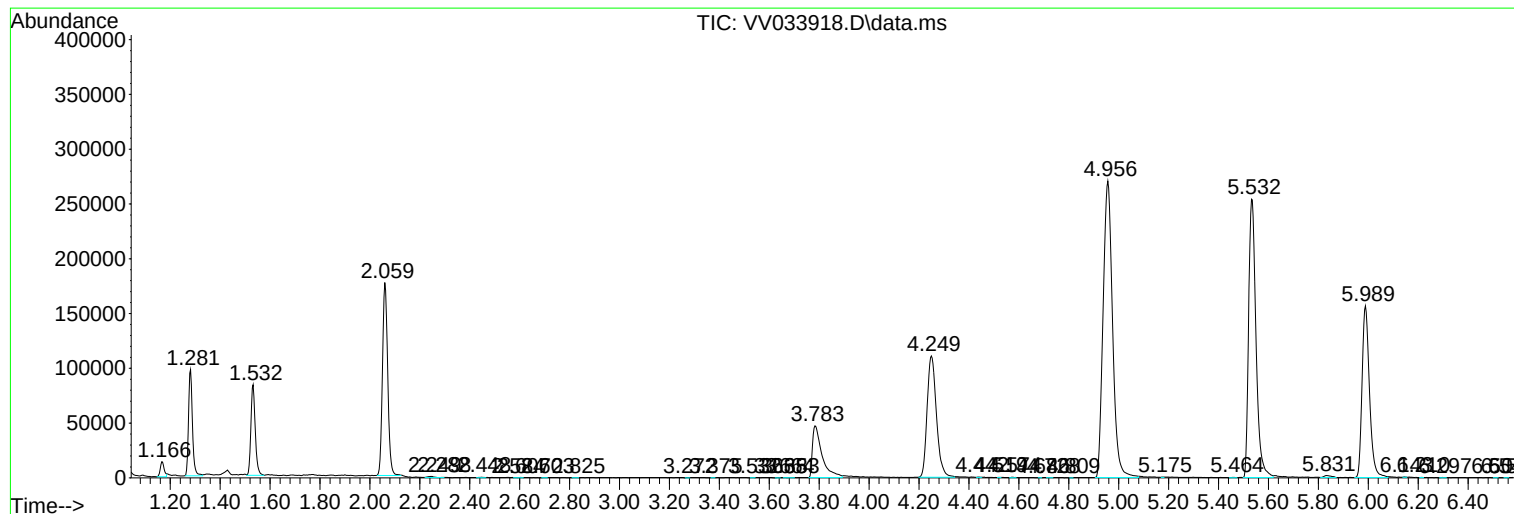

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033918.D
Acq On : 31 Jan 2024 13:54
Operator : SY/MD
Sample : P1299-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Z6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033918.D
Acq On : 31 Jan 2024 13:54
Operator : SY/MD
Sample : P1299-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Z6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------