

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033919.D
 Acq On : 31 Jan 2024 14:18
 Operator : SY/MD
 Sample : P1299-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	46	rBV	13840	15653	2.17%	0.277%
2	1.282	68	75	90	rBV	99360	106559	14.76%	1.887%
3	1.532	145	153	167	rVB	85042	101146	14.01%	1.791%
4	2.060	307	317	344	rVB	180692	271836	37.64%	4.814%
5	2.182	353	355	359	rVB2	491	346	0.05%	0.006%
6	2.243	369	374	384	rVB2	2056	2707	0.37%	0.048%
7	2.352	405	408	411	rVB	243	144	0.02%	0.003%
8	2.381	411	417	418	rBV	214	246	0.03%	0.004%
9	2.452	436	439	443	rVB2	336	238	0.03%	0.004%
10	2.526	458	462	467	rBV	246	299	0.04%	0.005%
11	2.690	510	513	517	rBV	122	141	0.02%	0.002%
12	2.966	595	599	602	rVB2	162	139	0.02%	0.002%
13	2.989	603	606	610	rVB	200	128	0.02%	0.002%
14	3.015	610	614	617	rVB2	157	160	0.02%	0.003%
15	3.156	654	658	660	rVB	171	138	0.02%	0.002%
16	3.185	664	667	670	rVB2	307	232	0.03%	0.004%
17	3.208	670	674	676	rBV2	256	201	0.03%	0.004%
18	3.230	676	681	686	rVB2	255	271	0.04%	0.005%
19	3.256	686	689	695	rBV	234	240	0.03%	0.004%
20	3.330	707	712	715	rBV2	132	158	0.02%	0.003%
21	3.465	751	754	757	rVB2	251	207	0.03%	0.004%
22	3.497	757	764	773	rBV2	314	830	0.11%	0.015%
23	3.642	805	809	812	rBV	335	315	0.04%	0.006%
24	3.661	812	815	817	rBV	169	136	0.02%	0.002%
25	3.735	835	838	841	rBV	159	138	0.02%	0.002%
26	3.783	845	853	892	rBV	47405	127697	17.68%	2.262%
27	4.249	982	998	1027	rBV	111924	287725	39.84%	5.096%
28	4.471	1063	1067	1071	rBV	326	302	0.04%	0.005%
29	4.497	1071	1075	1077	rBV	150	162	0.02%	0.003%
30	4.558	1090	1094	1098	rBV2	289	347	0.05%	0.006%
31	4.706	1136	1140	1142	rBV	178	157	0.02%	0.003%
32	4.793	1160	1167	1170	rBV2	189	271	0.04%	0.005%
33	4.828	1175	1178	1181	rBV2	184	161	0.02%	0.003%
34	4.957	1201	1218	1248	rBV2	273179	722161	100.00%	12.789%
35	5.137	1272	1274	1281	rVB2	539	448	0.06%	0.008%
36	5.326	1328	1333	1336	rBV2	228	229	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033919.D
 Acq On : 31 Jan 2024 14:18
 Operator : SY/MD
 Sample : P1299-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.532	1385	1397	1422	rBV	231314	470477	65.15%	8.332%
38	5.738	1458	1461	1464	rBV	267	241	0.03%	0.004%
39	5.834	1484	1491	1500	rBV5	1805	3534	0.49%	0.063%
40	5.989	1526	1539	1570	rBV	155856	325331	45.05%	5.762%
41	6.179	1595	1598	1600	rBV	170	126	0.02%	0.002%
42	6.278	1623	1629	1632	rBV2	186	270	0.04%	0.005%
43	6.349	1647	1651	1654	rBV	164	163	0.02%	0.003%
44	6.407	1665	1669	1672	rBV2	163	161	0.02%	0.003%
45	6.545	1705	1712	1714	rBV2	160	217	0.03%	0.004%
46	6.584	1721	1724	1727	rBV	205	179	0.02%	0.003%
47	6.764	1774	1780	1785	rBV2	191	319	0.04%	0.006%
48	6.912	1816	1826	1862	rBV	91672	173959	24.09%	3.081%
49	7.243	1917	1929	1955	rBV	327523	577524	79.97%	10.228%
50	7.555	2016	2026	2045	rBV	62688	111910	15.50%	1.982%
51	7.751	2083	2087	2090	rBV2	253	181	0.03%	0.003%
52	7.780	2092	2096	2099	rBV3	178	129	0.02%	0.002%
53	7.950	2144	2149	2152	rBV2	181	187	0.03%	0.003%
54	8.024	2163	2172	2212	rBV	165108	328307	45.46%	5.814%
55	8.449	2299	2304	2307	rVB3	312	318	0.04%	0.006%
56	8.783	2397	2408	2445	rBV	347167	576022	79.76%	10.201%
57	9.059	2491	2494	2499	rVB2	173	144	0.02%	0.003%
58	9.233	2543	2548	2549	rBV	150	161	0.02%	0.003%
59	9.670	2681	2684	2686	rBV	175	151	0.02%	0.003%
60	9.754	2705	2710	2711	rBV2	184	172	0.02%	0.003%
61	9.821	2727	2731	2734	rBV2	193	211	0.03%	0.004%
62	10.104	2816	2819	2822	rBV2	145	133	0.02%	0.002%
63	10.153	2822	2834	2856	rVV	208250	331042	45.84%	5.863%
64	10.317	2878	2885	2888	rBV2	287	382	0.05%	0.007%
65	10.448	2921	2926	2931	rBV2	166	218	0.03%	0.004%
66	10.529	2946	2951	2954	rBV2	186	201	0.03%	0.004%
67	10.973	3085	3089	3091	rBV	198	166	0.02%	0.003%
68	11.114	3126	3133	3137	rVB3	475	568	0.08%	0.010%
69	11.185	3144	3155	3179	rBV	362357	562583	77.90%	9.963%
70	11.358	3207	3209	3212	rVB3	336	165	0.02%	0.003%
71	11.561	3260	3272	3295	rBV	334239	528044	73.12%	9.352%
72	11.870	3364	3368	3370	rBV2	261	154	0.02%	0.003%
73	11.905	3376	3379	3386	rBV2	207	324	0.04%	0.006%
74	12.050	3418	3424	3426	rBV2	184	190	0.03%	0.003%
75	12.162	3456	3459	3462	rVB	181	129	0.02%	0.002%
76	12.223	3474	3478	3480	rBV2	139	129	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033919.D
 Acq On : 31 Jan 2024 14:18
 Operator : SY/MD
 Sample : P1299-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.300	3495	3502	3513	rVV6	2527	3822	0.53%	0.068%
78	12.545	3570	3578	3582	rBV	222	312	0.04%	0.006%
79	12.625	3600	3603	3609	rVV2	236	237	0.03%	0.004%
80	12.767	3644	3647	3650	rBV	217	196	0.03%	0.003%
81	12.808	3657	3660	3663	rBV2	171	180	0.02%	0.003%
82	13.075	3741	3743	3747	rBV2	157	145	0.02%	0.003%
83	13.127	3754	3759	3761	rBV2	198	224	0.03%	0.004%
84	13.165	3768	3771	3777	rBV2	248	291	0.04%	0.005%
85	13.243	3792	3795	3799	rBV	164	155	0.02%	0.003%
86	13.362	3824	3832	3835	rBV2	253	340	0.05%	0.006%
87	13.384	3835	3839	3842	rBV2	208	192	0.03%	0.003%
88	13.455	3859	3861	3865	rBV2	317	218	0.03%	0.004%
89	13.551	3886	3891	3893	rBV	228	250	0.03%	0.004%
90	13.606	3904	3908	3911	rBV2	217	174	0.02%	0.003%
91	13.988	4021	4027	4033	rVB3	418	657	0.09%	0.012%
92	14.104	4060	4063	4064	rBV	249	149	0.02%	0.003%
93	14.185	4085	4088	4090	rBV2	228	130	0.02%	0.002%
94	14.294	4120	4122	4129	rBV2	261	233	0.03%	0.004%
95	14.323	4129	4131	4135	rVB2	315	228	0.03%	0.004%
96	14.345	4135	4138	4145	rBV3	212	222	0.03%	0.004%
97	14.509	4181	4189	4192	rBV3	258	366	0.05%	0.006%
98	15.050	4355	4357	4359	rVV2	341	161	0.02%	0.003%
99	15.075	4363	4365	4369	rBV	318	199	0.03%	0.004%
100	15.567	4516	4518	4524	rBV4	366	388	0.05%	0.007%




Sum of corrected areas: 5646559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033919.D
Acq On : 31 Jan 2024 14:18
Operator : SY/MD
Sample : P1299-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

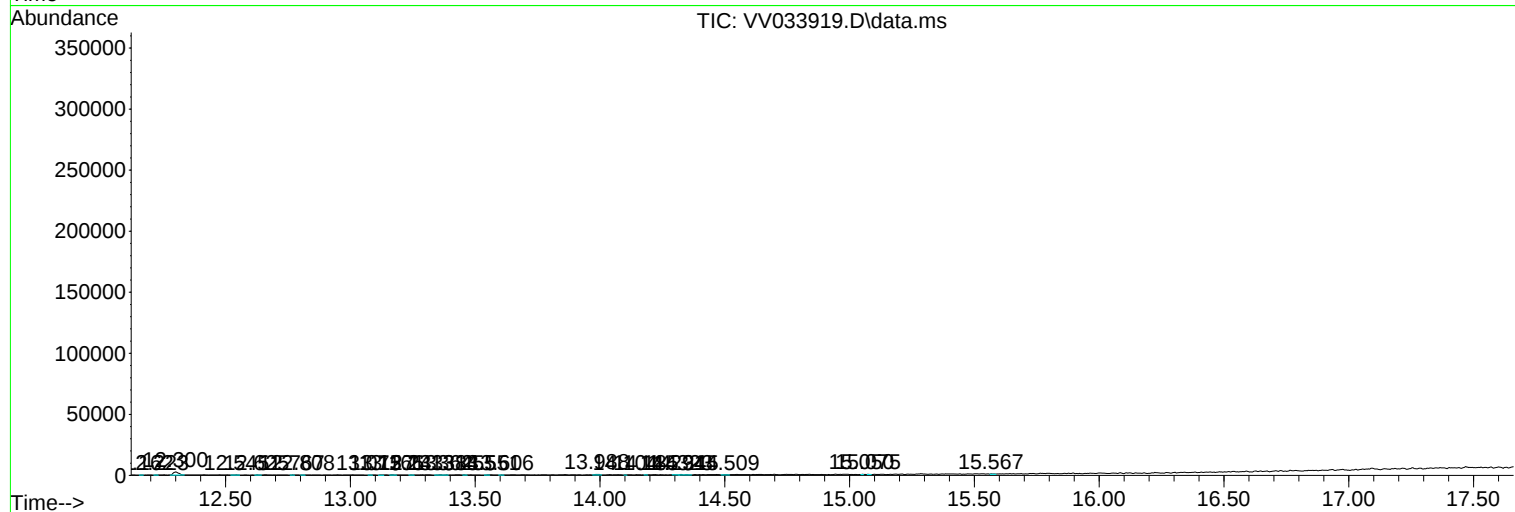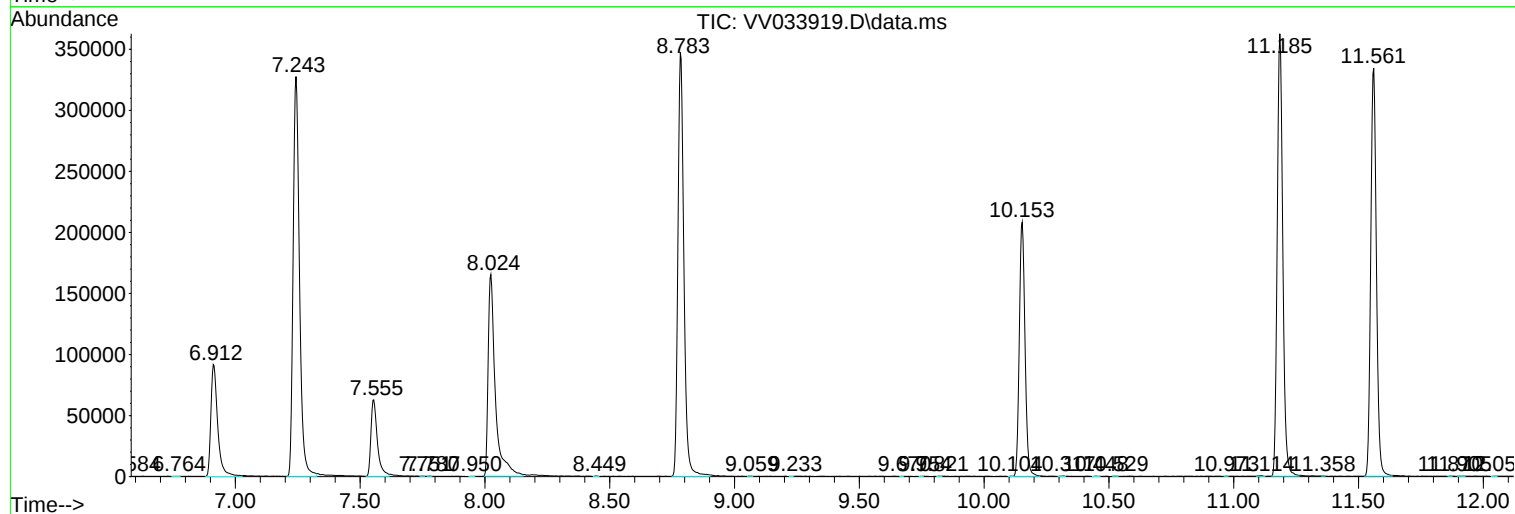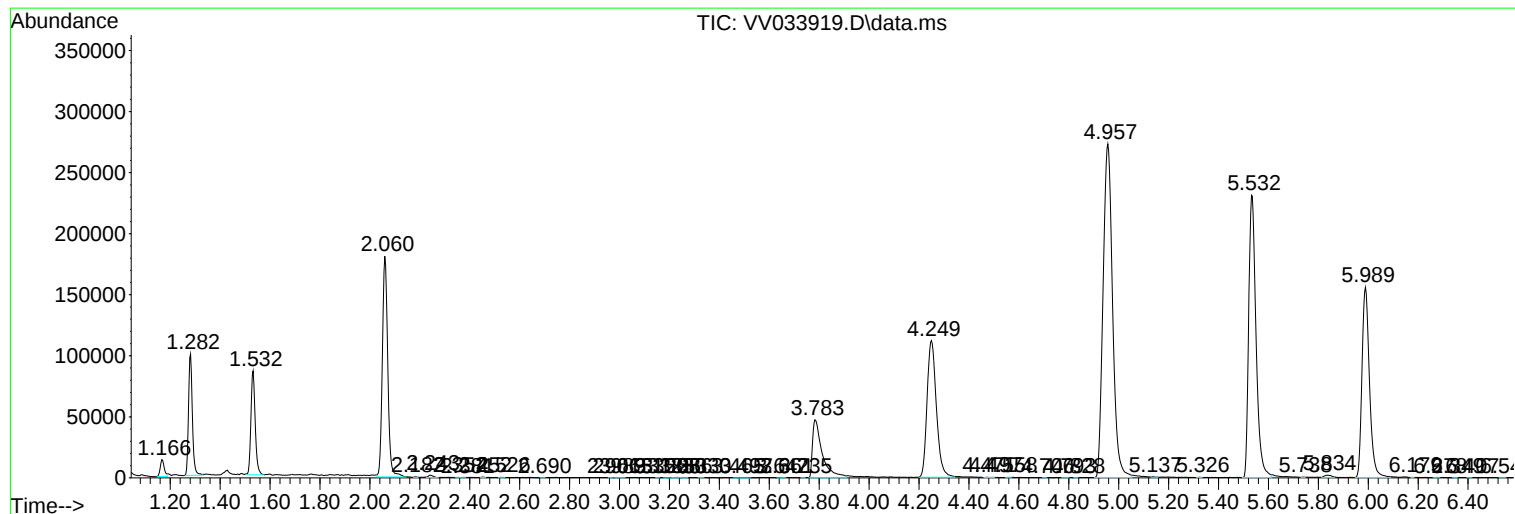

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033919.D
Acq On : 31 Jan 2024 14:18
Operator : SY/MD
Sample : P1299-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033919.D
Acq On : 31 Jan 2024 14:18
Operator : SY/MD
Sample : P1299-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------